

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
 Data File : VW026473.D
 Acq On : 30 Jun 2023 15:29
 Operator : SY/MD
 Sample : 03478-06
 Misc : 5.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW65

Quant Time: Jun 30 23:42:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 23:38:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	982957	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	824950	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	362549	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	221247	19.768	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.080%
7) Chloroethane-d5	2.893	69	183699	20.157	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.640%
11) 1,1-Dichloroethene-d2	4.021	65	119821	21.397	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.600%
21) 2-Butanone-d5	7.075	46	184592	43.642	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.280%
24) Chloroform-d	7.648	84	525524	21.934	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.720%
26) 1,2-Dichloroethane-d4	8.307	65	296229	22.620	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.480%
32) Benzene-d6	8.276	84	1127724	23.505	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.040%
36) 1,2-Dichloropropane-d6	9.270	67	364496	23.837	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.360%
41) Toluene-d8	10.325	98	961014	22.676	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.720%
43) trans-1,3-Dichloroprop...	10.575	79	136736	22.184	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.720%
47) 2-Hexanone-d5	10.922	63	118687	46.412	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.820%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	285353	24.168	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	281641	22.310	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.240%
Target Compounds					Qvalue	
13) Acetone	4.119	43	20510	6.864	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
Data File : VW026473.D
Acq On : 30 Jun 2023 15:29
Operator : SY/MD
Sample : 03478-06
Misc : 5.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YBW65

Quant Time: Jun 30 23:42:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 30 23:38:58 2023
Response via : Initial Calibration

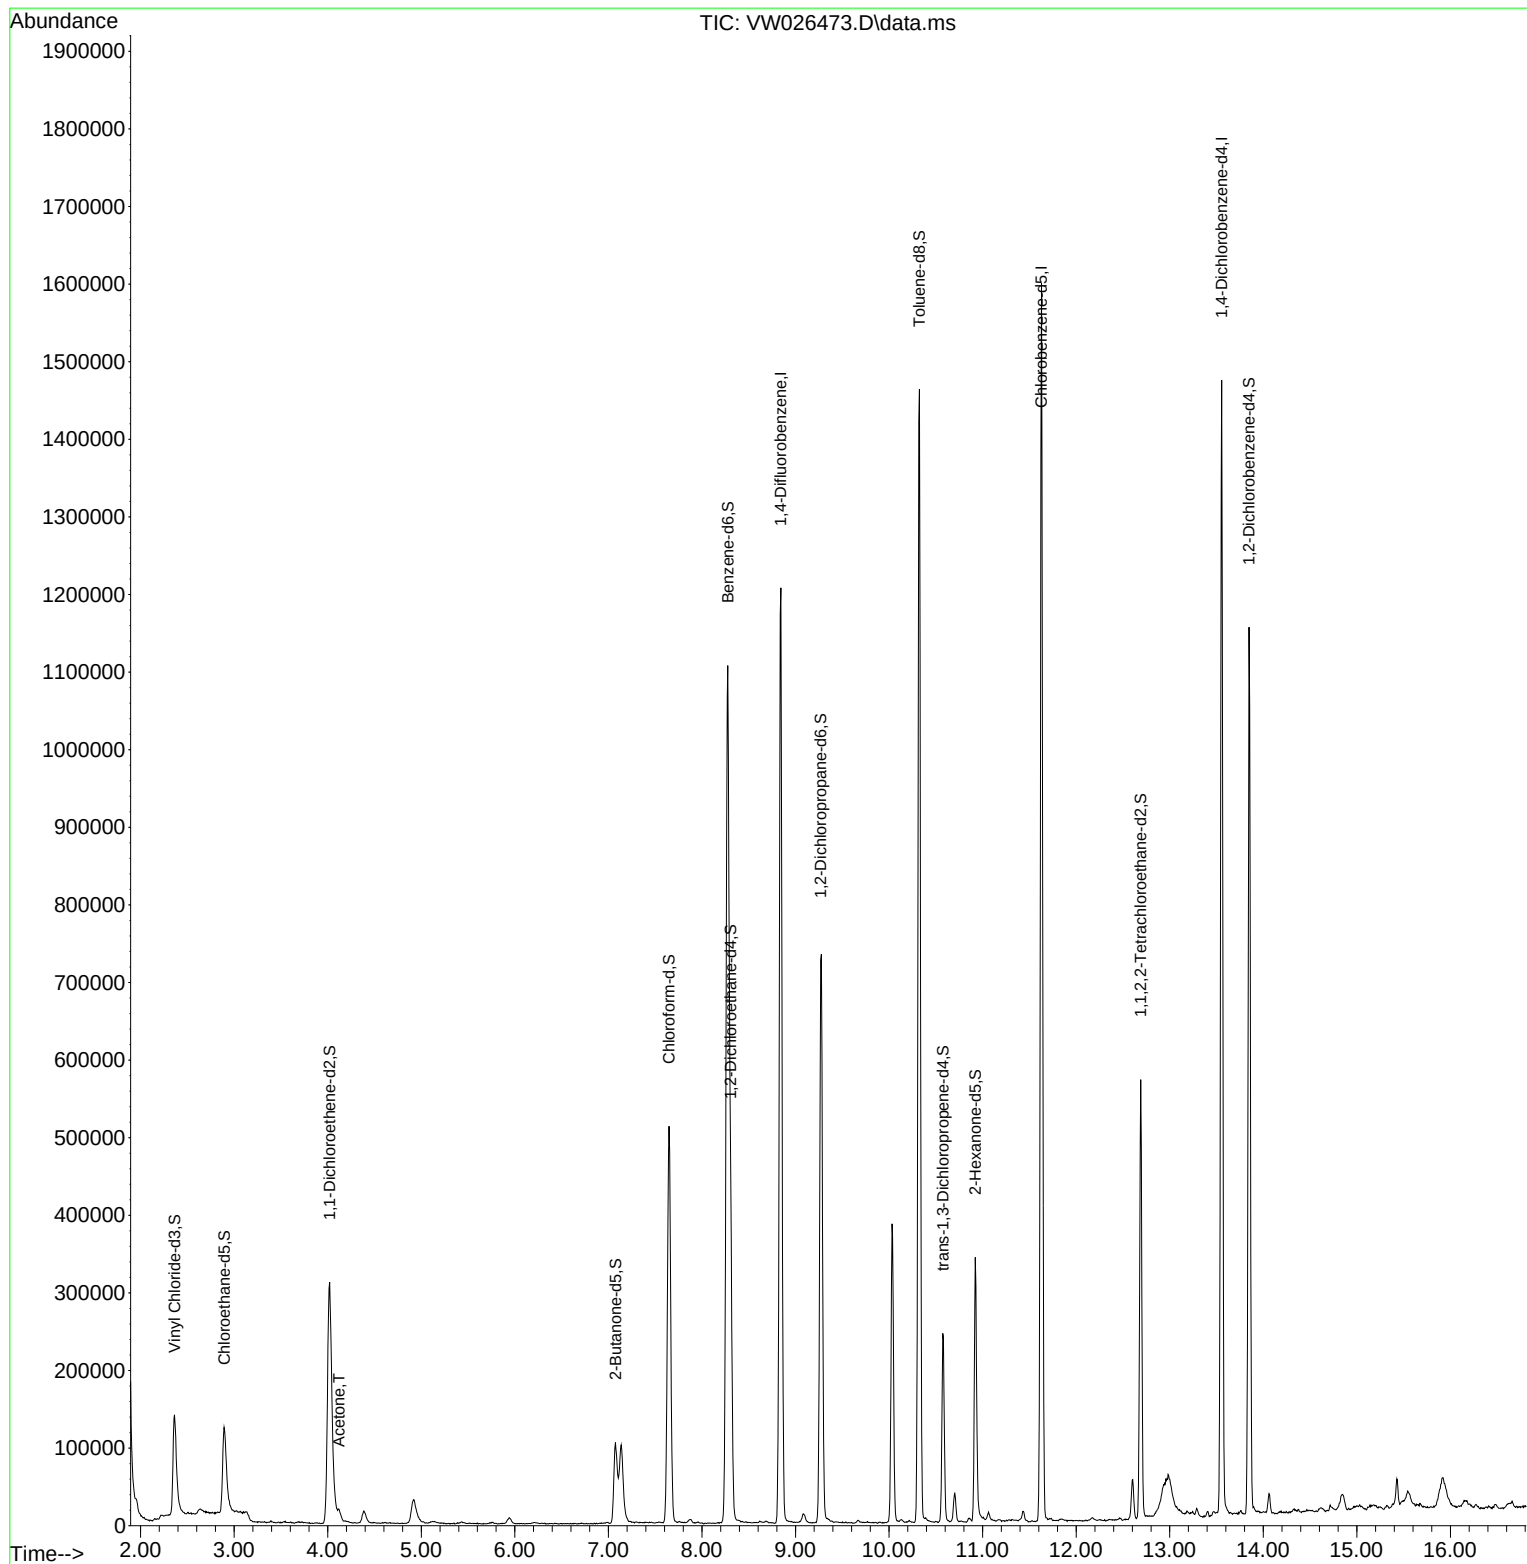

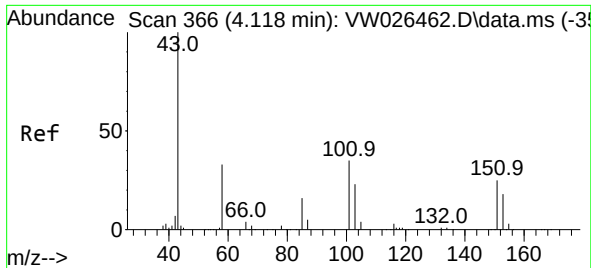

#13
 Acetone
 Concen: 6.864 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW026473.D
 Acq: 30 Jun 2023 15:29

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW65

Tgt Ion: 43 Resp: 20510
 Ion Ratio Lower Upper
 43 100
 58 30.7 0.0 63.2

