

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
 Data File : VW023554.D
 Acq On : 01 Jul 2022 11:44
 Operator : SY/VA
 Sample : VW0701SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK536

Quant Time: Jul 04 01:22:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 04 01:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	318174	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	298669	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	138433	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	155218	34.105	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	136.400%
7) Chloroethane-d5	2.879	69	73052	23.307	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.240%
11) 1,1-Dichloroethene-d2	4.013	63	112302	19.943	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.760%
21) 2-Butanone-d5	7.080	46	57723	50.639	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.280%
24) Chloroform-d	7.646	84	206963	23.828	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.320%
26) 1,2-Dichloroethane-d4	8.305	65	118230	24.650	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.600%
32) Benzene-d6	8.274	84	409884	25.383	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.520%
36) 1,2-Dichloropropane-d6	9.274	67	118426	24.805	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.240%
41) Toluene-d8	10.323	98	386293	24.596	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.400%
43) trans-1,3-Dichloroprop...	10.579	79	50251	23.759	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.040%
47) 2-Hexanone-d5	10.926	63	44061	48.653	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.300%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	106736	23.285	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	125567	24.871	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.480%
Target Compounds						Qvalue
9) Trichlorofluoromethane	3.050	101	148	0.062	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
Data File : VW023554.D
Acq On : 01 Jul 2022 11:44
Operator : SY/VA
Sample : VW0701SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK536

Quant Time: Jul 04 01:22:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 04 01:19:17 2022
Response via : Initial Calibration

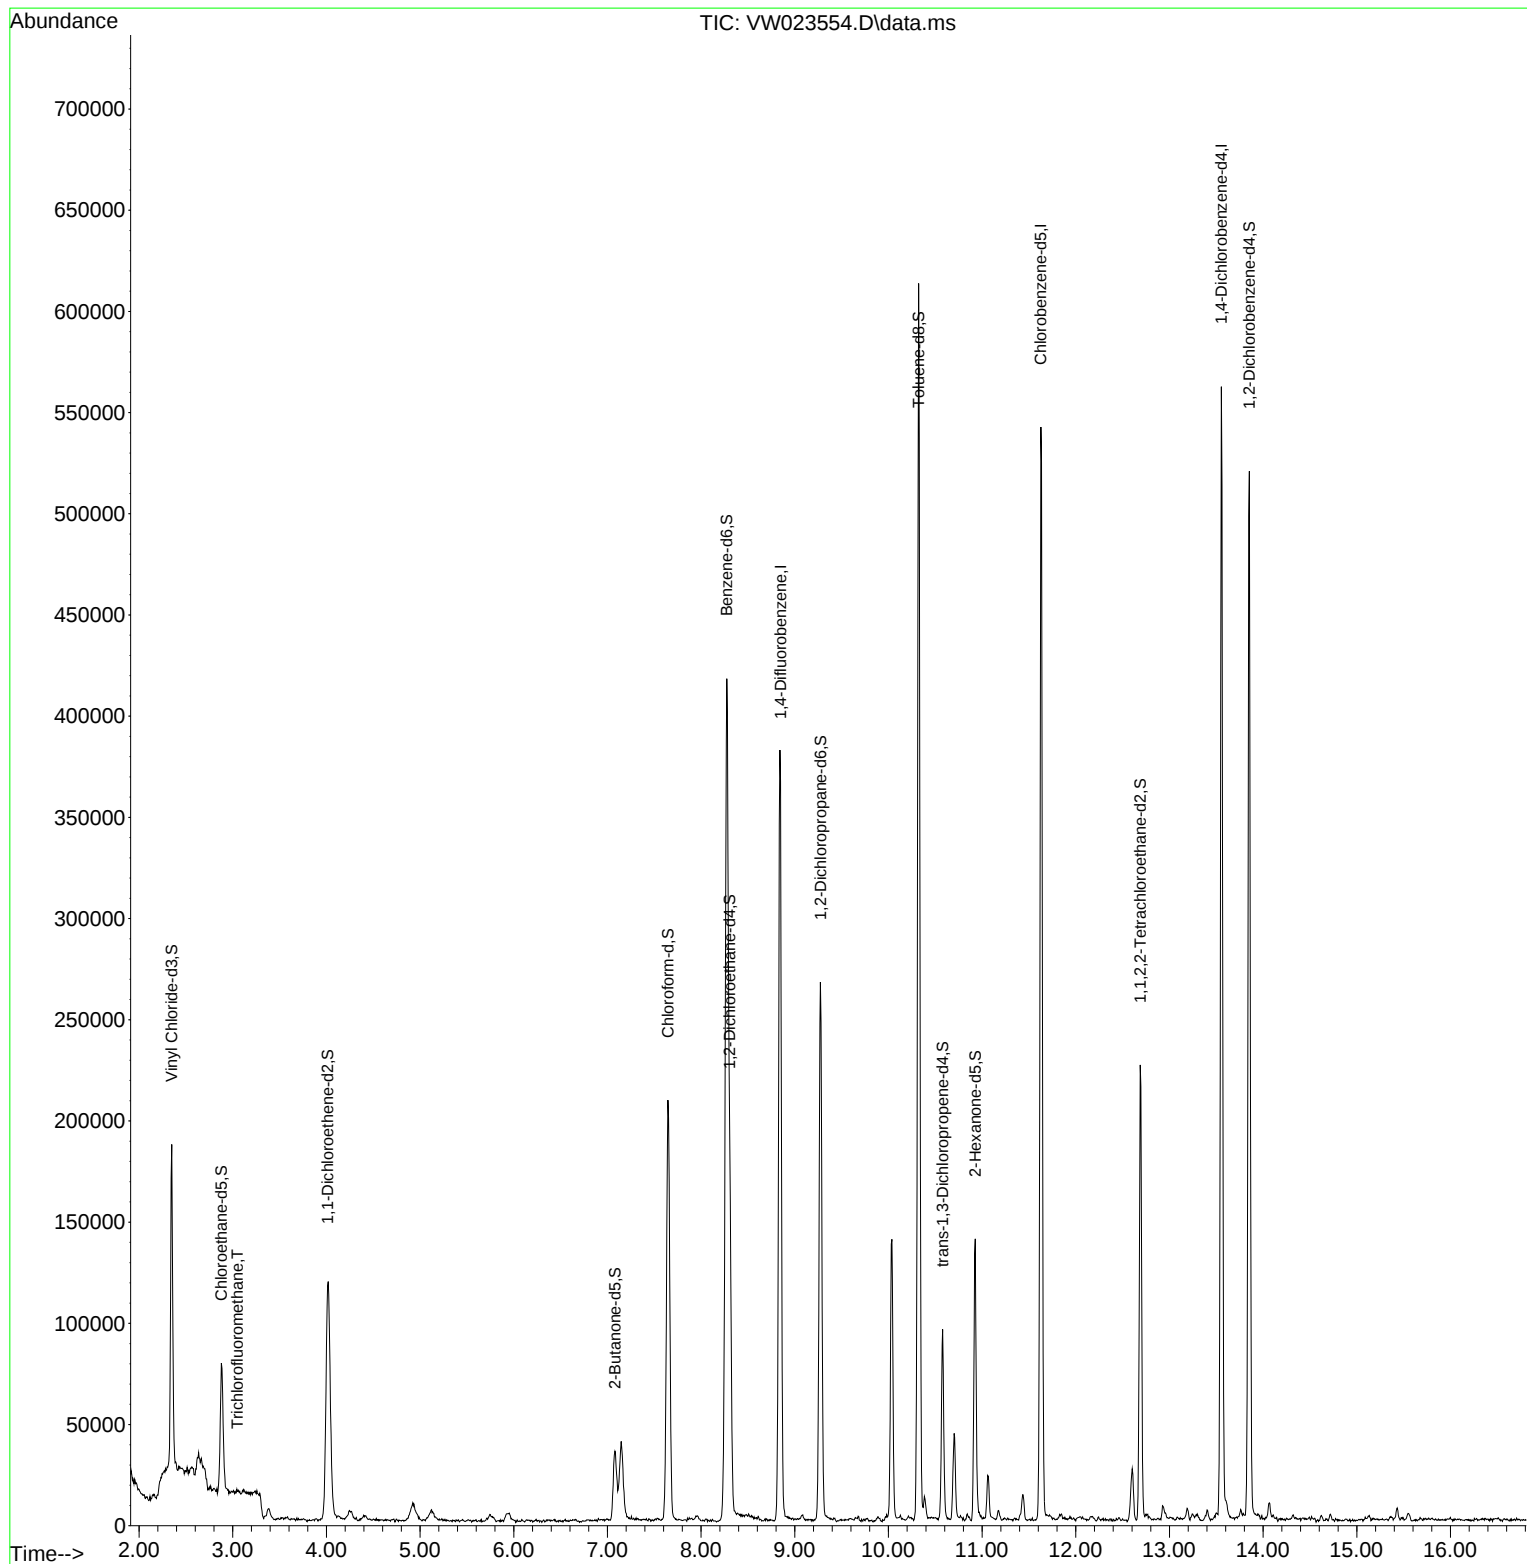

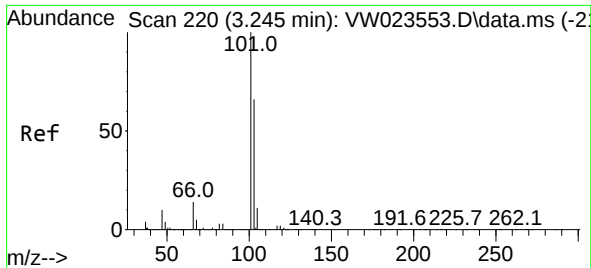

#9
 Trichlorofluoromethane
 Concen: 0.062 ug/L
 RT: 3.050 min Scan# 11
 Delta R.T. -0.195 min
 Lab File: VW023554.D
 Acq: 01 Jul 2022 11:44

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK536

Tgt Ion:101 Resp: 148
 Ion Ratio Lower Upper
 101 100
 103 64.2 53.2 79.8

