

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
 Data File : VW023555.D
 Acq On : 01 Jul 2022 13:09
 Operator : SY/VA
 Sample : N3553-08
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF8

Quant Time: Jul 04 01:22:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 04 01:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	391778	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	363191	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	168325	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	118803	21.200	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.800%
7) Chloroethane-d5	2.879	69	70179	18.184	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.720%
11) 1,1-Dichloroethene-d2	4.007	63	99927	14.412	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.640%
21) 2-Butanone-d5	7.080	46	71474	50.922	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.840%
24) Chloroform-d	7.647	84	250494	23.422	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.680%
26) 1,2-Dichloroethane-d4	8.305	65	132261	22.394	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.560%
32) Benzene-d6	8.269	84	431959	21.998	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.000%
36) 1,2-Dichloropropane-d6	9.275	67	142487	24.543	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.160%
41) Toluene-d8	10.323	98	417580	21.865	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.440%
43) trans-1,3-Dichloroprop...	10.573	79	57976	22.542	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.160%
47) 2-Hexanone-d5	10.921	63	55568	50.458	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.920%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	133652	23.977	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	151725	24.715	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.840%
Target Compounds						Qvalue
9) Trichlorofluoromethane	2.934	101	112	0.038	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
Data File : VW023555.D
Acq On : 01 Jul 2022 13:09
Operator : SY/VA
Sample : N3553-08
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AF8

Quant Time: Jul 04 01:22:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 04 01:19:17 2022
Response via : Initial Calibration

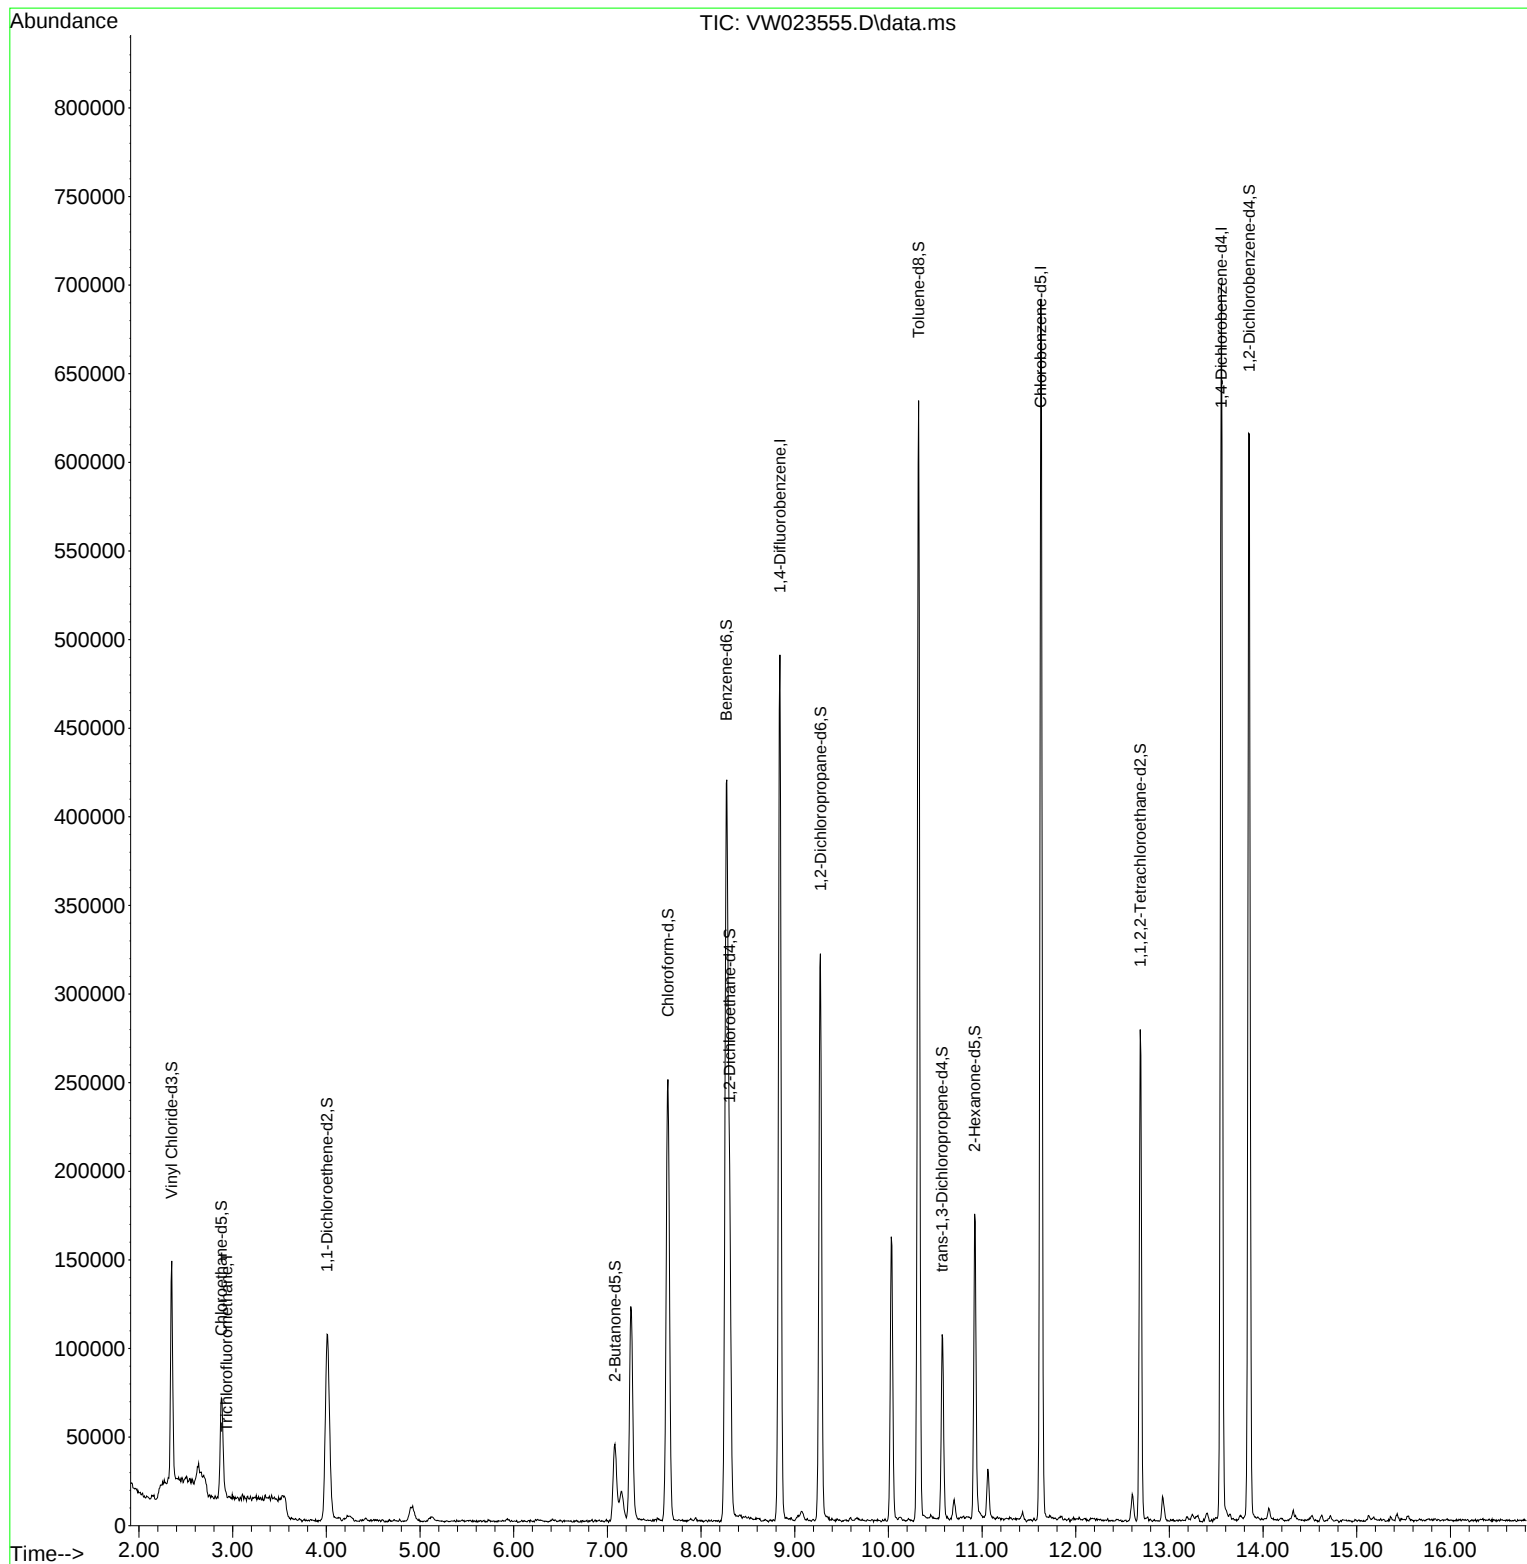

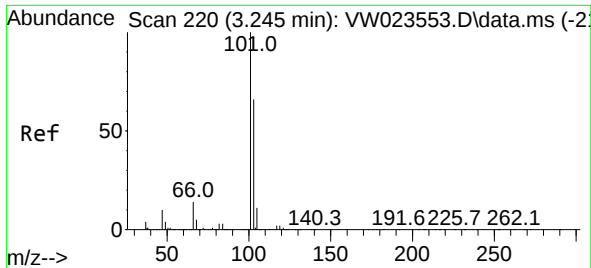

#9
 Trichlorofluoromethane
 Concen: 0.038 ug/L
 RT: 2.934 min Scan# 1
 Delta R.T. -0.311 min
 Lab File: VW023555.D
 Acq: 01 Jul 2022 13:09

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF8

Tgt Ion:101 Resp: 112
 Ion Ratio Lower Upper
 101 100
 103 73.2 53.2 79.8

