

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
 Data File : VW023557.D
 Acq On : 01 Jul 2022 13:59
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK502

Quant Time: Jul 04 01:23:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 04 01:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	322186	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	311699	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	136766	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	151642	32.904	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	131.600%
7) Chloroethane-d5	2.879	69	76534	24.114	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.440%
11) 1,1-Dichloroethene-d2	4.013	63	105493	18.501	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.000%
21) 2-Butanone-d5	7.080	46	61730	53.479	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.960%
24) Chloroform-d	7.647	84	201507	22.911	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.640%
26) 1,2-Dichloroethane-d4	8.305	65	117556	24.204	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.800%
32) Benzene-d6	8.274	84	388547	23.056	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.240%
36) 1,2-Dichloropropane-d6	9.274	67	113765	22.833	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.320%
41) Toluene-d8	10.323	98	365234	22.283	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.120%
43) trans-1,3-Dichloroprop...	10.579	79	49825	22.573	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.280%
47) 2-Hexanone-d5	10.926	63	46847	49.567	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.140%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111271	23.260	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	121387	24.336	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.360%
Target Compounds						Qvalue
9) Trichlorofluoromethane	3.233	101	107	0.045	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
Data File : VW023557.D
Acq On : 01 Jul 2022 13:59
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK502

Quant Time: Jul 04 01:23:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 04 01:19:17 2022
Response via : Initial Calibration

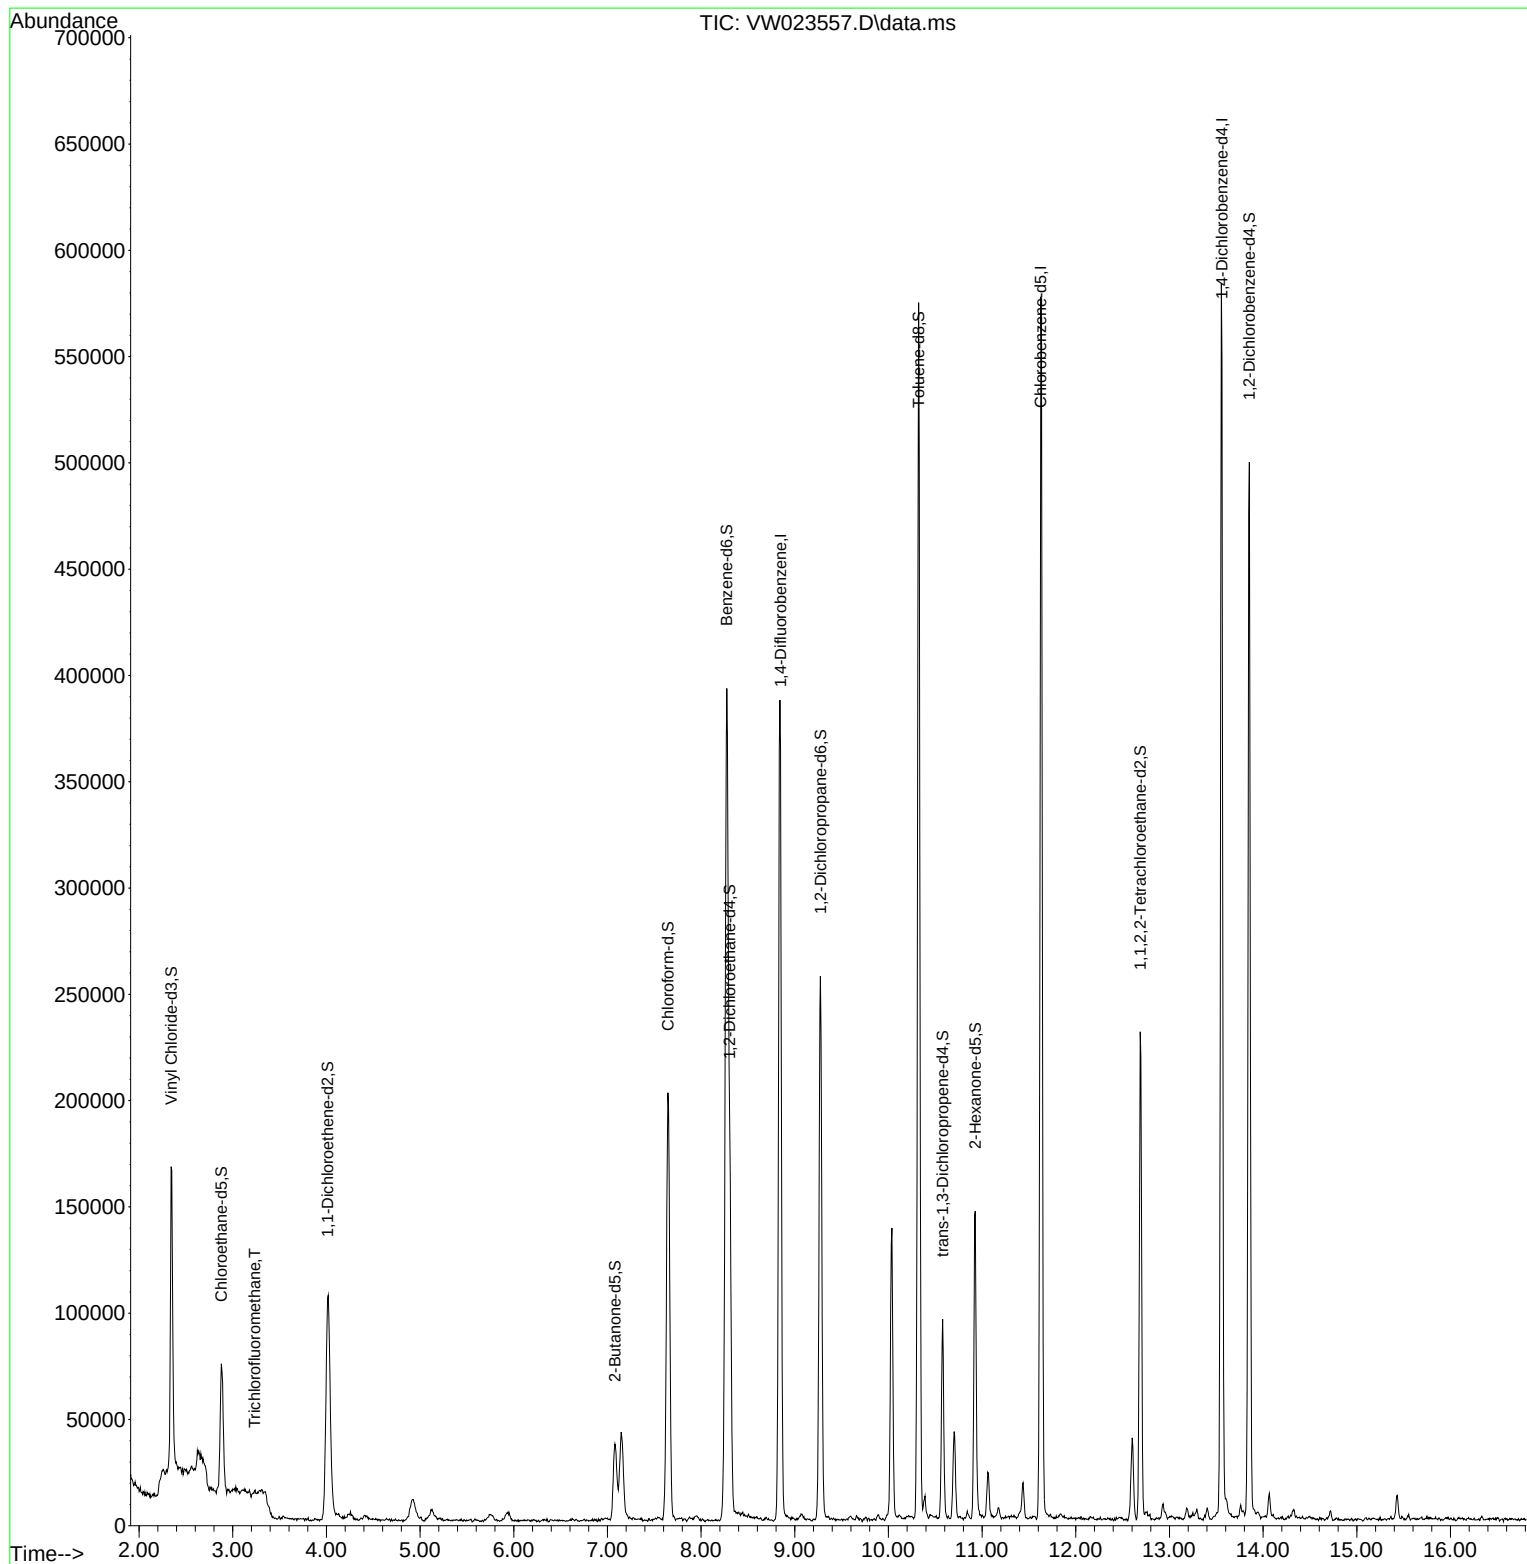

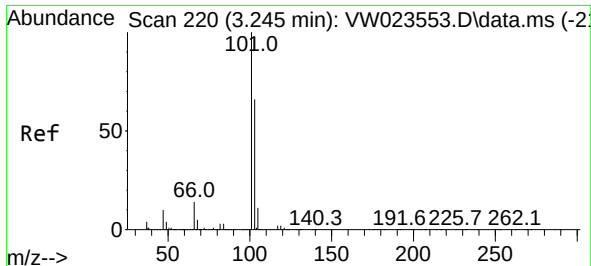

#9
 Trichlorofluoromethane
 Concen: 0.045 ug/L
 RT: 3.233 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: VW023557.D
 Acq: 01 Jul 2022 13:59

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK502

Tgt Ion:101 Resp: 107
 Ion Ratio Lower Upper
 101 100
 103 59.8 53.2 79.8

