

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
 Data File : VW023558.D
 Acq On : 01 Jul 2022 14:24
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK503

Quant Time: Jul 04 01:23:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 04 01:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	302853	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	285530	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	126309	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	149657	34.546	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	138.200%
7) Chloroethane-d5	2.885	69	72937	24.447	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.800%
11) 1,1-Dichloroethene-d2	4.013	63	99121	18.493	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.960%
21) 2-Butanone-d5	7.080	46	57765	53.239	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.480%
24) Chloroform-d	7.647	84	202534	24.498	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.000%
26) 1,2-Dichloroethane-d4	8.305	65	119093	26.086	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.360%
32) Benzene-d6	8.275	84	392832	25.446	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.800%
36) 1,2-Dichloropropane-d6	9.275	67	117007	25.636	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.560%
41) Toluene-d8	10.323	98	367963	24.507	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.040%
43) trans-1,3-Dichloroprop...	10.579	79	48897	24.183	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.720%
47) 2-Hexanone-d5	10.921	63	43877	50.679	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.360%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	107818	24.603	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	127821	27.747	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.000%
Target Compounds						Qvalue
9) Trichlorofluoromethane	3.300	101	72	0.032	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
Data File : VW023558.D
Acq On : 01 Jul 2022 14:24
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK503

Quant Time: Jul 04 01:23:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 04 01:19:17 2022
Response via : Initial Calibration

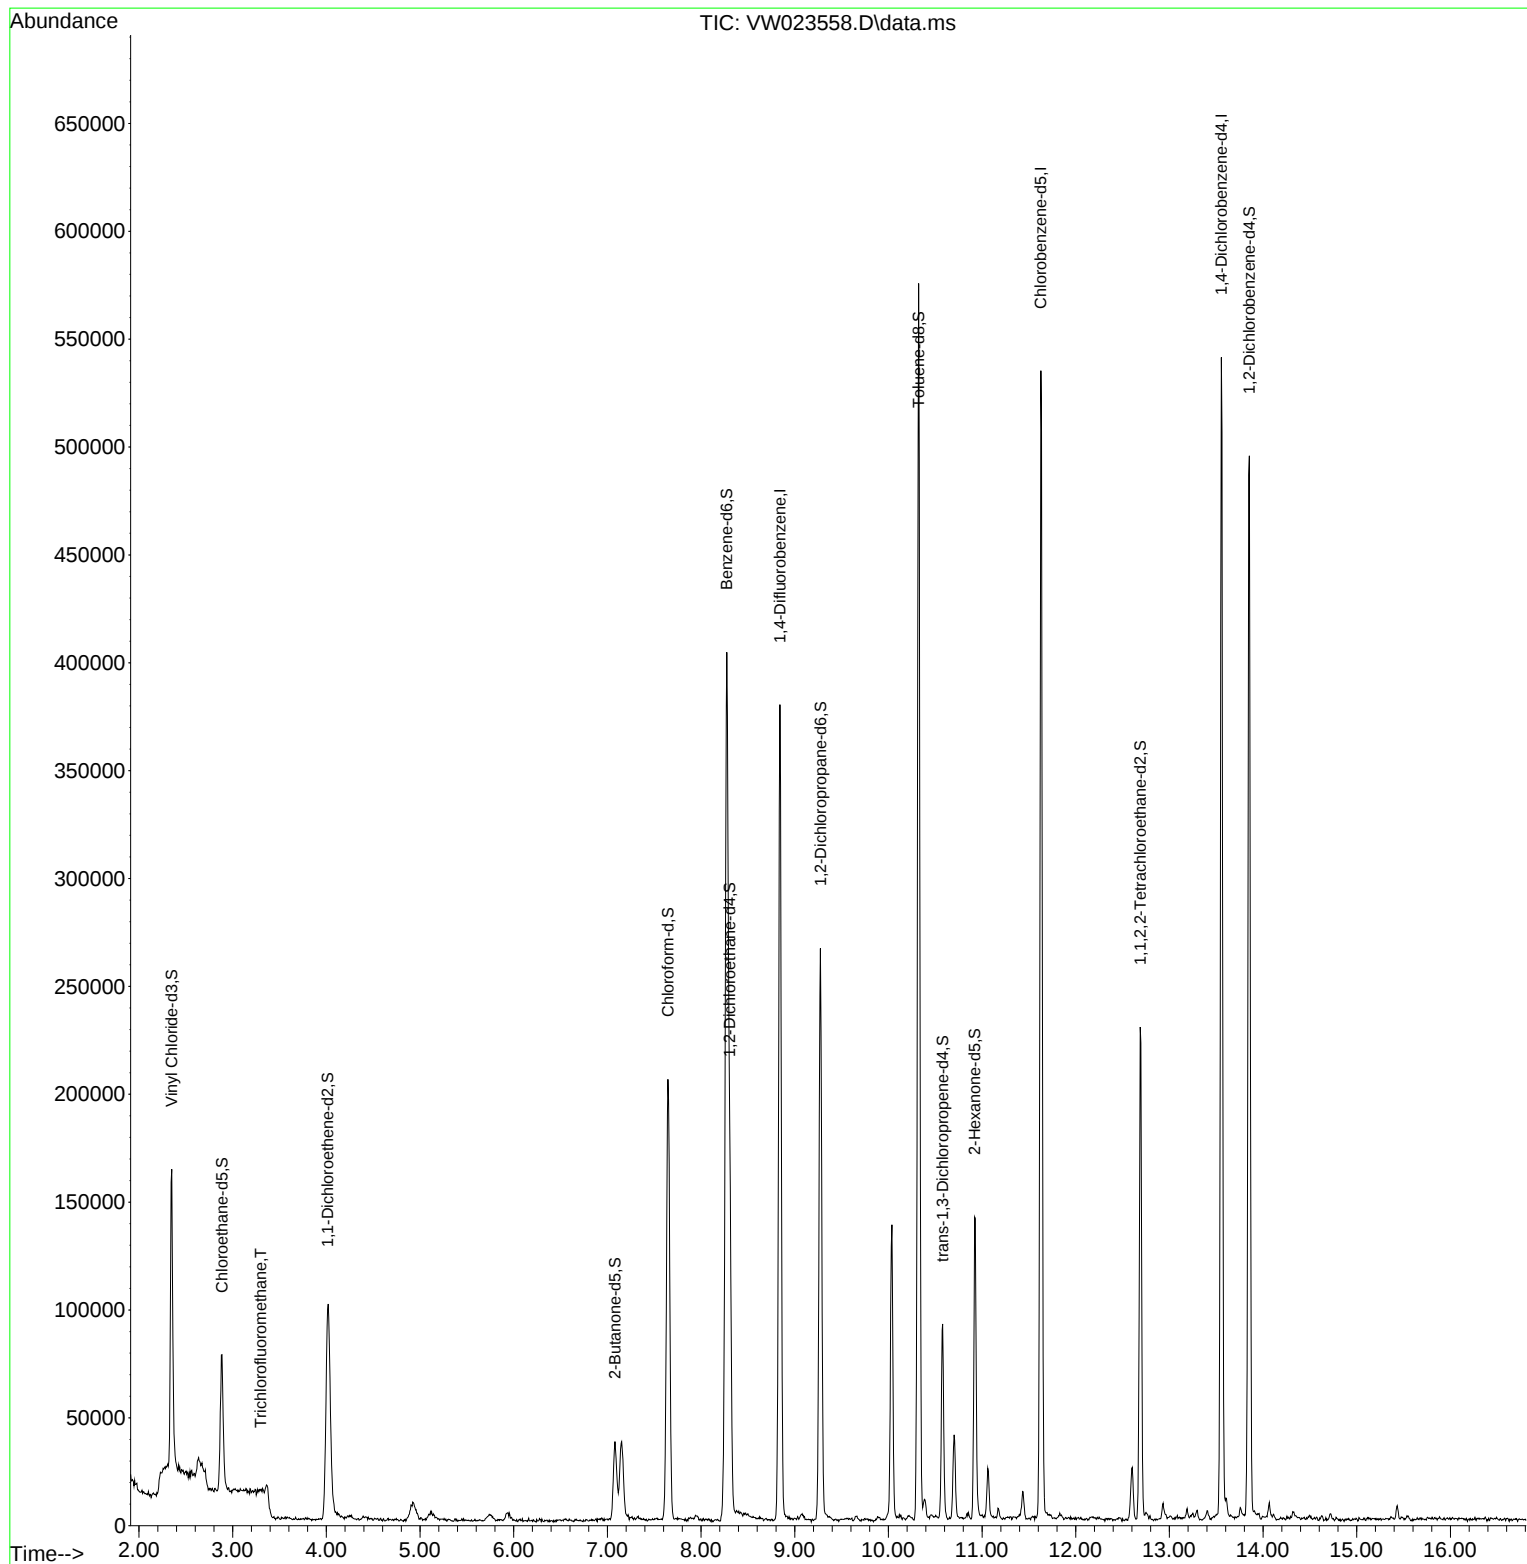

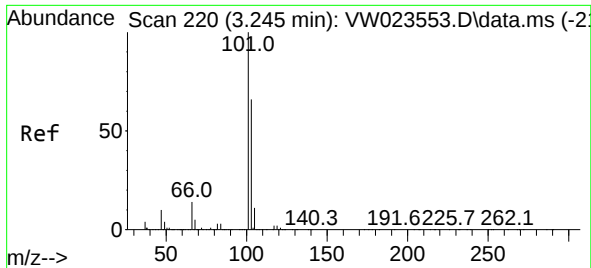

#9
 Trichlorofluoromethane
 Concen: 0.032 ug/L
 RT: 3.300 min Scan# 21
 Delta R.T. 0.055 min
 Lab File: VW023558.D
 Acq: 01 Jul 2022 14:24

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK503

Tgt Ion:101 Resp: 72
 Ion Ratio Lower Upper
 101 100
 103 65.3 53.2 79.8

