
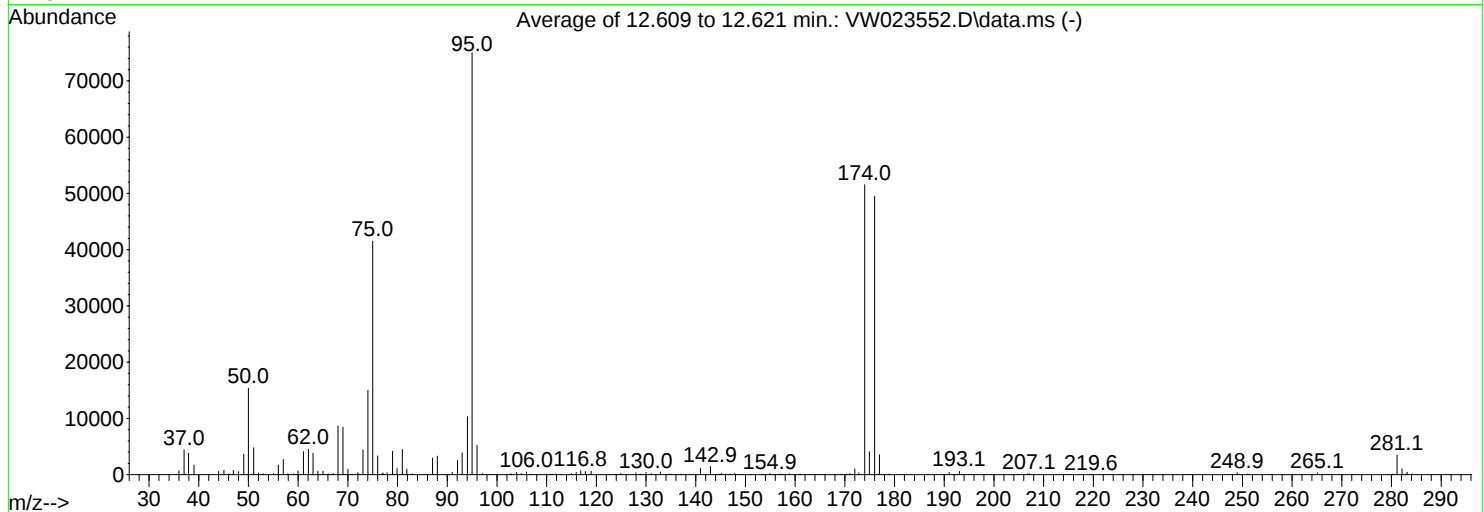


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070122\
Data File : VW023552.D
Acq On : 01 Jul 2022 09:28
Operator : SY/VA
Sample : BFB579
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB579

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Title : SFAM01.0
Last Update : Mon Jul 04 01:19:17 2022

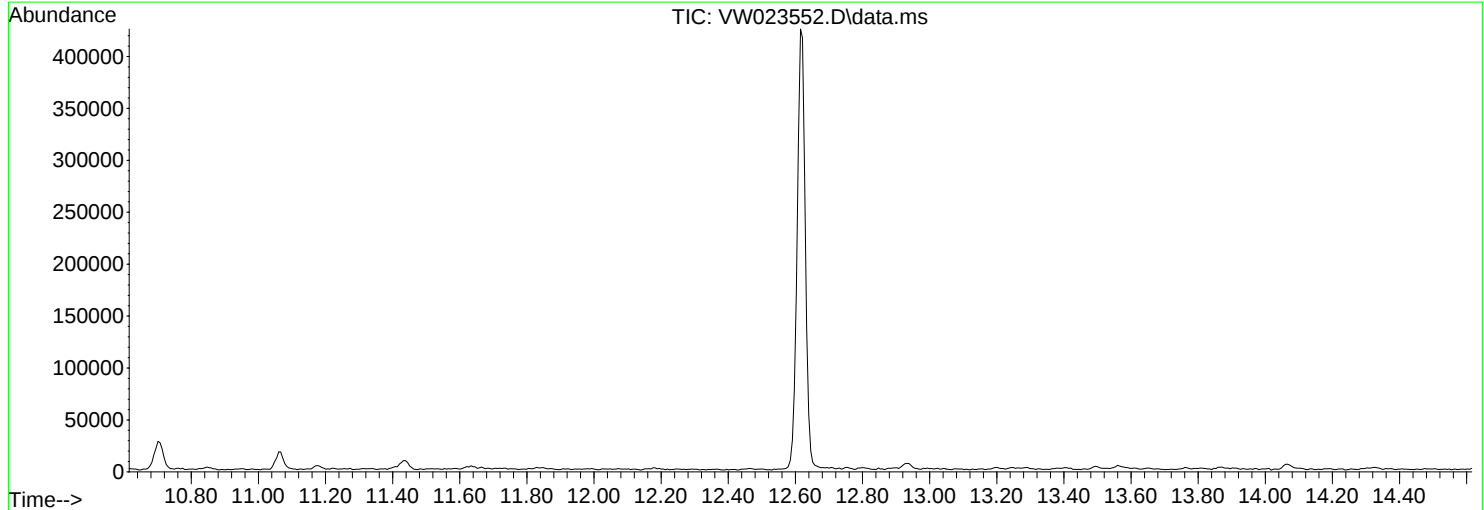

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	15366	PASS
75	95	30	80	55.3	41507	PASS
95	95	100	100	100.0	74995	PASS
96	95	5	9	7.0	5240	PASS
173	174	0.00	2	0.6	315	PASS
174	95	50	120	68.8	51563	PASS
175	174	5	9	7.9	4082	PASS
176	174	95	105	96.1	49531	PASS
177	176	5	10	7.1	3534	PASS

m/z	Abundance
35.20	61.0
36.40	59.0
37.90	79.0
40.00	248.0
40.90	73.0
41.10	74.0
42.40	65.0
42.80	90.0
43.90	195.0
45.10	91.0
45.80	83.0
46.20	67.0
46.70	51.0
47.00	53.0
47.70	68.0
50.10	59.0
50.70	96.0
51.40	63.0
54.50	59.0
55.20	122.0
57.00	146.0
64.30	50.0
68.50	64.0
76.90	63.0
78.50	64.0
79.90	84.0
81.70	62.0
82.30	66.0
84.30	113.0
86.30	73.0
93.20	60.0
95.50	77.0
103.40	64.0
130.70	73.0
155.50	62.0
181.00	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

m/z	Abundance
36.10	689.0
37.00	3944.0
38.00	3334.0
39.00	1593.0
39.90	251.0
40.80	78.0
43.10	116.0
44.10	780.0
45.00	865.0
46.10	363.0
47.00	650.0
48.00	465.0
49.10	2990.0
50.00	13449.0
51.00	3878.0
51.90	229.0
52.50	76.0
53.10	133.0
53.80	104.0
55.00	286.0
56.00	1457.0
57.10	2350.0
57.90	184.0
59.10	249.0
61.10	3556.0
62.10	3636.0
63.00	3059.0
64.00	583.0
65.00	644.0
65.90	127.0
67.10	238.0
68.00	7580.0
69.00	7420.0
70.00	832.0
72.00	394.0
73.00	3815.0
74.10	12370.0
75.00	35592.0
76.00	3203.0
76.90	680.0
77.90	340.0
79.00	3089.0
79.90	1005.0
80.90	4328.0
81.90	895.0
83.10	133.0
84.10	102.0
87.00	2549.0
88.00	2662.0
91.10	357.0
92.00	2139.0
93.00	2995.0
94.00	7808.0
95.00	60808.0
96.00	4647.0
97.10	157.0
97.90	60.0
98.70	51.0
102.90	254.0
104.00	424.0
104.90	163.0
106.00	488.0
107.10	102.0
110.00	133.0
110.90	100.0
111.90	87.0
115.00	157.0
115.90	353.0
116.80	557.0
117.80	601.0
118.90	586.0
120.00	58.0
120.80	75.0
125.00	339.0
128.00	242.0
128.80	132.0
130.00	330.0
131.00	265.0
132.90	815.0
134.80	173.0
136.90	103.0
140.90	953.0
143.00	1079.0
144.00	75.0
145.10	313.0
146.10	95.0
147.90	216.0
151.10	67.0
153.80	78.0
154.90	180.0
155.80	56.0
157.20	270.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

157.70	59.0
158.80	148.0
161.10	95.0
162.90	85.0
166.00	58.0
169.20	107.0
170.30	95.0
171.10	123.0
172.00	609.0
172.80	945.0
174.00	39608.0
174.90	3183.0
176.00	36080.0
176.90	2879.0
177.90	117.0
178.80	231.0
191.00	484.0
191.90	123.0
193.00	870.0
193.90	206.0
194.90	77.0
205.00	76.0
207.10	350.0
208.00	83.0
239.30	63.0
249.00	528.0
249.90	68.0
251.00	213.0
265.10	522.0
266.10	127.0
266.90	238.0
279.20	98.0
281.10	5169.0
282.10	1321.0
283.10	599.0
284.10	244.0
286.10	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

m/z	Abundance
35.90	754.0
37.10	4890.0
38.00	4343.0
39.10	1777.0
40.00	217.0
41.30	99.0
42.20	88.0
42.90	123.0
44.10	831.0
45.10	891.0
46.00	289.0
46.90	760.0
48.00	540.0
49.00	4119.0
50.00	16201.0
51.10	5044.0
52.00	214.0
53.00	163.0
54.00	82.0
55.00	343.0
56.00	1782.0
57.00	3212.0
57.90	173.0
59.10	192.0
59.90	963.0
61.00	4674.0
62.00	5142.0
63.00	4410.0
64.00	466.0
64.90	608.0
66.10	130.0
67.00	456.0
68.00	9657.0
69.00	9143.0
70.00	953.0
70.90	139.0
72.00	666.0
73.10	5191.0
74.00	16792.0
75.00	46272.0
76.00	3464.0
77.10	581.0
77.90	343.0
79.00	5120.0
79.90	1202.0
81.00	4945.0
81.90	1089.0
83.00	195.0
84.00	70.0
85.90	325.0
87.10	3164.0
88.00	3369.0
89.40	59.0
90.10	65.0
91.00	496.0
92.10	2996.0
93.00	4684.0
94.00	11776.0
95.00	82528.0
96.00	6124.0
97.10	208.0
102.90	136.0
103.80	594.0
104.90	174.0
106.00	453.0
106.80	152.0
109.90	157.0
110.60	265.0
111.10	87.0
111.90	220.0
113.00	148.0
114.90	359.0
116.00	376.0
116.90	798.0
117.70	451.0
118.90	803.0
120.10	169.0
120.80	61.0
124.00	165.0
124.90	247.0
127.90	372.0
129.00	195.0
130.00	308.0
130.70	196.0
131.10	223.0
132.90	327.0
134.00	97.0
134.80	194.0
136.10	90.0
137.10	141.0
138.90	68.0
139.90	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

141.00	1133.0
142.90	1618.0
144.10	103.0
145.20	324.0
146.00	134.0
146.90	212.0
147.80	292.0
149.60	77.0
151.10	66.0
153.20	73.0
154.00	55.0
155.00	184.0
156.80	154.0
157.70	62.0
158.90	235.0
161.00	153.0
163.20	76.0
165.10	77.0
166.00	60.0
169.30	68.0
170.40	133.0
170.90	219.0
172.00	1375.0
174.00	56472.0
175.00	4556.0
176.00	52544.0
176.90	3742.0
177.90	135.0
179.00	179.0
191.00	391.0
193.10	636.0
194.20	130.0
195.10	68.0
204.90	63.0
206.80	225.0
207.10	193.0
208.10	81.0
239.20	58.0
248.90	334.0
251.10	131.0
265.10	257.0
266.20	127.0
267.30	69.0
280.30	258.0
281.20	3148.0
282.10	1130.0
283.20	672.0
284.20	167.0
285.20	75.0
286.20	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

m/z	Abundance
36.00	580.0
37.00	4478.0
38.00	3891.0
39.00	1791.0
39.90	222.0
40.90	81.0
41.90	60.0
42.40	62.0
43.90	757.0
45.00	870.0
46.00	176.0
47.00	976.0
48.00	544.0
49.10	3846.0
50.00	16624.0
51.00	5445.0
52.00	484.0
52.80	116.0
53.10	117.0
54.10	122.0
55.10	382.0
56.00	1885.0
57.10	3024.0
58.00	204.0
58.30	207.0
60.00	1021.0
61.00	4094.0
62.00	4779.0
63.00	3938.0
63.90	770.0
65.10	586.0
66.00	189.0
68.00	8673.0
69.00	8828.0
70.00	1081.0
70.90	115.0
72.20	460.0
73.00	4198.0
74.00	15832.0
75.00	42656.0
76.00	3285.0
77.00	335.0
77.90	372.0
79.00	4230.0
79.90	1339.0
80.90	4175.0
81.90	1204.0
82.90	197.0
87.00	3083.0
88.00	3898.0
90.90	467.0
92.10	2478.0
93.00	4130.0
94.10	11281.0
95.00	81648.0
96.00	4948.0
97.10	161.0
102.70	161.0
103.80	304.0
104.10	322.0
104.90	245.0
105.90	498.0
106.80	132.0
110.00	123.0
110.80	110.0
111.10	124.0
111.80	161.0
113.00	117.0
114.60	71.0
115.10	127.0
115.90	475.0
116.90	778.0
117.90	546.0
119.00	515.0
122.90	53.0
123.80	69.0
127.90	396.0
128.90	184.0
130.00	534.0
131.10	95.0
133.00	278.0
134.10	73.0
135.00	237.0
136.10	91.0
136.80	203.0
138.90	105.0
140.00	107.0
141.00	1298.0
142.00	90.0
142.90	1646.0
144.00	115.0
144.80	253.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

146.00	209.0
146.90	122.0
147.80	268.0
148.90	82.0
149.70	111.0
153.20	119.0
153.90	85.0
155.00	248.0
155.80	111.0
156.90	236.0
157.70	60.0
158.70	149.0
160.90	113.0
169.30	70.0
170.40	92.0
171.10	251.0
172.00	1106.0
174.00	58608.0
175.00	4508.0
176.00	59968.0
177.00	3982.0
178.10	186.0
186.70	79.0
190.90	290.0
192.20	89.0
193.00	223.0
194.90	51.0
195.20	62.0
204.80	57.0
206.70	158.0
207.20	102.0
219.60	54.0
248.90	178.0
251.20	75.0
265.10	146.0
265.60	58.0
266.00	65.0
280.10	104.0
281.00	2062.0
282.10	733.0
282.90	345.0
284.30	76.0
285.10	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579