



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070125\
Data File : VW031737.D
Acq On : 01 Jul 2025 09:32
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Title : SW846 8260
Last Update : Tue Jul 01 03:35:17 2025

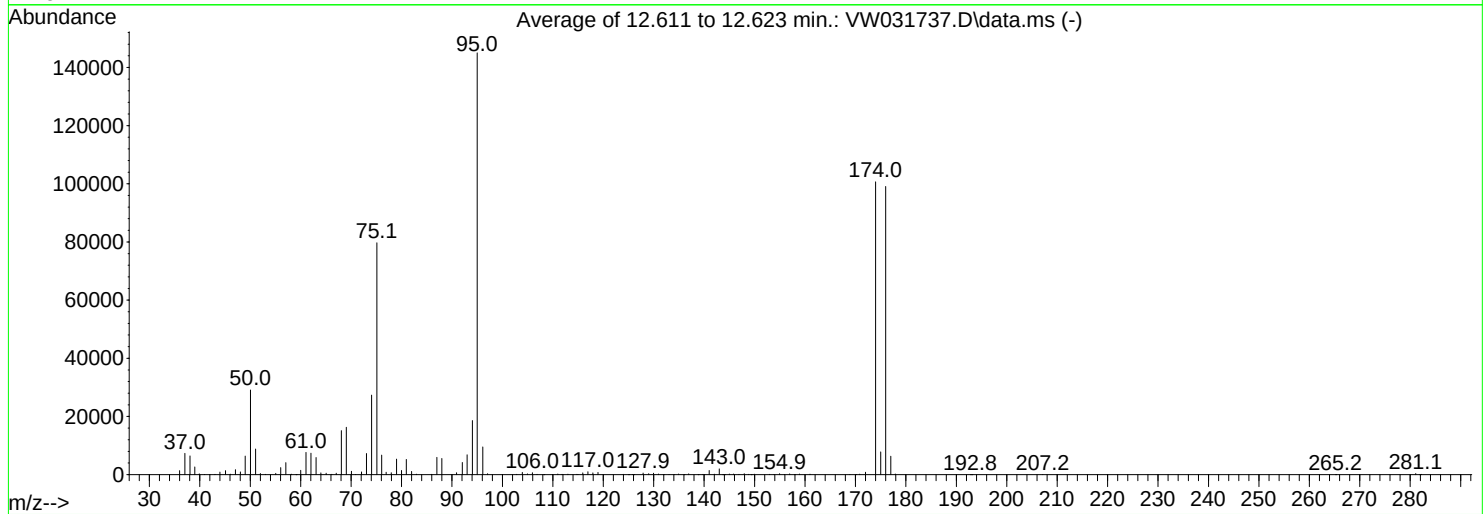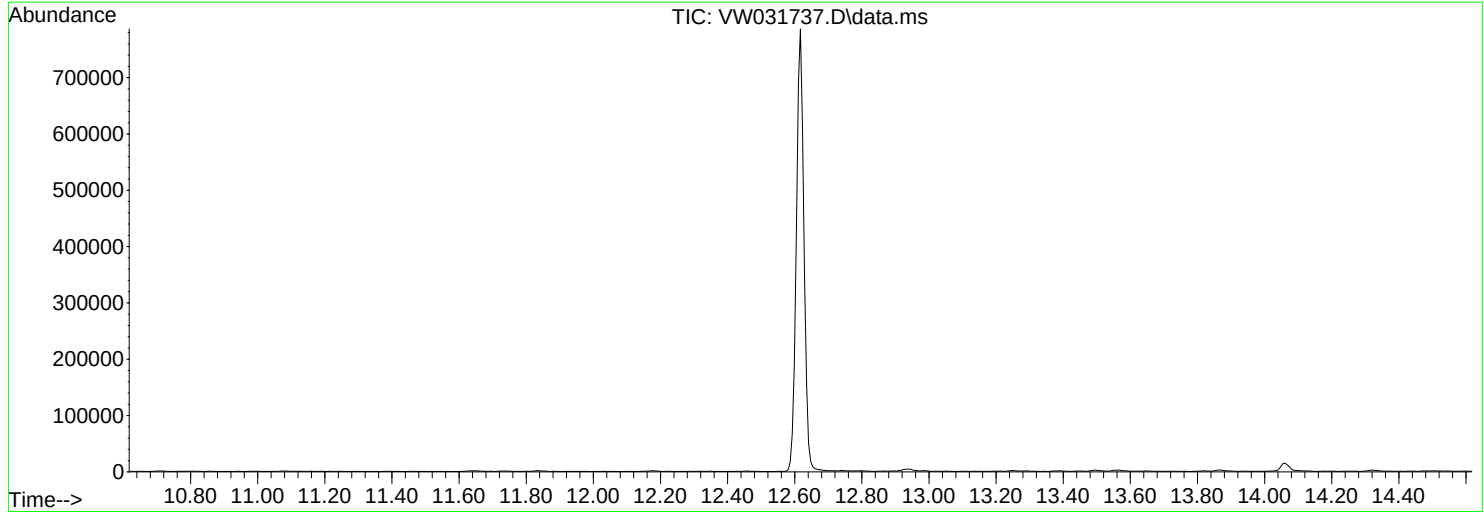

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	29117	PASS
75	95	30	60	55.0	79691	PASS
95	95	100	100	100.0	145024	PASS
96	95	5	9	6.6	9525	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.4	100696	PASS
175	174	5	9	7.8	7805	PASS
176	174	95	101	98.4	99080	PASS
177	176	5	9	6.4	6350	PASS