

Data File : VW011106.D
Acq On : 02 Jul 2019 13:27
Operator : SY/VA
Sample : VW0702SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK30

Quant Time: Jul 03 05:14:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 02 12:27:54 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	374203	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	337430	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	158840	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	142618	24.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.84%
7) Chloroethane-d5	2.88	69	95433	23.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.24%
10) 1,1-Dichloroethene-d2	4.01	63	222285	18.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.48%
20) 2-Butanone-d5	7.07	46	105242	46.76	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.52%
24) Chloroform-d	7.65	84	236865	23.09	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.36%
26) 1,2-Dichloroethane-d4	8.31	65	153167	24.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.00%
29) Benzene-d6	8.27	84	511249	24.59	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.36%
33) 1,2-Dichloropropane-d6	9.27	67	165285	24.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.68%
37) Toluene-d8	10.32	98	451017	24.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.40%
38) trans-1,3-Dichloropropene-	10.58	79	67113	23.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.28%
39) 2-Hexanone-d5	10.92	63	73314	47.23	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.46%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	132107	23.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	150003	24.60	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.40%


Target Compounds					Qvalue
42) cis-1,3-Dichloropropene	10.04	75	4679	0.549 ug/L	# 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011106.D
Acq On : 02 Jul 2019 13:27
Operator : SY/VA
Sample : VW0702SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK30

Quant Time: Jul 03 05:14:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 02 12:27:54 2019
Response via : Initial Calibration

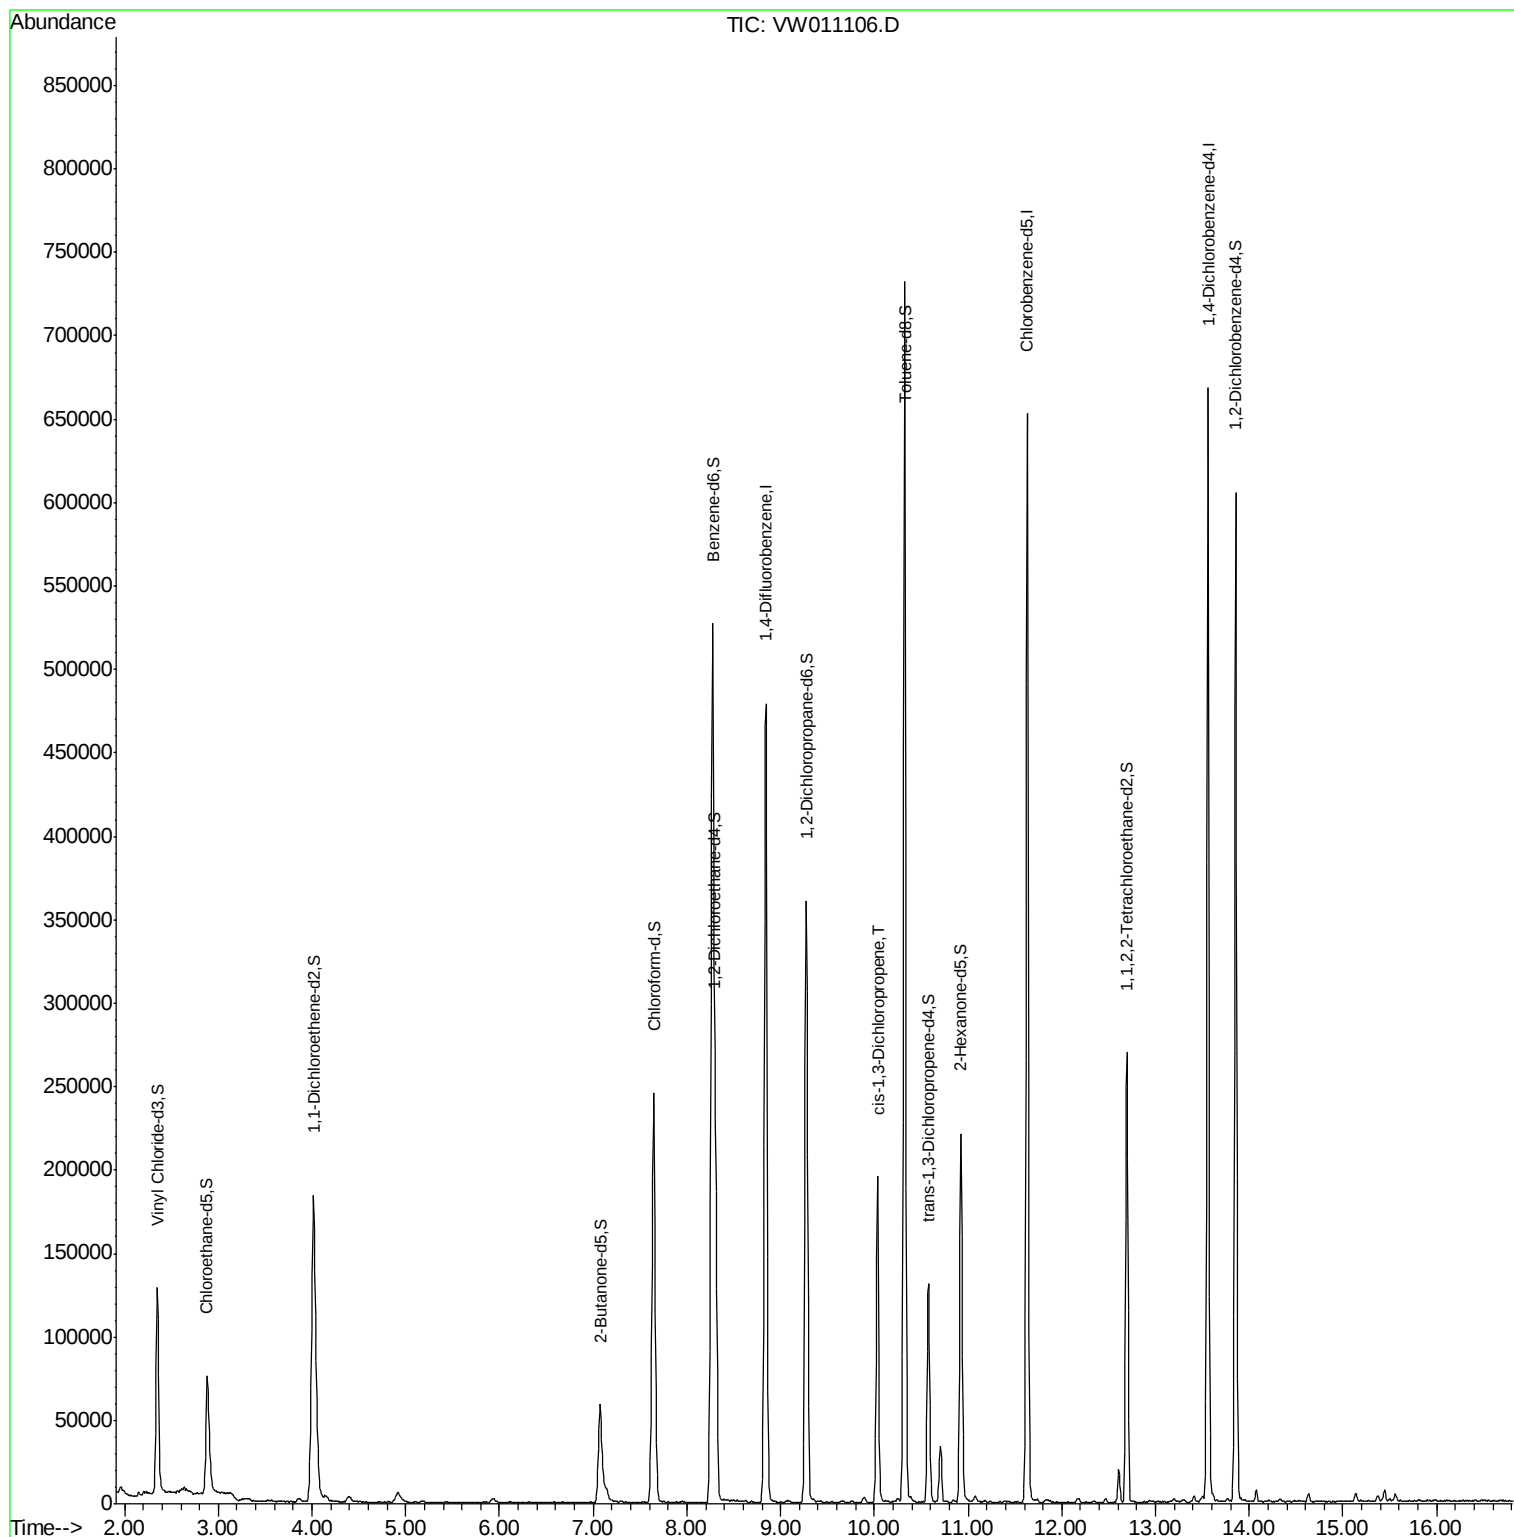

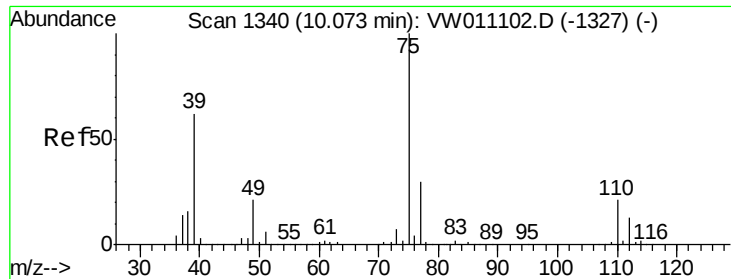

#42

cis-1,3-Dichloropropene

Concen: 0.549 ug/L

RT: 10.04 min Scan# 1334

Delta R.T. -0.04 min

Lab File: VW011106.D

Acq: 02 Jul 2019 13:27

Instrument :

MSVOA_W

ClientSampleId :

VBLK30

Tgt Ion: 75 Resp: 4679

Ion Ratio Lower Upper

75 100

77 52.9 21.1 39.1#

