

Data File : VW011115.D
Acq On : 02 Jul 2019 19:11
Operator : SY/VA
Sample : VW0702SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK01

Quant Time: Jul 03 05:54:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 03 05:51:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	345729	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	320939	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	149220	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	124280	23.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.16%
7) Chloroethane-d5	2.88	69	84204	22.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.92%
10) 1,1-Dichloroethene-d2	4.02	63	196025	17.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.12%
20) 2-Butanone-d5	7.07	46	101974	49.04	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.08%
24) Chloroform-d	7.65	84	220965	23.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.28%
26) 1,2-Dichloroethane-d4	8.30	65	143804	24.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.56%
29) Benzene-d6	8.27	84	465138	23.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.08%
33) 1,2-Dichloropropane-d6	9.27	67	154374	23.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.92%
37) Toluene-d8	10.32	98	413791	23.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.96%
38) trans-1,3-Dichloropropene-	10.57	79	60519	22.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.44%
39) 2-Hexanone-d5	10.92	63	69246	46.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.80%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	125765	23.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	138603	24.20	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.80%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.56	75	21278	5.472 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011115.D
Acq On : 02 Jul 2019 19:11
Operator : SY/VA
Sample : VW0702SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK01

Quant Time: Jul 03 05:54:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 03 05:51:41 2019
Response via : Initial Calibration

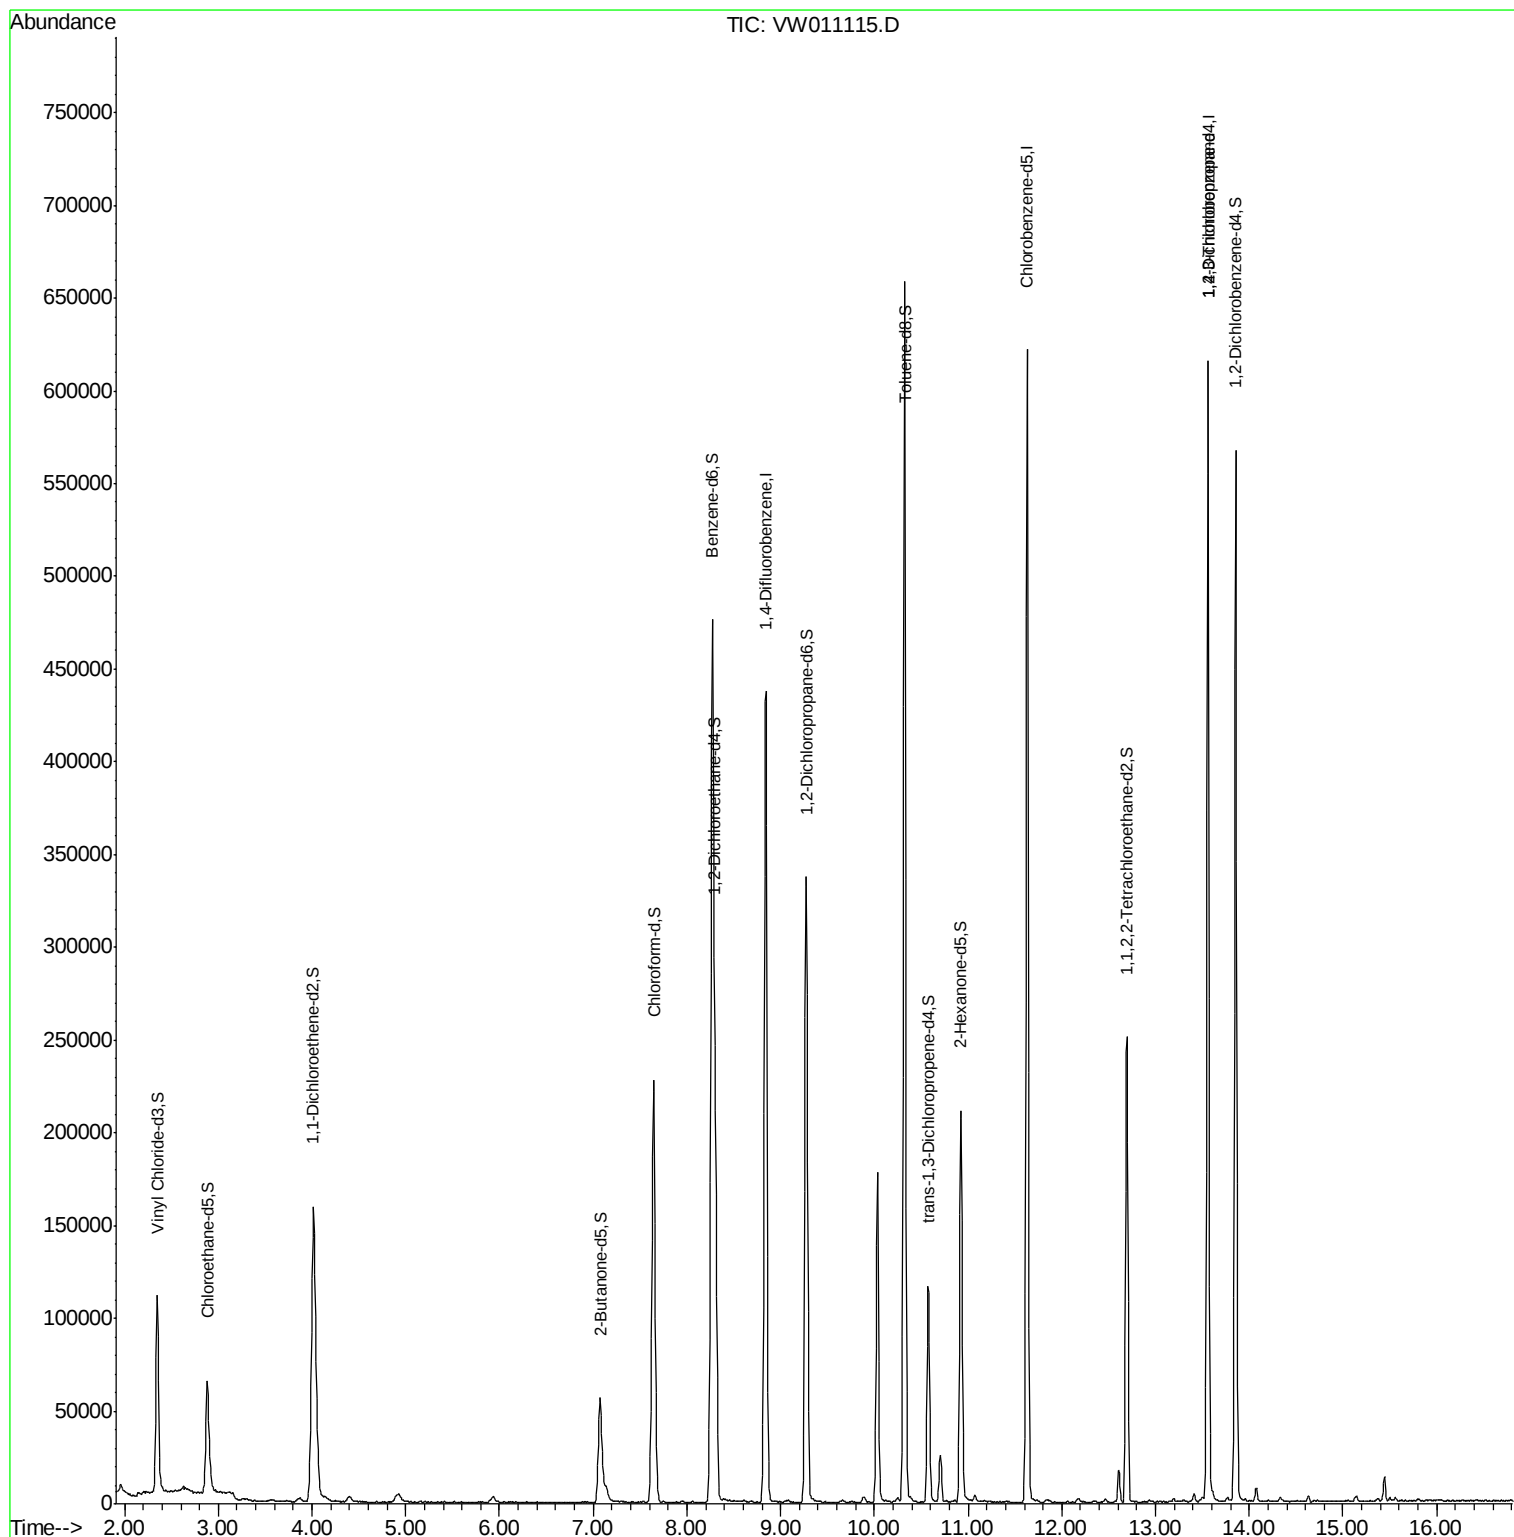

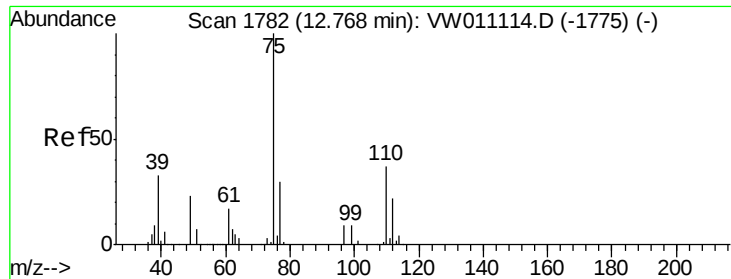

#59

1,2,3-Trichloropropane

Concen: 5.472 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW011115.D

Acq: 02 Jul 2019 19:11

Instrument :

MSVOA_W

ClientSampleId :

VBLK01

Tgt Ion: 75 Resp: 21278

Ion Ratio Lower Upper

75 100

77 36.1 25.4 38.0

