

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW070219\
 Data File : VW011112.D
 Acq On : 02 Jul 2019 16:56
 Operator : SY/VA
 Sample : K3599-07
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAM16

Quant Time: Jul 03 05:48:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 02 12:27:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	294844	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	265473	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	121743	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	79751	17.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.84%
7) Chloroethane-d5	2.88	69	59693	18.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.60%
10) 1,1-Dichloroethene-d2	4.01	63	139690	14.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.60%
20) 2-Butanone-d5	7.07	46	83909	47.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.62%
24) Chloroform-d	7.65	84	175219	21.68	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.72%
26) 1,2-Dichloroethane-d4	8.30	65	113516	22.81	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.24%
29) Benzene-d6	8.27	84	354736	21.69	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.76%
33) 1,2-Dichloropropane-d6	9.27	67	120615	22.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.60%
37) Toluene-d8	10.32	98	317155	21.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.04%
38) trans-1,3-Dichloropropene-	10.58	79	44447	19.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.52%
39) 2-Hexanone-d5	10.93	63	52723	43.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.34%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	101691	23.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	107177	22.93	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.72%


Target Compounds					Ovalue
13) Acetone	4.12	43	14053	8.113 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW070219\
Data File : VW011112.D
Acq On : 02 Jul 2019 16:56
Operator : SY/VA
Sample : K3599-07
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAM16

Quant Time: Jul 03 05:48:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 02 12:27:54 2019
Response via : Initial Calibration

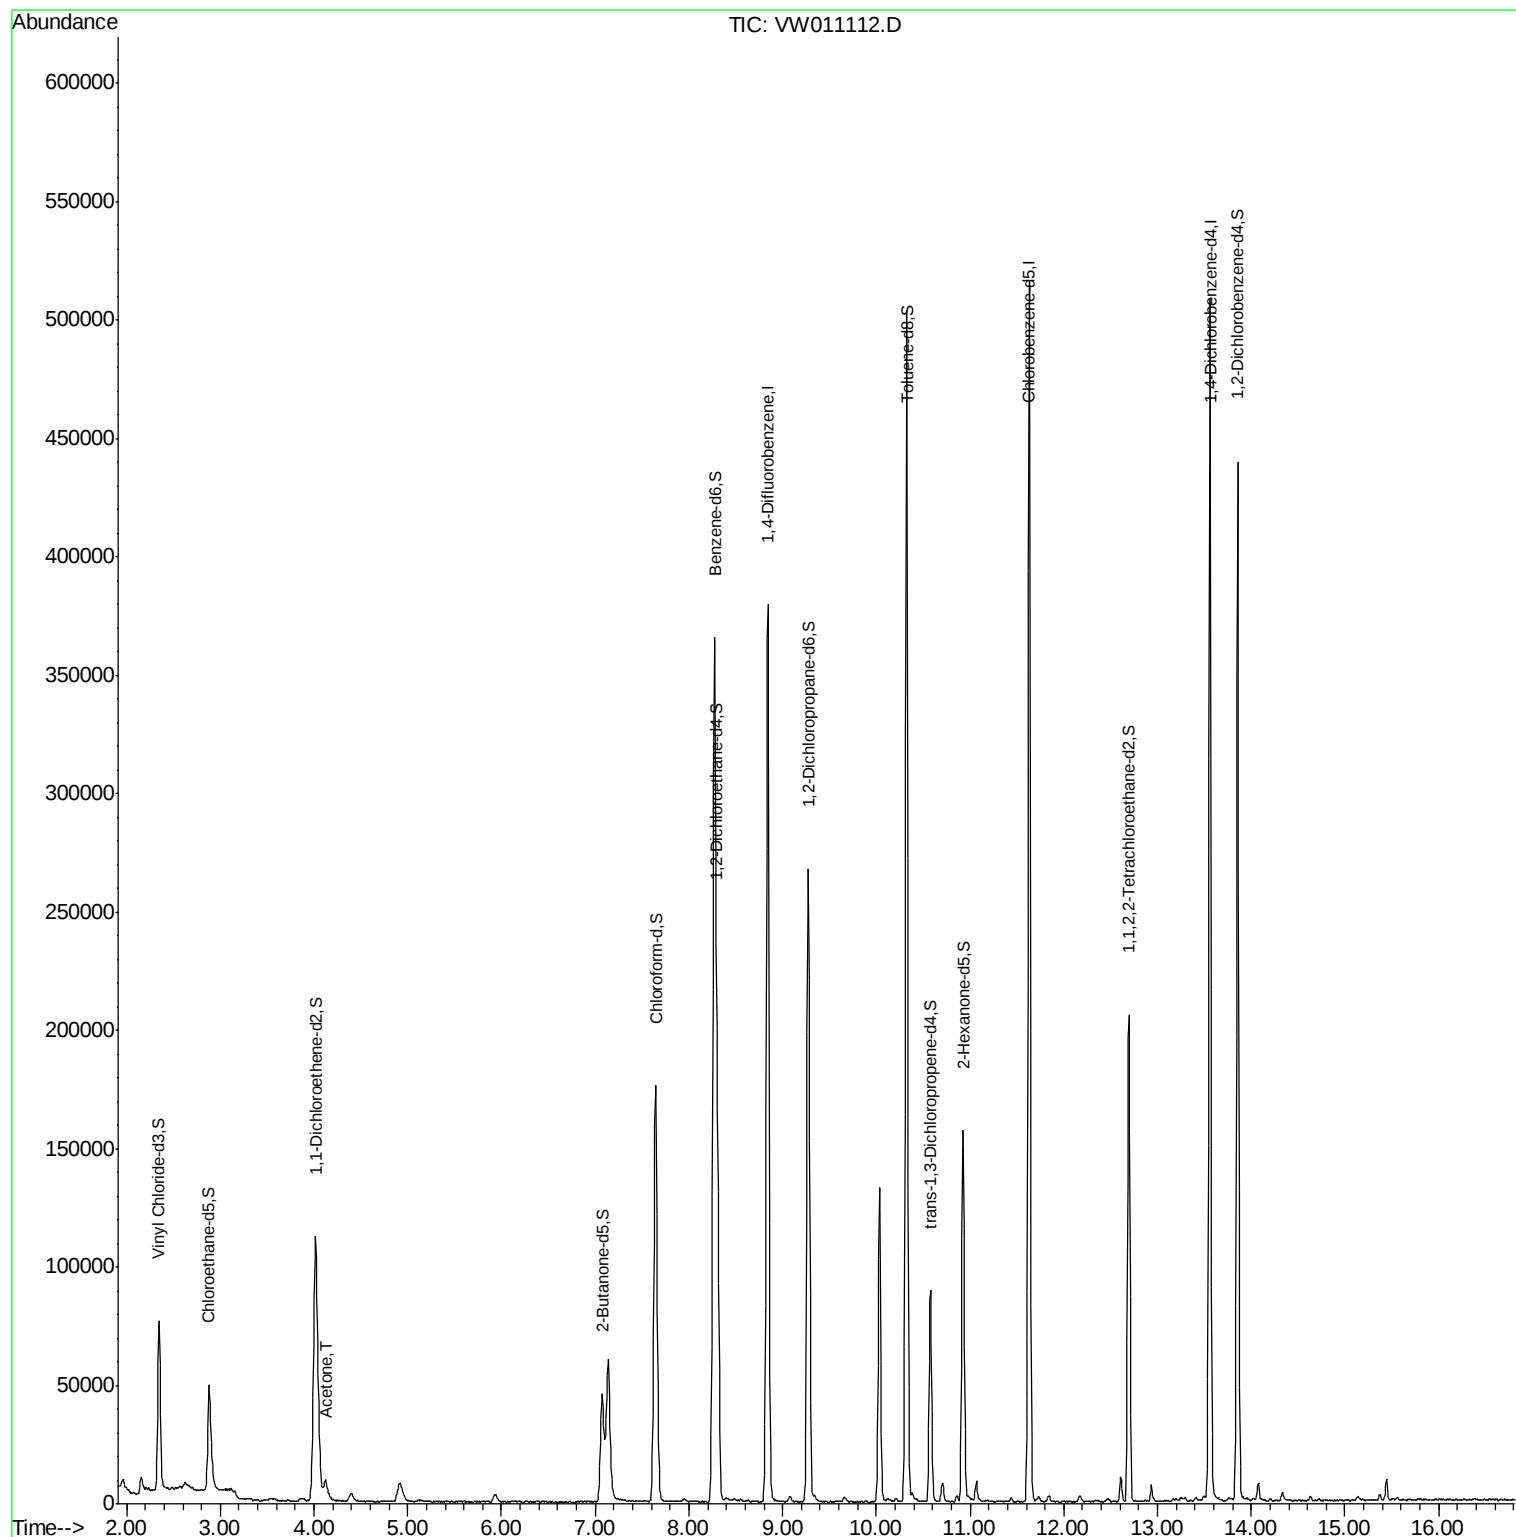

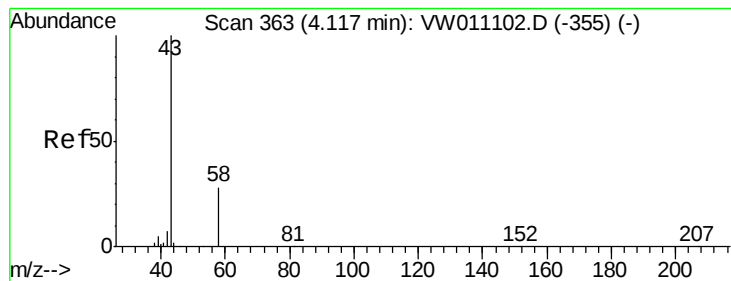

#13
 Acetone
 Concen: 8.113 ug/L
 RT: 4.12 min Scan# 363
 Delta R.T. 0.00 min
 Lab File: VW011112.D
 Acq: 02 Jul 2019 16:56

Instrument :
 MSVOA_W
 ClientSampleId :
 GAM16

Tot Ion: 43 Resp: 14053
 Ion Ratio Lower Upper
 43 100
 58 30.1 0.0 55.0

