

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
 Data File : VW029438.D
 Acq On : 02 Jul 2024 12:39
 Operator : SY/MD
 Sample : VW0702SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 03 05:42:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 03 05:41:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	242724	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	224684	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	102808	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	63063	18.771	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.080%
7) Chloroethane-d5	2.899	69	58143	20.494	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.960%
11) 1,1-Dichloroethene-d2	4.027	65	33652	20.746	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.000%
21) 2-Butanone-d5	7.081	46	53315	53.043	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.080%
24) Chloroform-d	7.648	84	173896	24.017	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.080%
26) 1,2-Dichloroethane-d4	8.307	65	102757	24.718	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.880%
32) Benzene-d6	8.276	84	329520	24.145	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.600%
36) 1,2-Dichloropropane-d6	9.270	67	111717	25.752	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.000%
41) Toluene-d8	10.319	98	288849	23.923	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.680%
43) trans-1,3-Dichloroprop...	10.575	79	42113	24.089	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.360%
47) 2-Hexanone-d5	10.922	63	34605	50.885	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.760%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	86912	25.172	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	98243	27.530	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.120%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3406	0.635	ug/L	Qvalue # 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029438.D
Acq On : 02 Jul 2024 12:39
Operator : SY/MD
Sample : VW0702SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jul 03 05:42:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

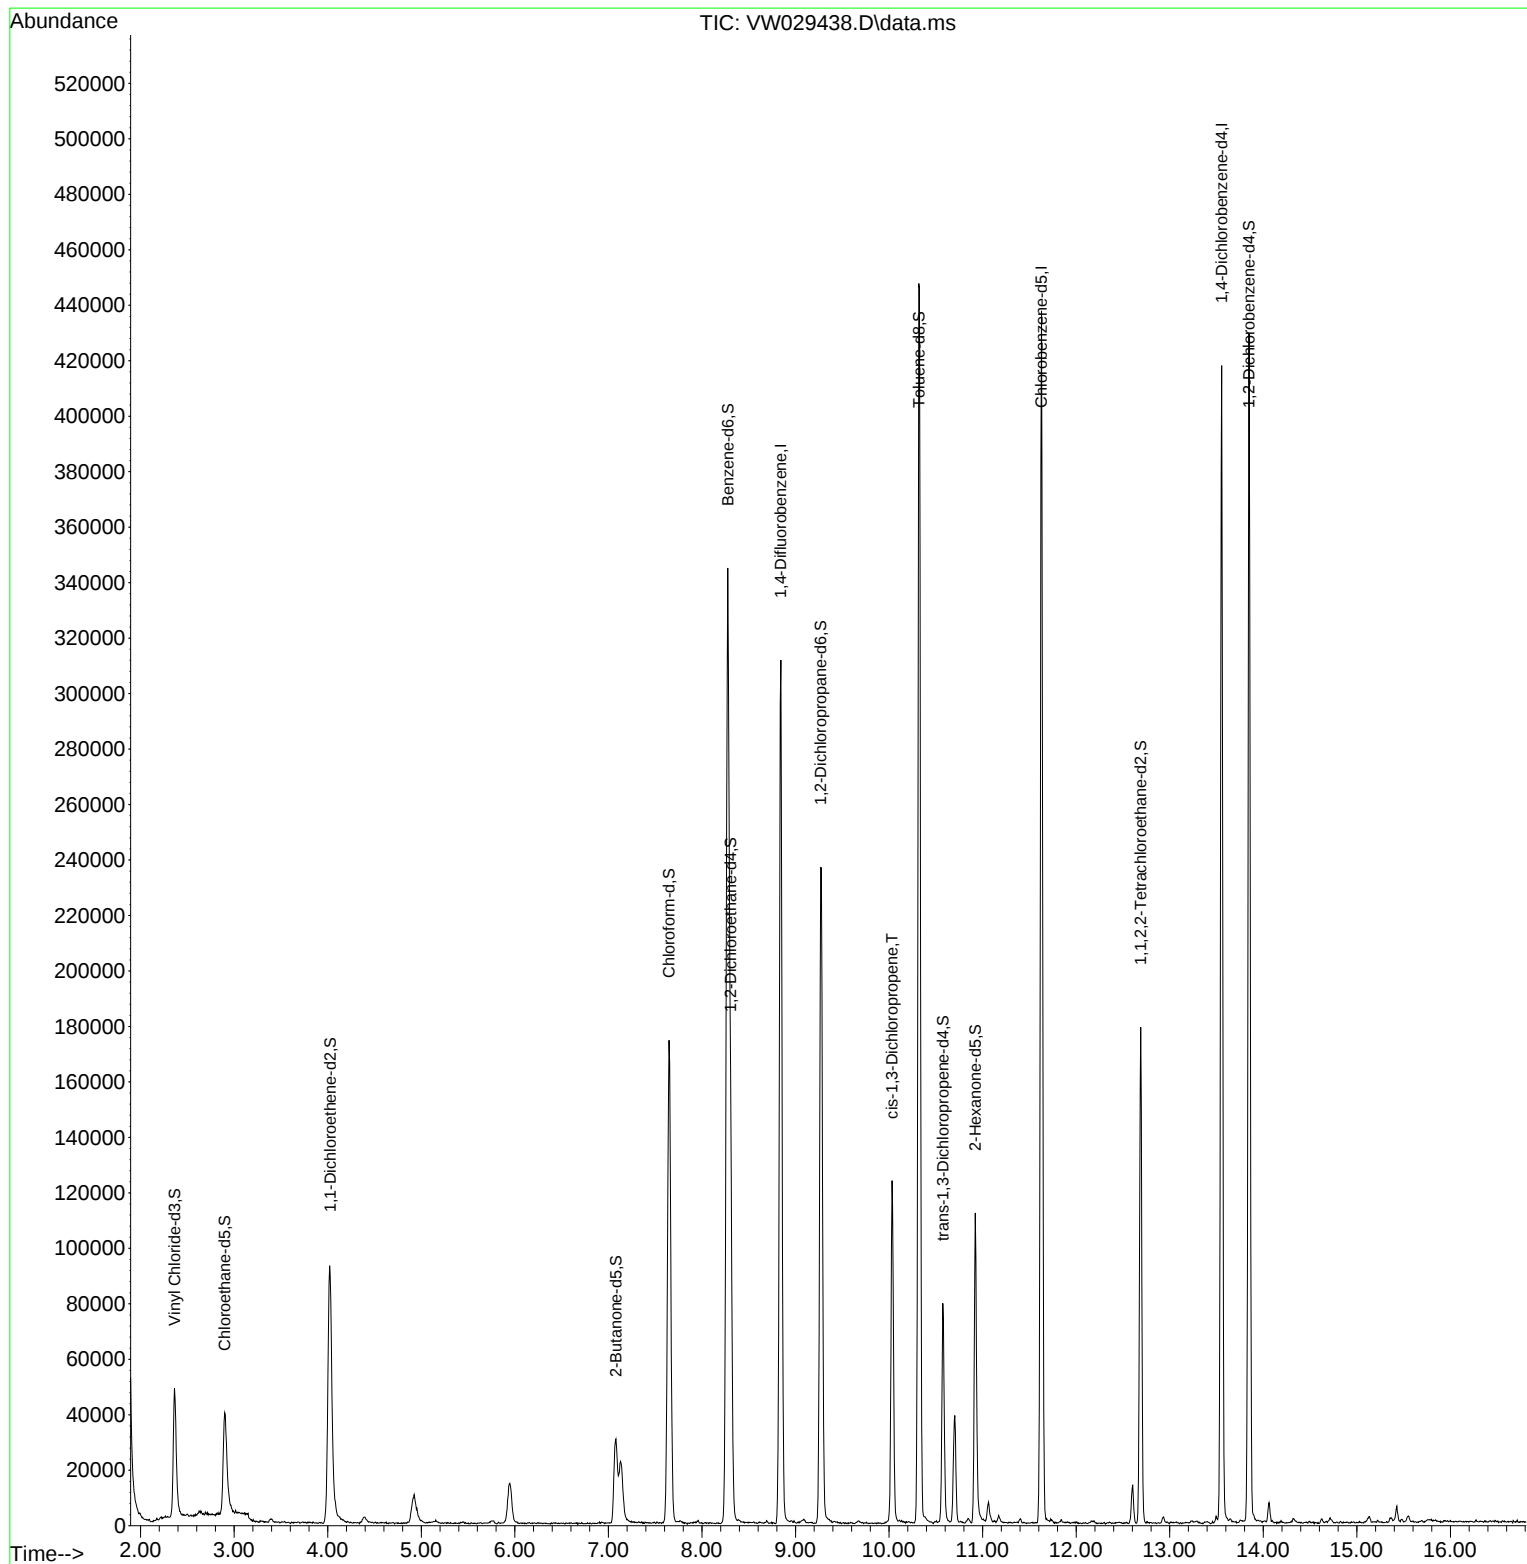

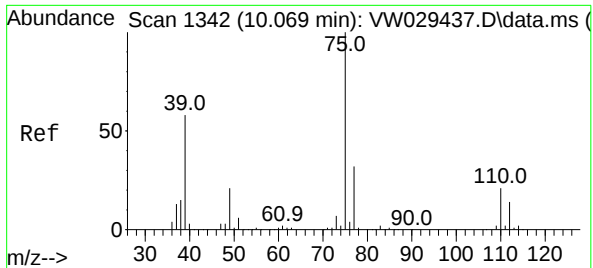

#39
cis-1,3-Dichloropropene
Concen: 0.635 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.037 min
Lab File: VW029438.D
Acq: 02 Jul 2024 12:39

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 3406
Ion Ratio Lower Upper
75 100
77 54.4 22.7 42.1#

