




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029442.D
Acq On : 02 Jul 2024 14:19
Operator : SY/MD
Sample : P3088-14RE
Misc : 4.94g/10mL/MSVOA_W/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4D02RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:43:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

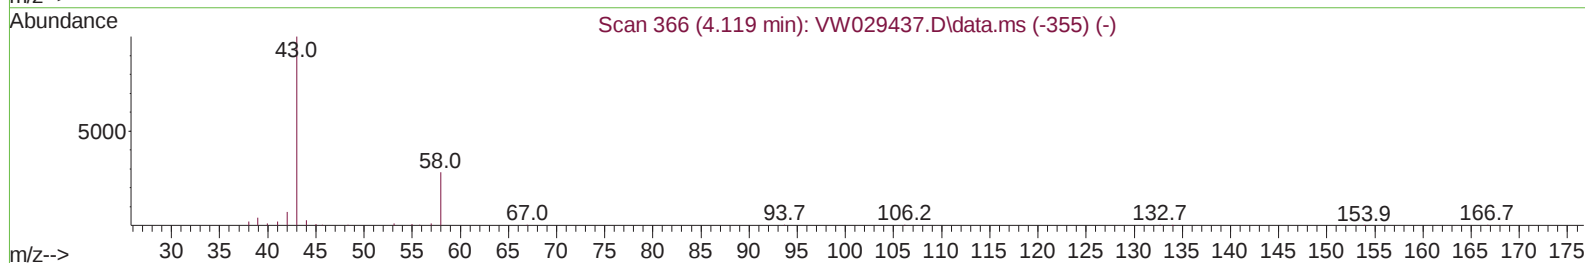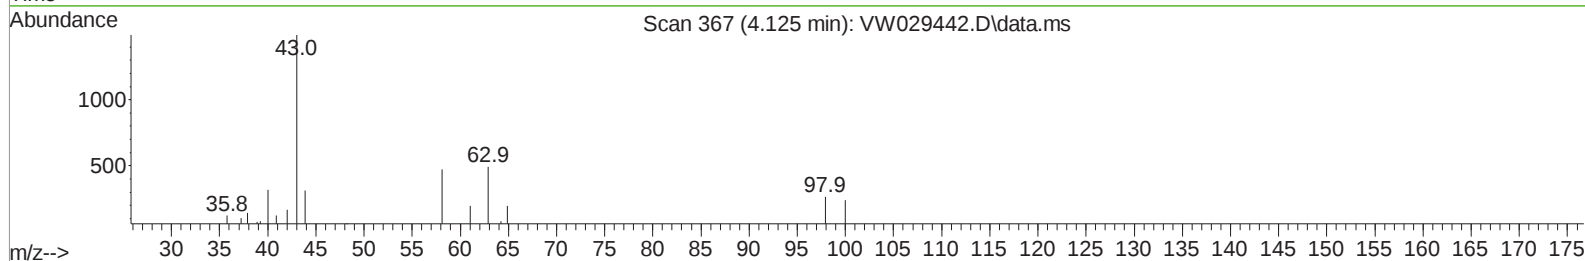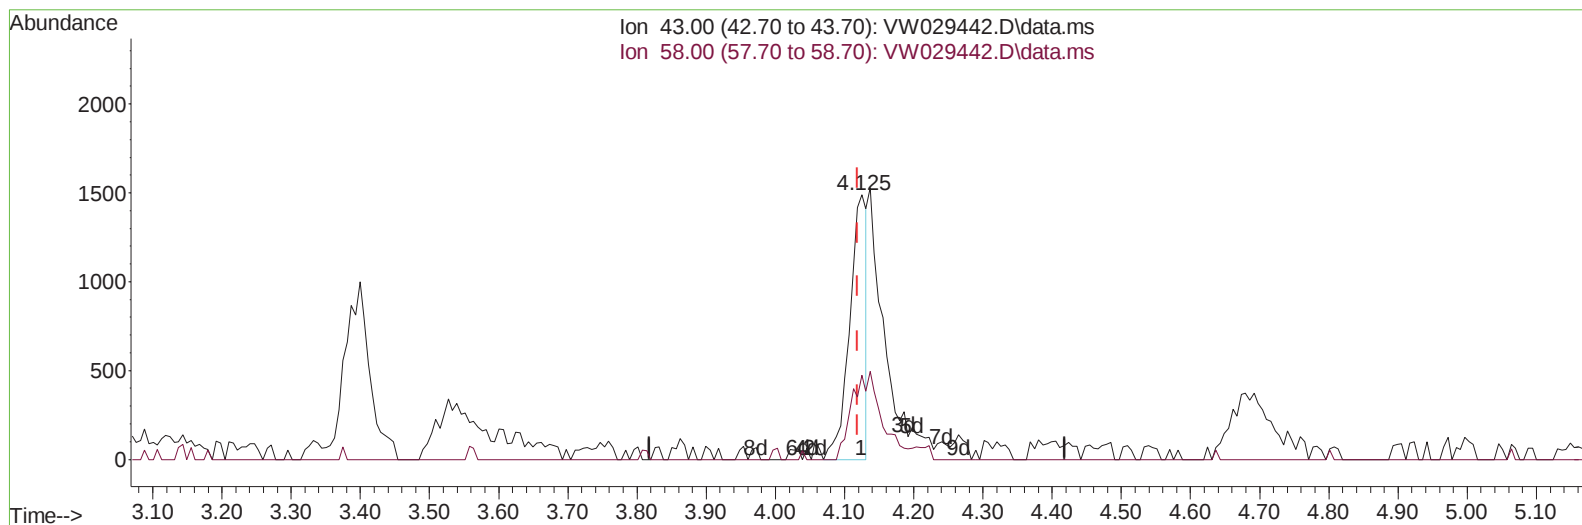

TIC: VW029442.D\data.ms

(13) Acetone (T)

4.125min (+ 0.006) 6.32 ug/L

response 2571

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.70	50.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
 Data File : VW029442.D
 Acq On : 02 Jul 2024 14:19
 Operator : SY/MD
 Sample : P3088-14RE
 Misc : 4.94g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4D02RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:43:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 03 05:41:51 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

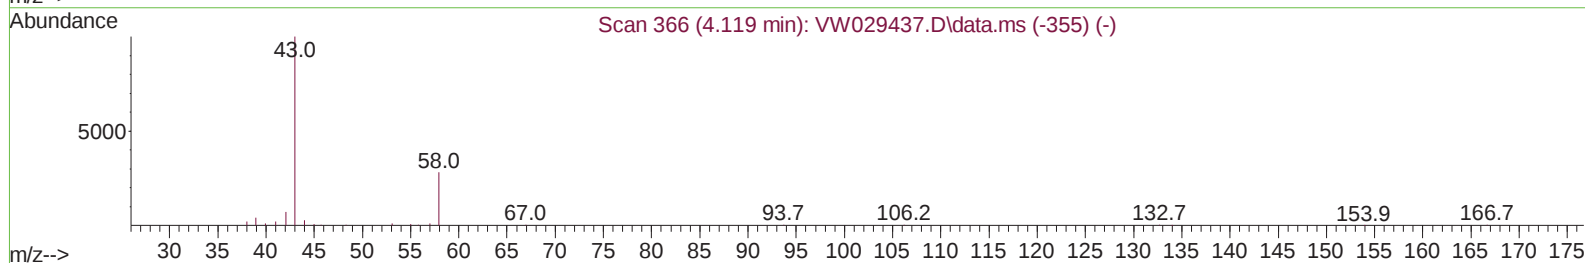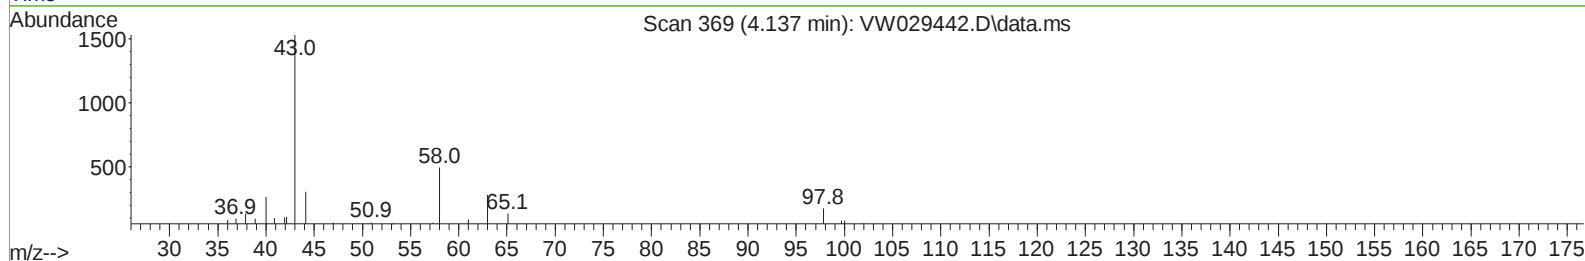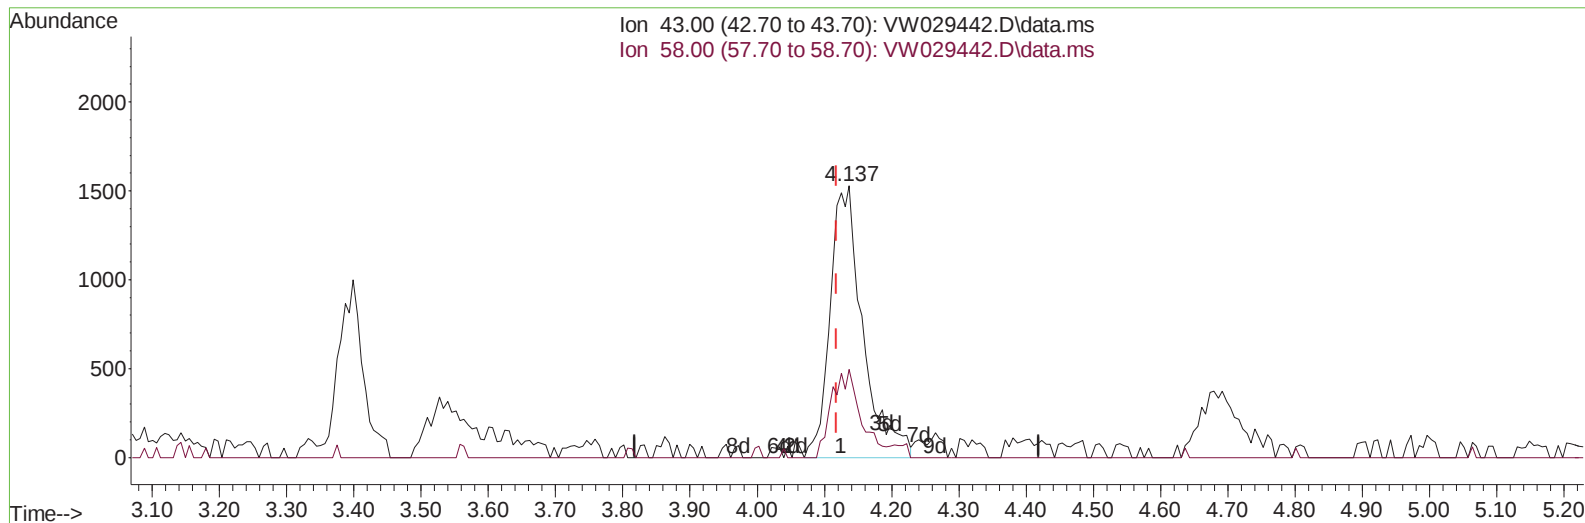

TIC: VW029442.D\data.ms

(13) Acetone (T)

4.137min (+ 0.018) 12.62 ug/L m

response 5135

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.70	25.34
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
 Data File : VW029442.D
 Acq On : 02 Jul 2024 14:19
 Operator : SY/MD
 Sample : P3088-14RE
 Misc : 4.94g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4D02RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:43:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 03 05:41:51 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		115634	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		43424	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		6407	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		69975	43.720	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	174.880%#	
7) Chloroethane-d5	2.899	69		59407	43.954	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	175.800%#	
11) 1,1-Dichloroethene-d2	4.021	65		25974	33.611	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	134.440%#	
21) 2-Butanone-d5	7.081	46		13185	27.535	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	55.060%	
24) Chloroform-d	7.648	84		112547	32.628	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	130.520%	
26) 1,2-Dichloroethane-d4	8.307	65		68892	34.786	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	139.160%#	
32) Benzene-d6	8.276	84		174356	66.105	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	264.400%#	
36) 1,2-Dichloropropane-d6	9.276	67		63279	75.473	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	301.880%#	
41) Toluene-d8	10.319	98		79897	34.238	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	136.960%#	
43) trans-1,3-Dichloroprop...	10.575	79		9670	28.621	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	114.480%	
47) 2-Hexanone-d5	0.000	63		0d	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135		Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		19794	29.663	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	118.640%	
66) 1,2-Dichlorobenzene-d4	13.849	152		5424	24.389	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	97.560%	
Target Compounds							
13) Acetone	4.137	43		5135m	12.619	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029442.D
Acq On : 02 Jul 2024 14:19
Operator : SY/MD
Sample : P3088-14RE
Misc : 4.94g/10mL/MSVOA_W/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4D02RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:43:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

