




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029444.D
Acq On : 02 Jul 2024 15:07
Operator : SY/MD
Sample : P3124-01
Misc : 5.79g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CB3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

Quant Time: Jul 03 05:43:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

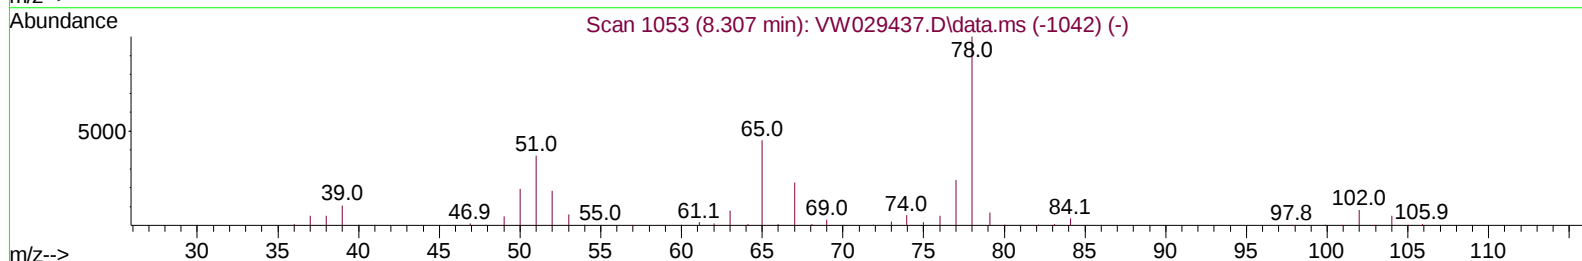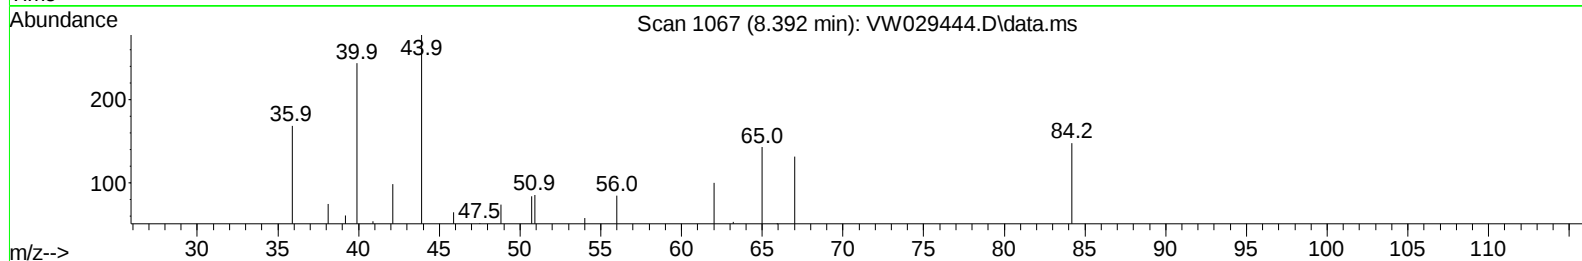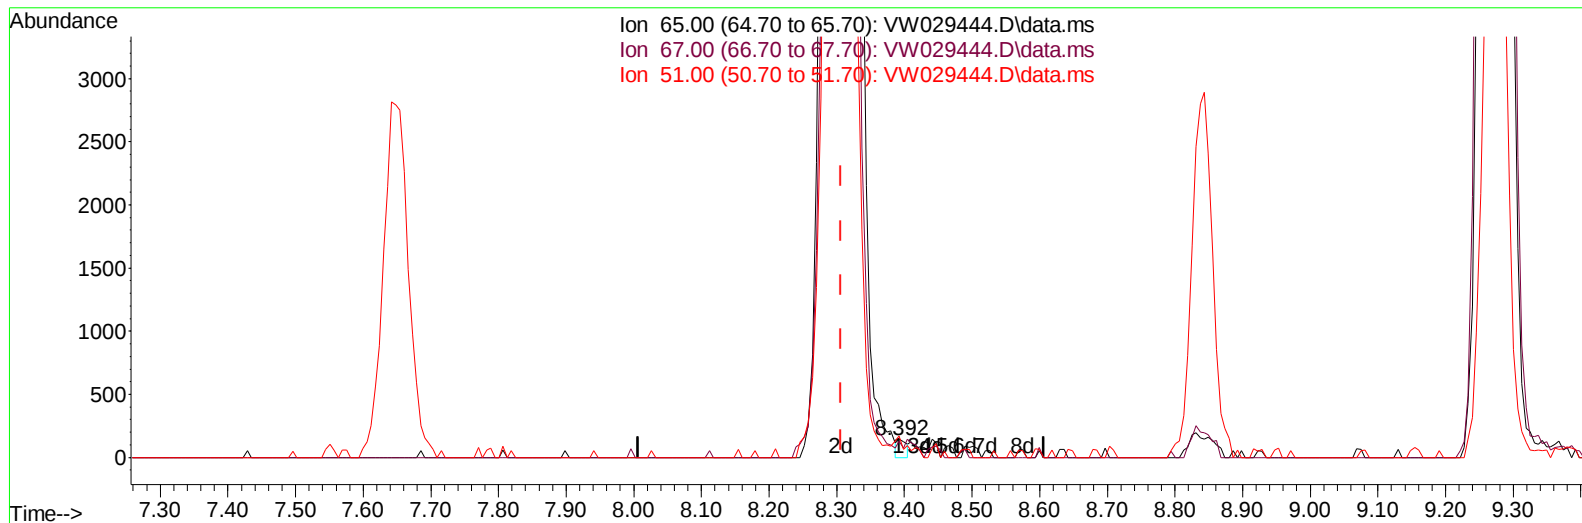

TIC: VW029444.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.392min (+ 0.085) 0.03 ug/L

response 137

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.50	55.47
51.00	99.20	97.08
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
 Data File : VW029444.D
 Acq On : 02 Jul 2024 15:07
 Operator : SY/MD
 Sample : P3124-01
 Misc : 5.79g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CB3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:43:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 03 05:41:51 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

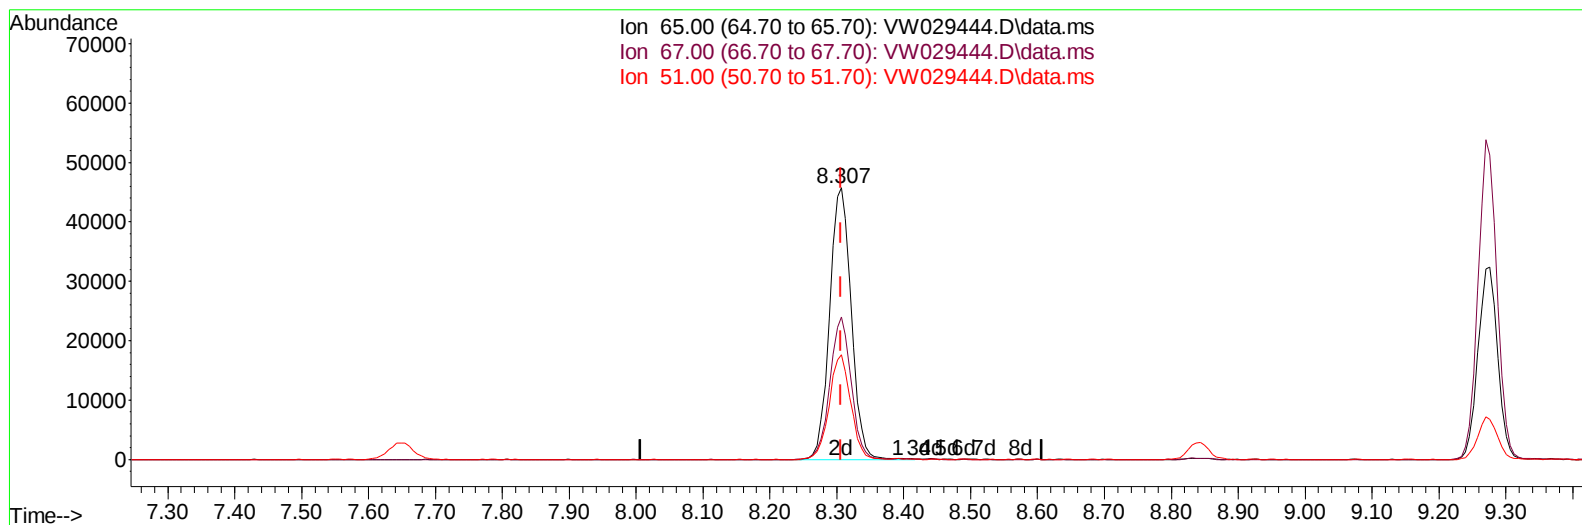

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
 Data File : VW029444.D
 Acq On : 02 Jul 2024 15:07
 Operator : SY/MD
 Sample : P3124-01
 Misc : 5.79g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CB3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:43:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 03 05:41:51 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		253036	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		151529	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		31279	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		81589	23.296	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.200%	
7) Chloroethane-d5	2.899	69		69128	23.373	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.480%	
11) 1,1-Dichloroethene-d2	4.021	65		36381	21.514	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	86.040%	
21) 2-Butanone-d5	7.075	46		38762	36.993	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	73.980%	
24) Chloroform-d	7.648	84		170929	22.645	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	90.600%	
26) 1,2-Dichloroethane-d4	8.307	65		103059m	23.780	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	95.120%	
32) Benzene-d6	8.276	84		311243	33.816	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	135.280%#	
36) 1,2-Dichloropropane-d6	9.270	67		105789	36.158	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	144.640%#	
41) Toluene-d8	10.319	98		206636	25.376	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	101.520%	
43) trans-1,3-Dichloroprop...	10.575	79		23653	20.062	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	80.240%	
47) 2-Hexanone-d5	10.922	63		20353	44.377	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	88.760%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		51710	22.207	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	88.840%	
66) 1,2-Dichlorobenzene-d4	13.848	152		23302	21.462	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	85.840%	
Target Compounds							
13) Acetone	4.125	43		5005	5.621	ug/L	Qvalue 70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029444.D
Acq On : 02 Jul 2024 15:07
Operator : SY/MD
Sample : P3124-01
Misc : 5.79g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CB3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

Quant Time: Jul 03 05:43:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

