




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029455.D
Acq On : 02 Jul 2024 19:30
Operator : SY/MD
Sample : P3100-10
Misc : 4.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BW8

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:46:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

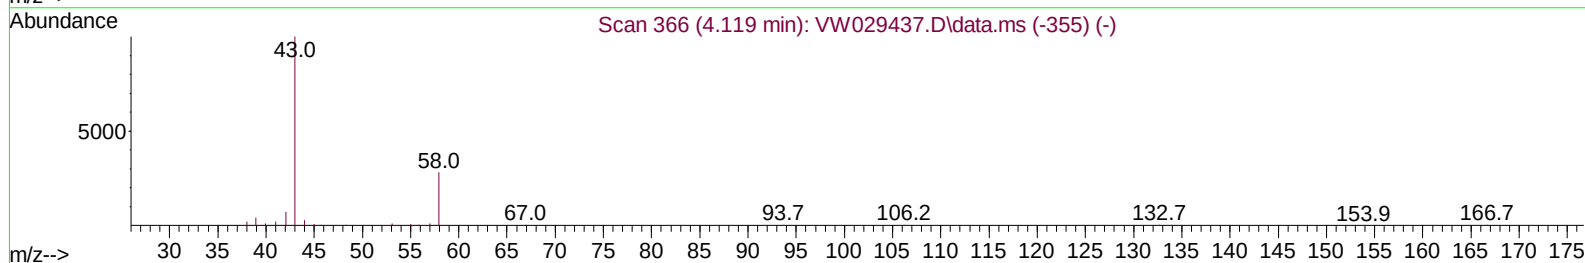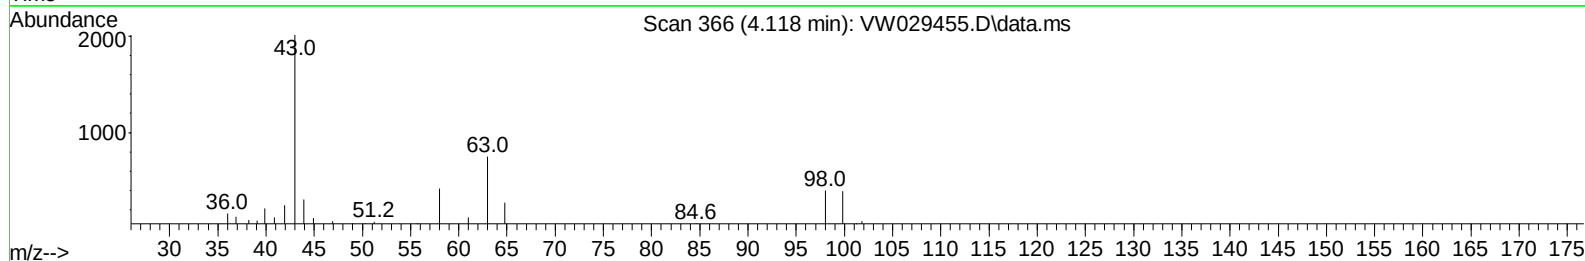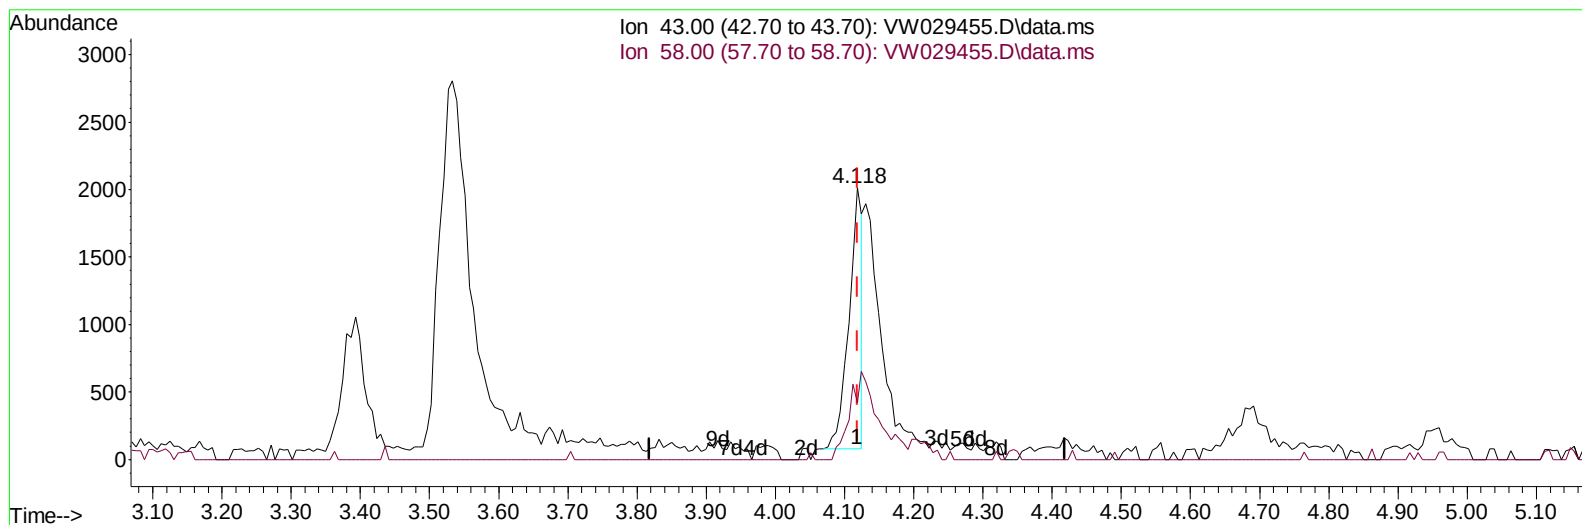

TIC: VW029455.D\data.ms

(13) Acetone (T)

4.118min (-0.000) 2.93 ug/L

response 2615

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.70	64.67#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029455.D
Acq On : 02 Jul 2024 19:30
Operator : SY/MD
Sample : P3100-10
Misc : 4.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BW8

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:46:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

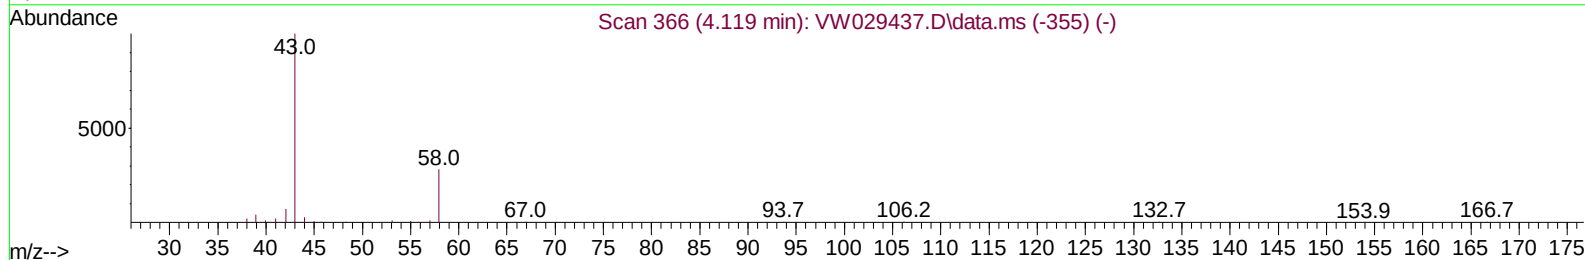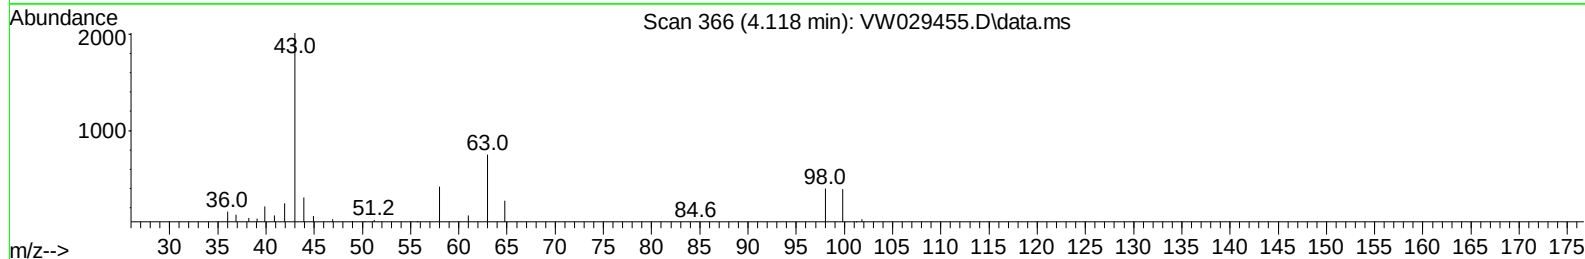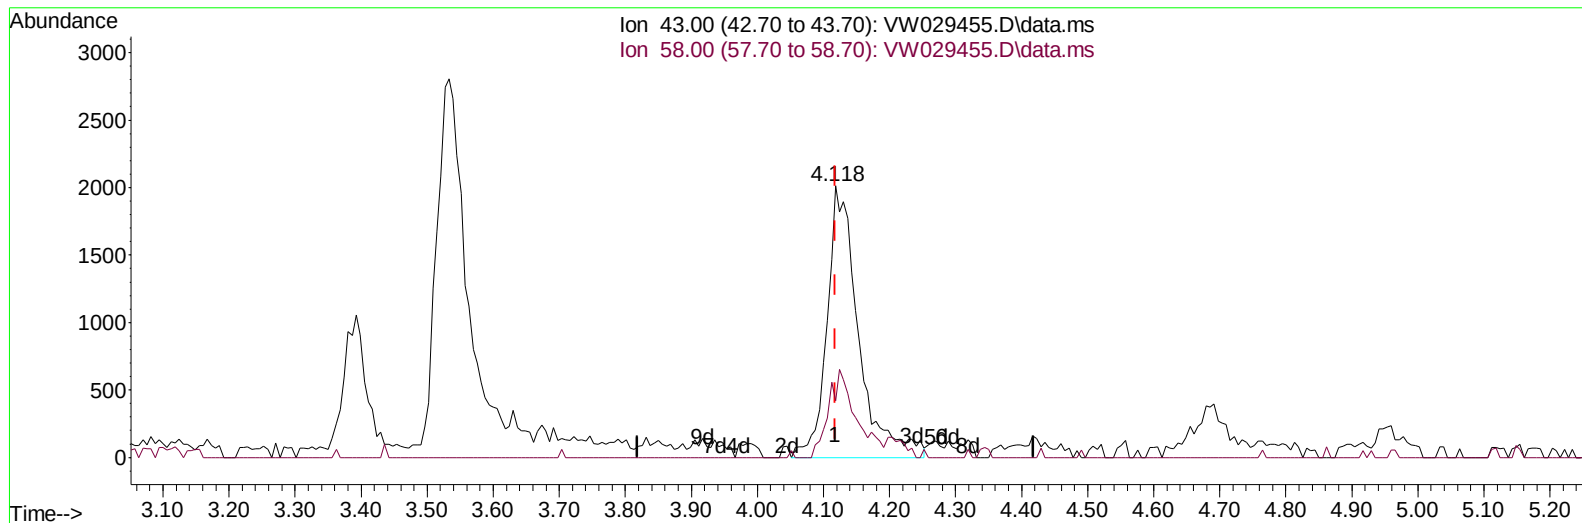

TIC: VW029455.D\data.ms

(13) Acetone (T)

4.118min (-0.000) 7.49 ug/L m

response 6680

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.70	25.31
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
 Data File : VW029455.D
 Acq On : 02 Jul 2024 19:30
 Operator : SY/MD
 Sample : P3100-10
 Misc : 4.68g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BW8

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:46:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 03 05:41:51 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		253546	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		149740	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		32690	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		88135	25.114	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	100.440%	
7) Chloroethane-d5	2.899	69		76514	25.818	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	103.280%	
11) 1,1-Dichloroethene-d2	4.021	65		39941	23.572	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	94.280%	
21) 2-Butanone-d5	7.075	46		37466	35.684	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	71.360%	
24) Chloroform-d	7.648	84		193746	25.616	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	102.480%	
26) 1,2-Dichloroethane-d4	8.300	65		114108	26.277	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	105.120%	
32) Benzene-d6	8.270	84		336600	37.008	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	148.040%#	
36) 1,2-Dichloropropane-d6	9.270	67		117200	40.537	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	162.160%#	
41) Toluene-d8	10.325	98		228395	28.383	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	113.520%	
43) trans-1,3-Dichloroprop...	10.581	79		16726	14.356	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	57.440%	
47) 2-Hexanone-d5	10.922	63		12989	28.659	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	57.320%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		57334	24.916	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	99.680%	
66) 1,2-Dichlorobenzene-d4	13.848	152		26318	23.194	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	92.760%	
Target Compounds							
13) Acetone	4.118	43		6680m	7.486	ug/L	
16) Methylene chloride	4.917	84		18806	4.218	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070224\
Data File : VW029455.D
Acq On : 02 Jul 2024 19:30
Operator : SY/MD
Sample : P3100-10
Misc : 4.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BW8

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:46:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 03 05:41:51 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

