

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070225\
 Data File : VW031750.D
 Acq On : 02 Jul 2025 10:41
 Operator : SY/MD
 Sample : VW0702SBL03
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0702SBL03

Quant Time: Jul 03 06:09:04 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:35:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.959	168	201759	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	378735	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.629	117	338286	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	159858	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	129062	44.574	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	89.140%
35) Dibromofluoromethane	7.898	113	112210	45.403	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	90.800%
50) Toluene-d8	10.325	98	423537	46.051	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	92.100%
62) 4-Bromofluorobenzene	12.617	95	146122	43.173	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	86.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070225\
Data File : VW031750.D
Acq On : 02 Jul 2025 10:41
Operator : SY/MD
Sample : VW0702SBL03
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0702SBL03

Quant Time: Jul 03 06:09:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:35:17 2025
Response via : Initial Calibration




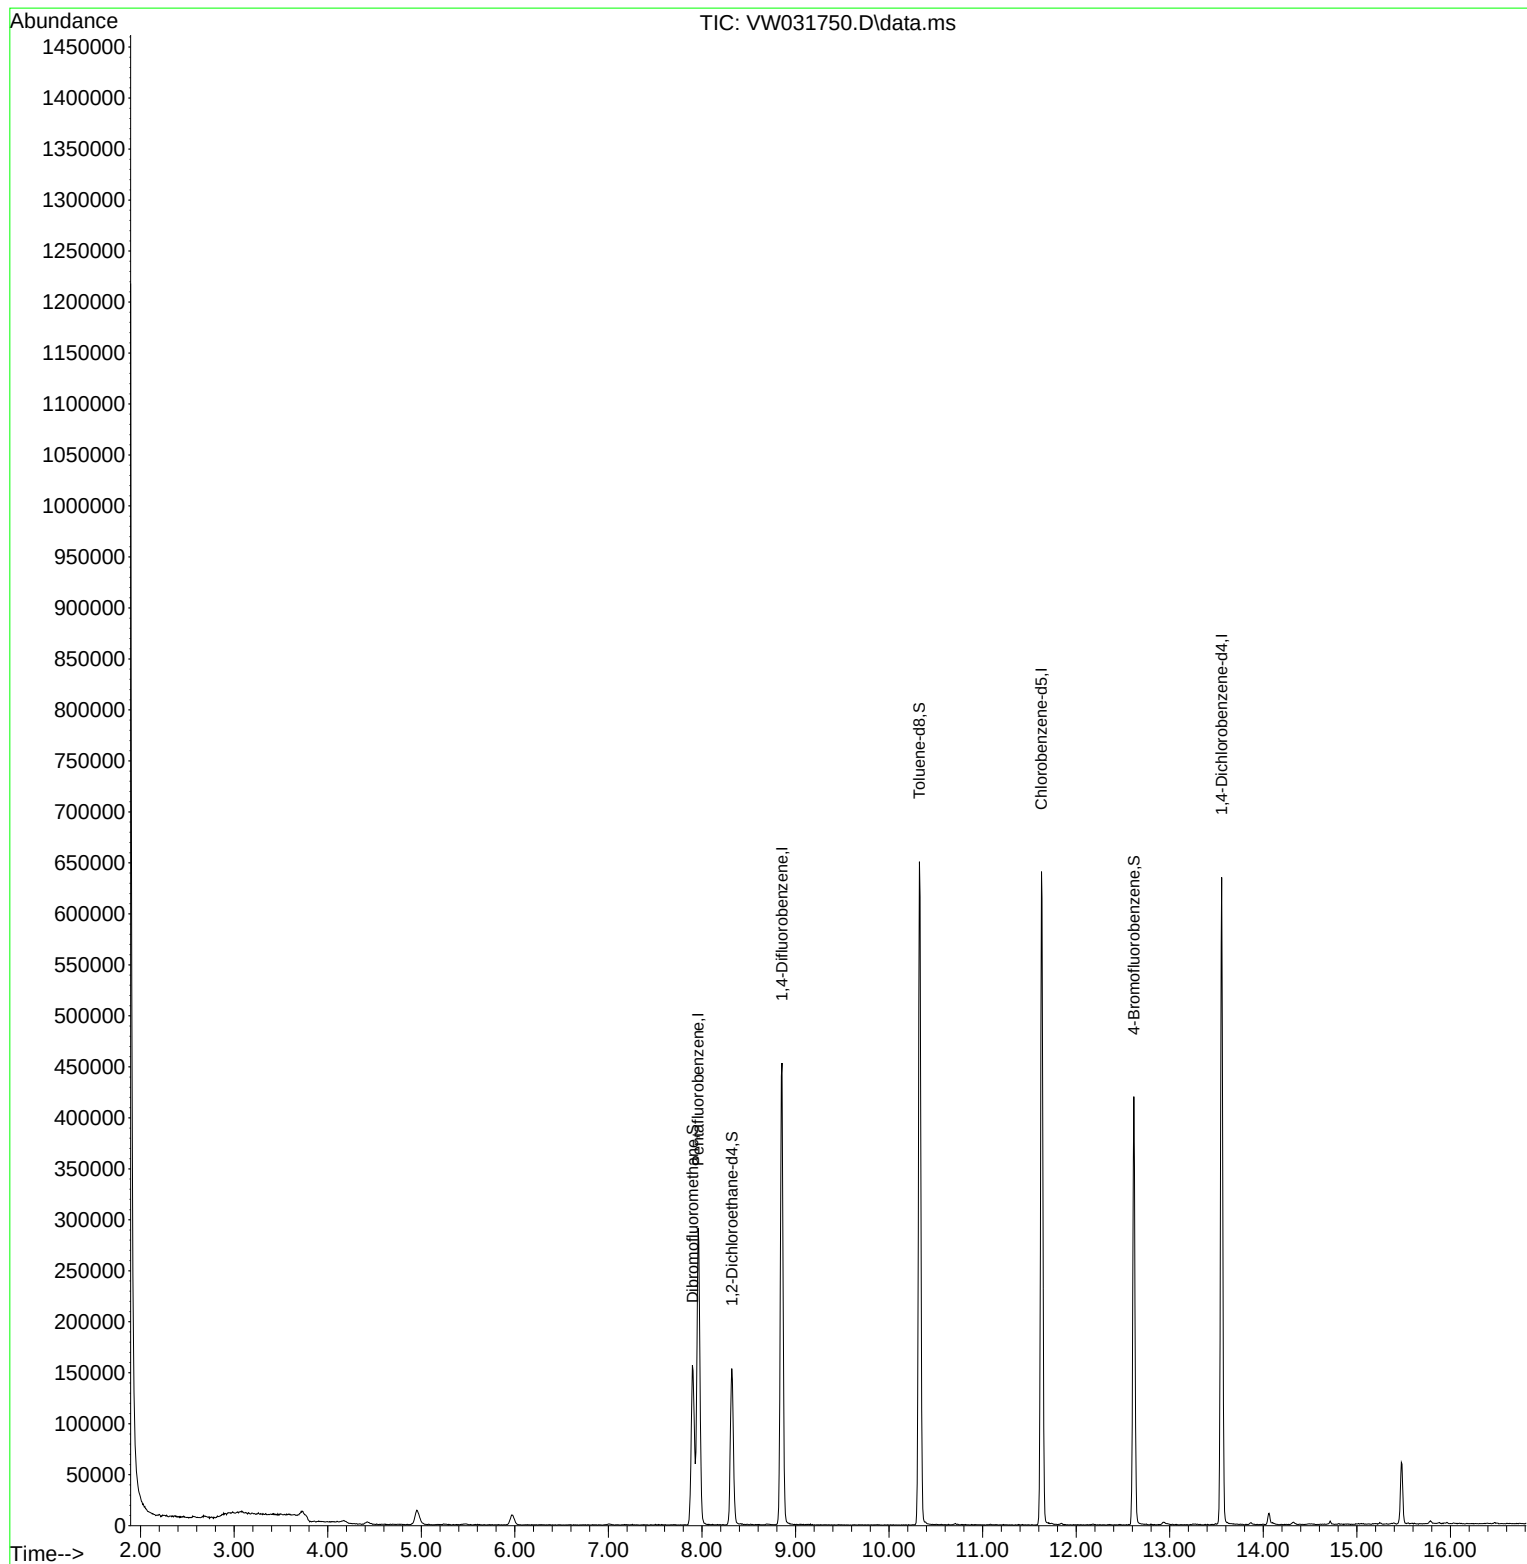


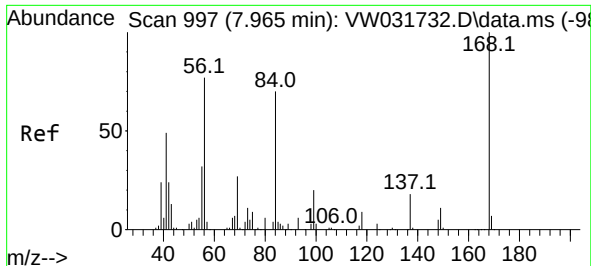

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 997
Delta R.T. -0.006 min
Lab File: VW031750.D
Acq: 02 Jul 2025 10:41




Instrument :
MSVOA_W
ClientSampleId :
VW0702SBL03


Tgt Ion:168 Resp: 201759
Ion Ratio Lower Upper
168 100
99 60.3 49.4 74.2

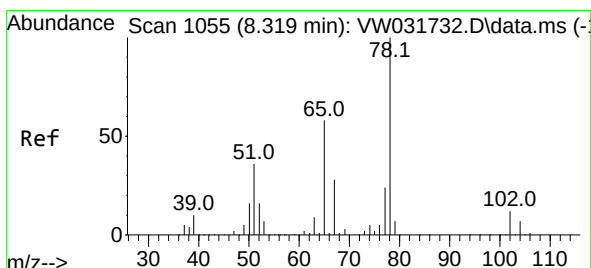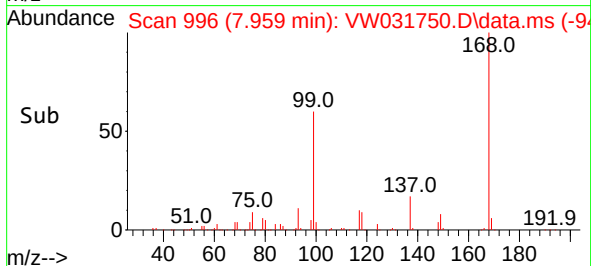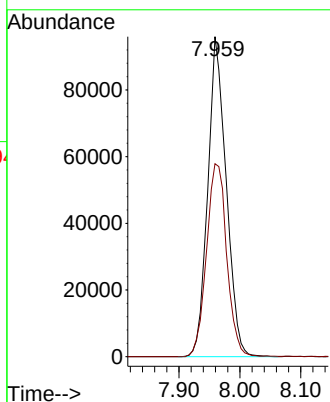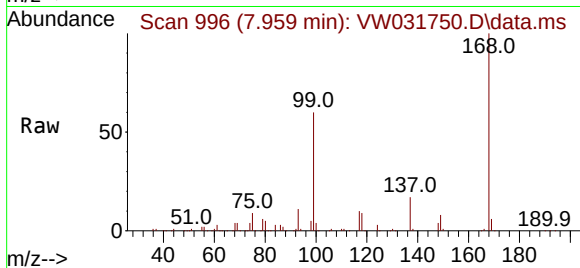

#33
1,2-Dichloroethane-d4
Concen: 44.574 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW031750.D
Acq: 02 Jul 2025 10:41

Tgt Ion: 65 Resp: 129062
Ion Ratio Lower Upper
65 100
67 50.3 0.0 99.4

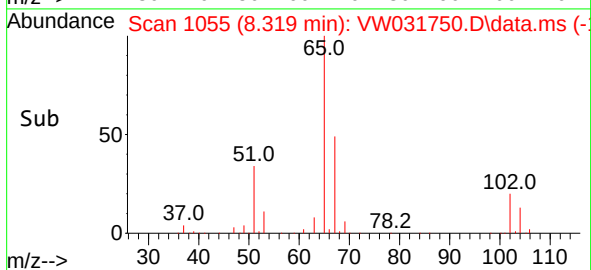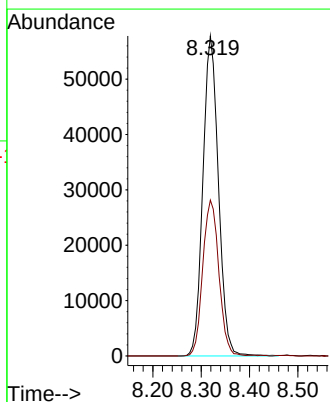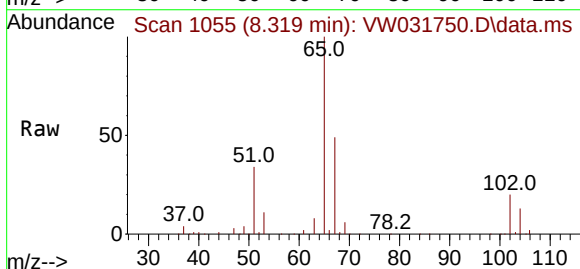

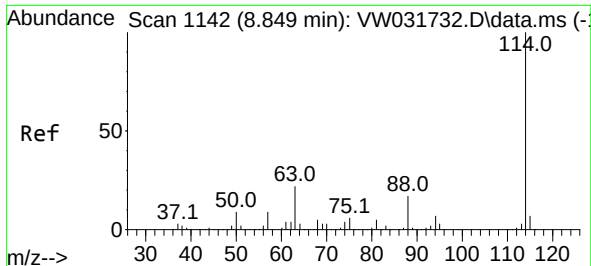

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1143

Delta R.T. 0.006 min

Lab File: VW031750.D

Acq: 02 Jul 2025 10:41

Instrument :

MSVOA_W

ClientSampleId :

VW0702SBL03





Tgt Ion:114 Resp: 378735

Ion Ratio Lower Upper

114 100

63 20.2 0.0 43.6

88 16.3 0.0 34.2

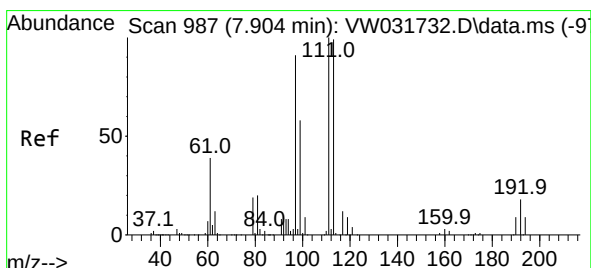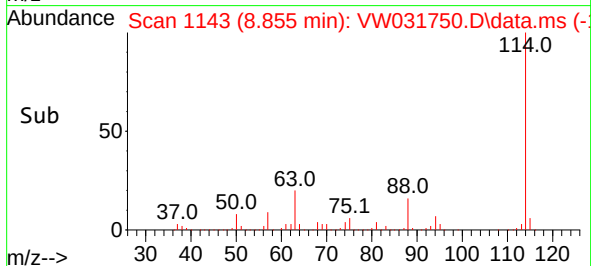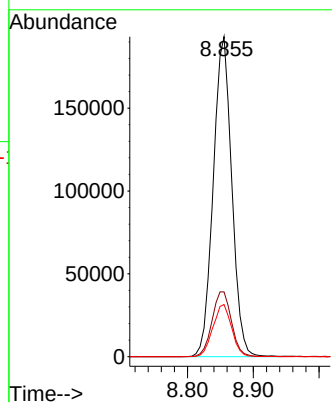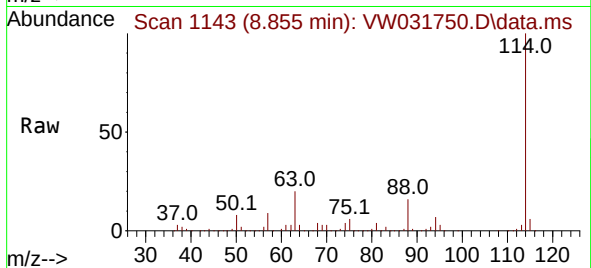

#35

Dibromofluoromethane

Concen: 45.403 ug/l

RT: 7.898 min Scan# 986

Delta R.T. -0.006 min

Lab File: VW031750.D

Acq: 02 Jul 2025 10:41




Tgt Ion:113 Resp: 112210


Ion Ratio Lower Upper

113 100

111 105.7 82.1 123.1

192 16.4 13.8 20.6


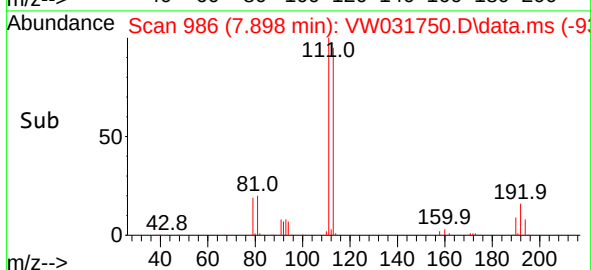
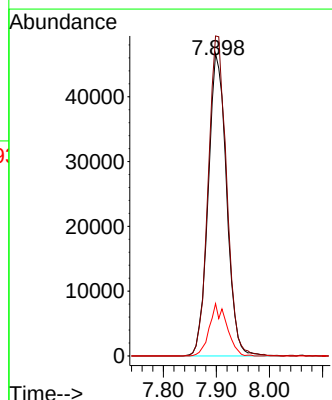
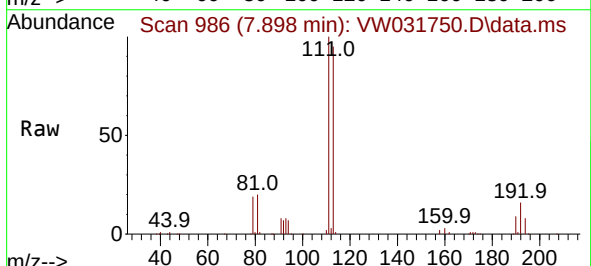


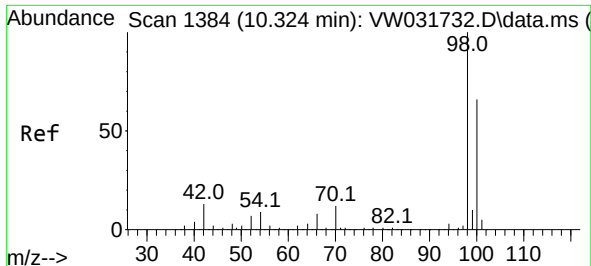

#50
Toluene-d8
Concen: 46.051 ug/l
RT: 10.325 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW031750.D
Acq: 02 Jul 2025 10:41




Instrument :
MSVOA_W
ClientSampleId :
VW0702SBL03


Tgt Ion: 98 Resp: 423537
Ion Ratio Lower Upper
98 100
100 66.2 53.0 79.4

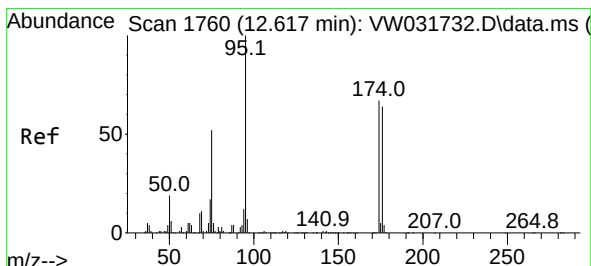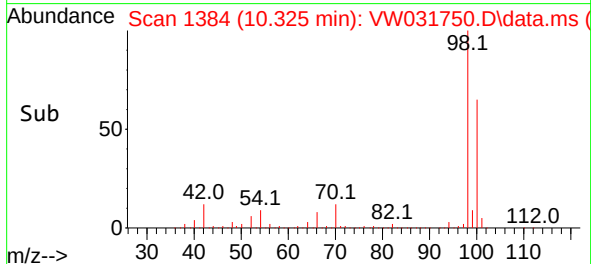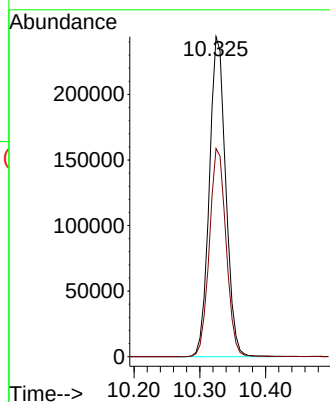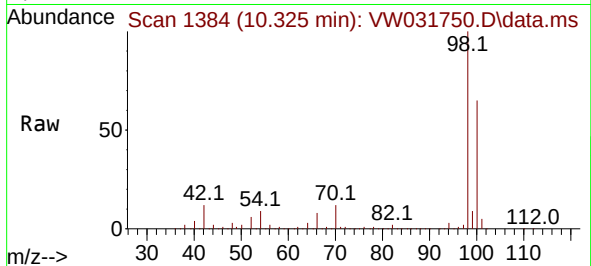

#62
4-Bromofluorobenzene
Concen: 43.173 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW031750.D
Acq: 02 Jul 2025 10:41

Tgt Ion: 95 Resp: 146122
Ion Ratio Lower Upper
95 100
174 65.3 0.0 133.8
176 63.9 0.0 126.0


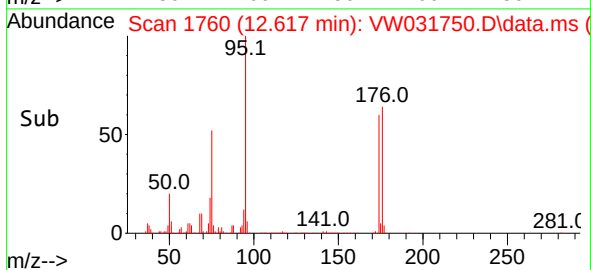
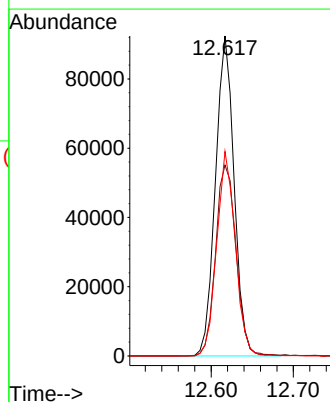
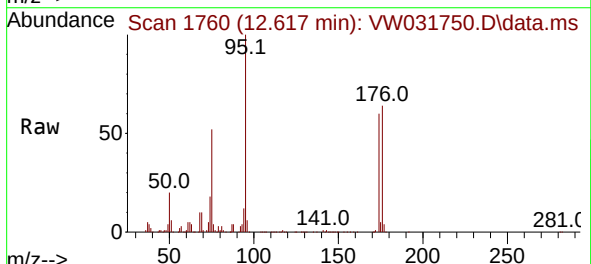


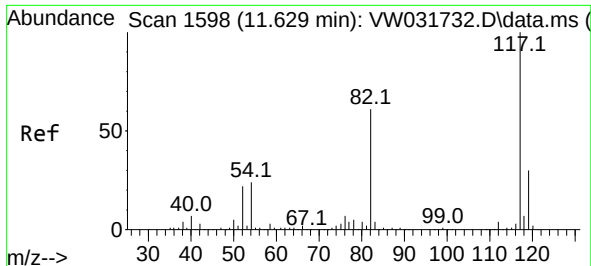

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.629 min Scan# 117
Delta R.T. 0.000 min
Lab File: VW031750.D
Acq: 02 Jul 2025 10:41

Instrument :
MSVOA_W
ClientSampleId :
VW0702SBL03

Tgt Ion:117 Resp: 338286
Ion Ratio Lower Upper
117 100
82 58.7 48.6 72.8
119 30.1 23.9 35.9

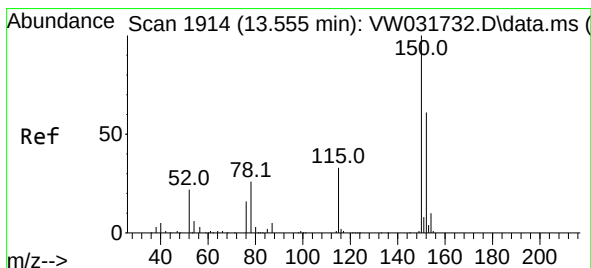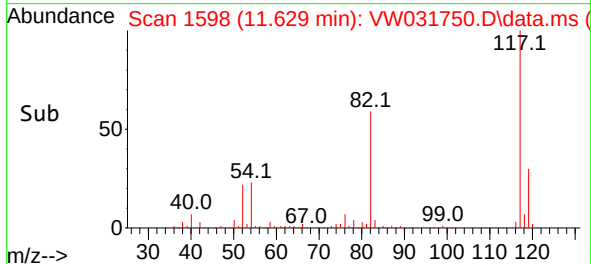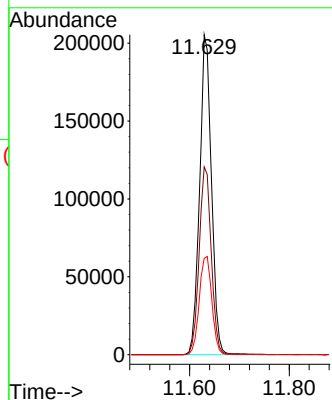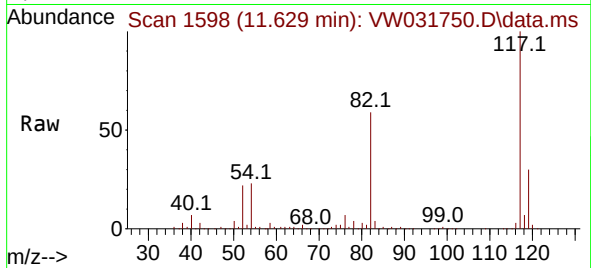

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. 0.000 min
Lab File: VW031750.D
Acq: 02 Jul 2025 10:41

Tgt Ion:152 Resp: 159858
Ion Ratio Lower Upper
152 100
115 63.0 31.9 95.7
150 154.1 0.0 356.4

