

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070524\
 Data File : VW029464.D
 Acq On : 05 Jul 2024 11:09
 Operator : SY/MD
 Sample : P3080-13
 Misc : 5.10g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 06 00:23:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 06 00:21:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	222538	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	217917	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	97149	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	55988	18.177	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.720%
7) Chloroethane-d5	2.899	69	51751	19.896	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.600%
11) 1,1-Dichloroethene-d2	4.021	65	30885	20.767	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.080%
21) 2-Butanone-d5	7.081	46	63454	68.857	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.720%#
24) Chloroform-d	7.648	84	165600	24.946	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	8.307	65	100475	26.361	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.440%
32) Benzene-d6	8.276	84	304719	23.021	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.080%
36) 1,2-Dichloropropane-d6	9.276	67	104417	24.817	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.280%
41) Toluene-d8	10.325	98	265718	22.690	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.760%
43) trans-1,3-Dichloroprop...	10.581	79	39892	23.528	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.120%
47) 2-Hexanone-d5	10.922	63	41673	63.181	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.360%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	95940	28.650	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	96511	28.620	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.480%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3101	0.596	ug/L	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070524\
Data File : VW029464.D
Acq On : 05 Jul 2024 11:09
Operator : SY/MD
Sample : P3080-13
Misc : 5.10g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jul 06 00:23:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 06 00:21:19 2024
Response via : Initial Calibration

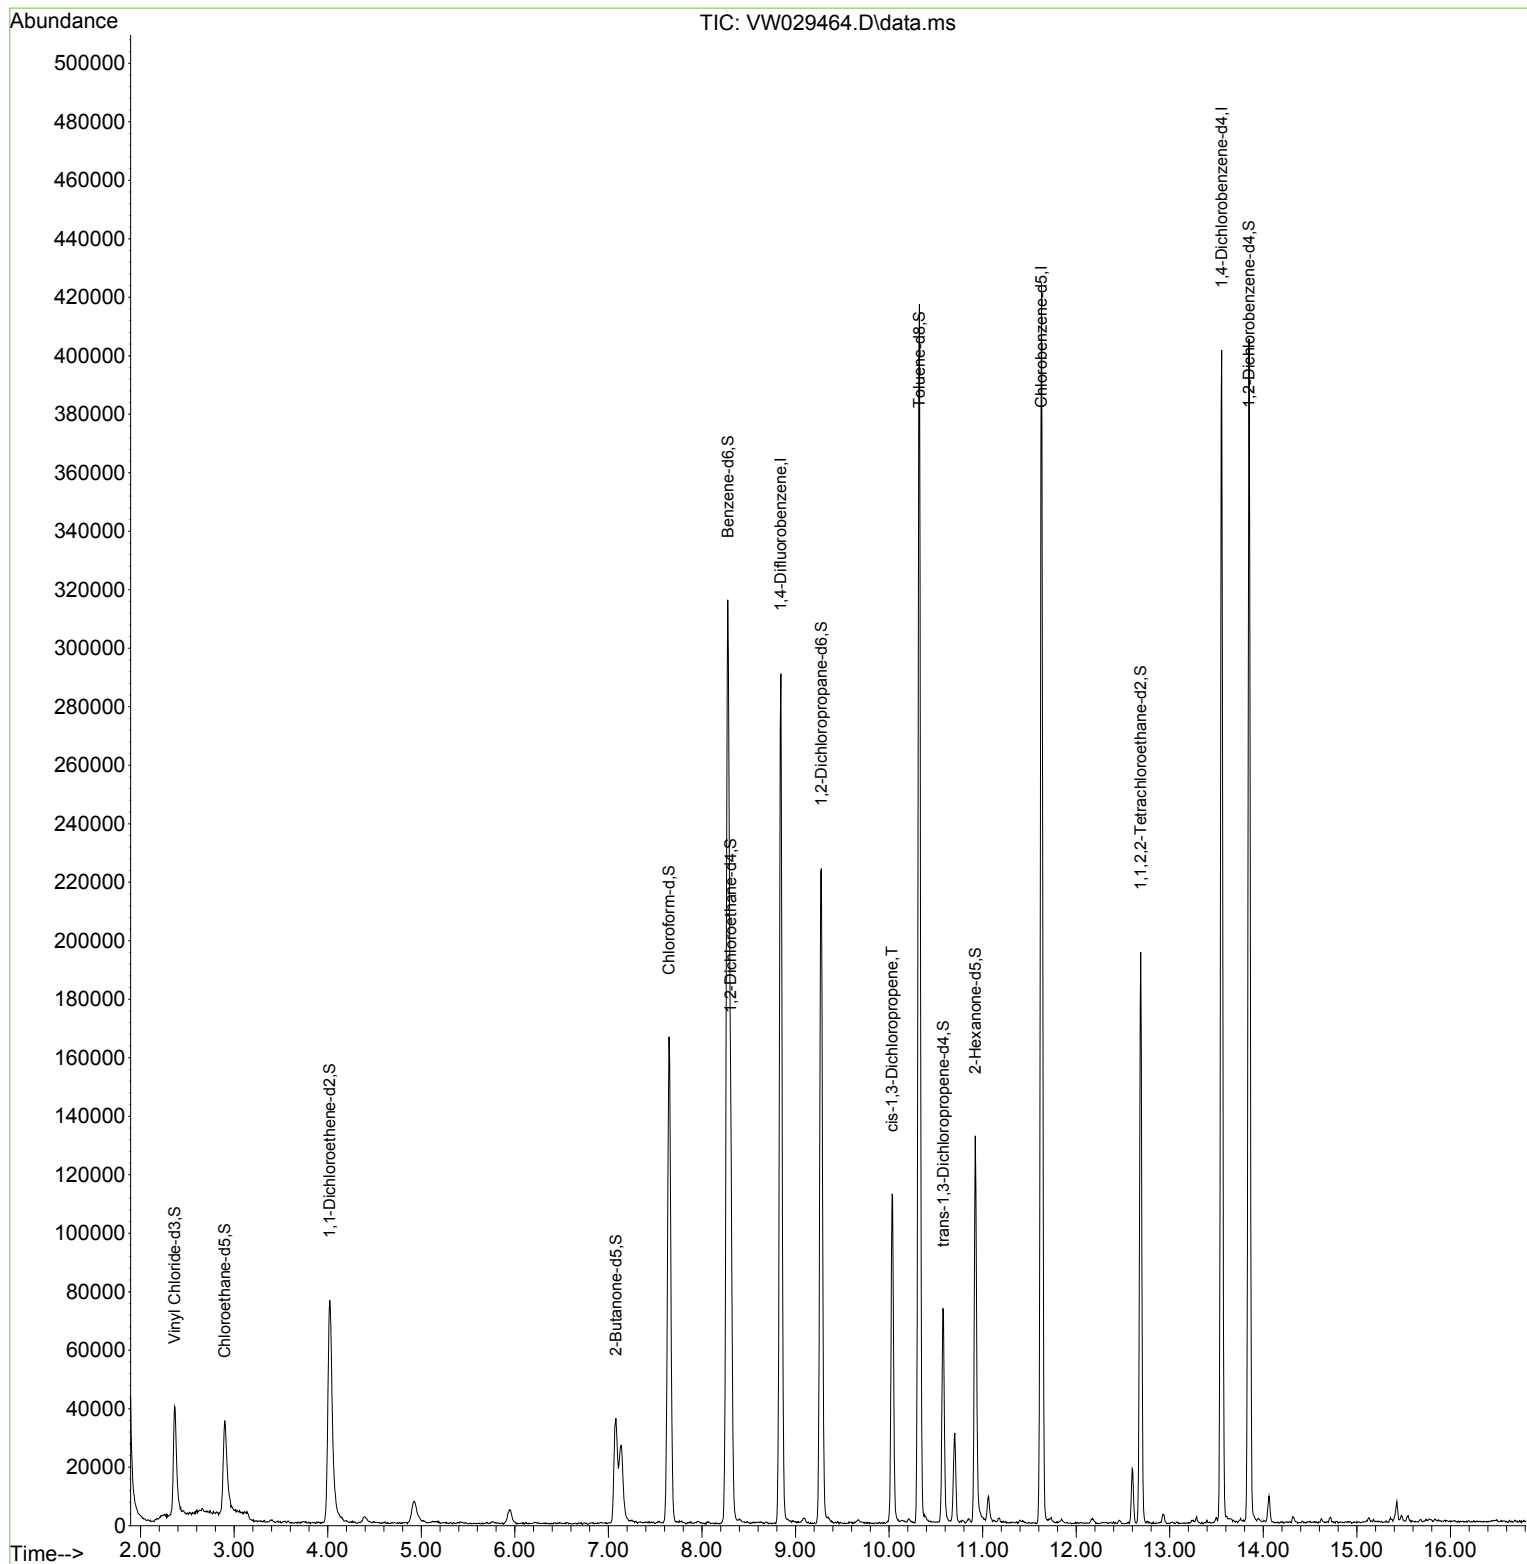

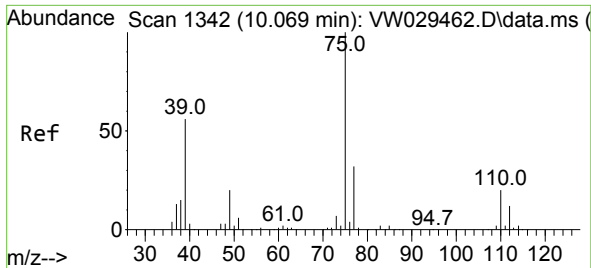

#39
 cis-1,3-Dichloropropene
 Concen: 0.596 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW029464.D
 Acq: 05 Jul 2024 11:09

Instrument :
 MSVOA_W
 ClientSampleId :

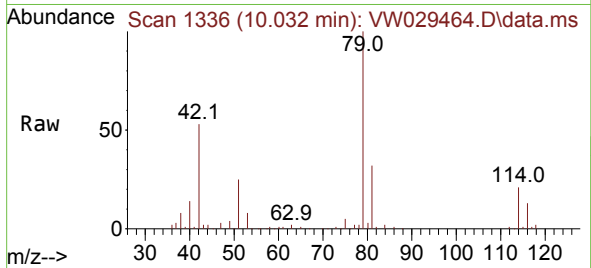

Tgt Ion: 75 Resp: 3101
 Ion Ratio Lower Upper
 75 100
 77 43.7 22.7 42.1#

