

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070524\
 Data File : VW029466.D
 Acq On : 05 Jul 2024 11:55
 Operator : SY/MD
 Sample : P3139-05
 Misc : 5.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 06 00:23:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 06 00:21:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	249871	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	238143	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	106410	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	54318	15.706	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	62.840%		
7) Chloroethane-d5	2.899	69	48556	16.625	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.520%		
11) 1,1-Dichloroethene-d2	4.021	65	28811	17.253	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	69.000%		
21) 2-Butanone-d5	7.075	46	55916	54.039	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.080%		
24) Chloroform-d	7.654	84	152912	20.515	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.040%		
26) 1,2-Dichloroethane-d4	8.307	65	92624	21.643	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	86.560%		
32) Benzene-d6	8.276	84	286404	19.800	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	79.200%		
36) 1,2-Dichloropropane-d6	9.276	67	96923	21.079	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.320%		
41) Toluene-d8	10.325	98	247197	19.316	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.280%		
43) trans-1,3-Dichloroprop...	10.575	79	36610	19.758	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.040%		
47) 2-Hexanone-d5	10.922	63	36674	50.879	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.760%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	84528	23.098	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	92.400%		
66) 1,2-Dichlorobenzene-d4	13.848	152	91116	24.669	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.680%		
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	11291	2.570	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070524\
Data File : VW029466.D
Acq On : 05 Jul 2024 11:55
Operator : SY/MD
Sample : P3139-05
Misc : 5.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001


Quant Time: Jul 06 00:23:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 06 00:21:19 2024
Response via : Initial Calibration

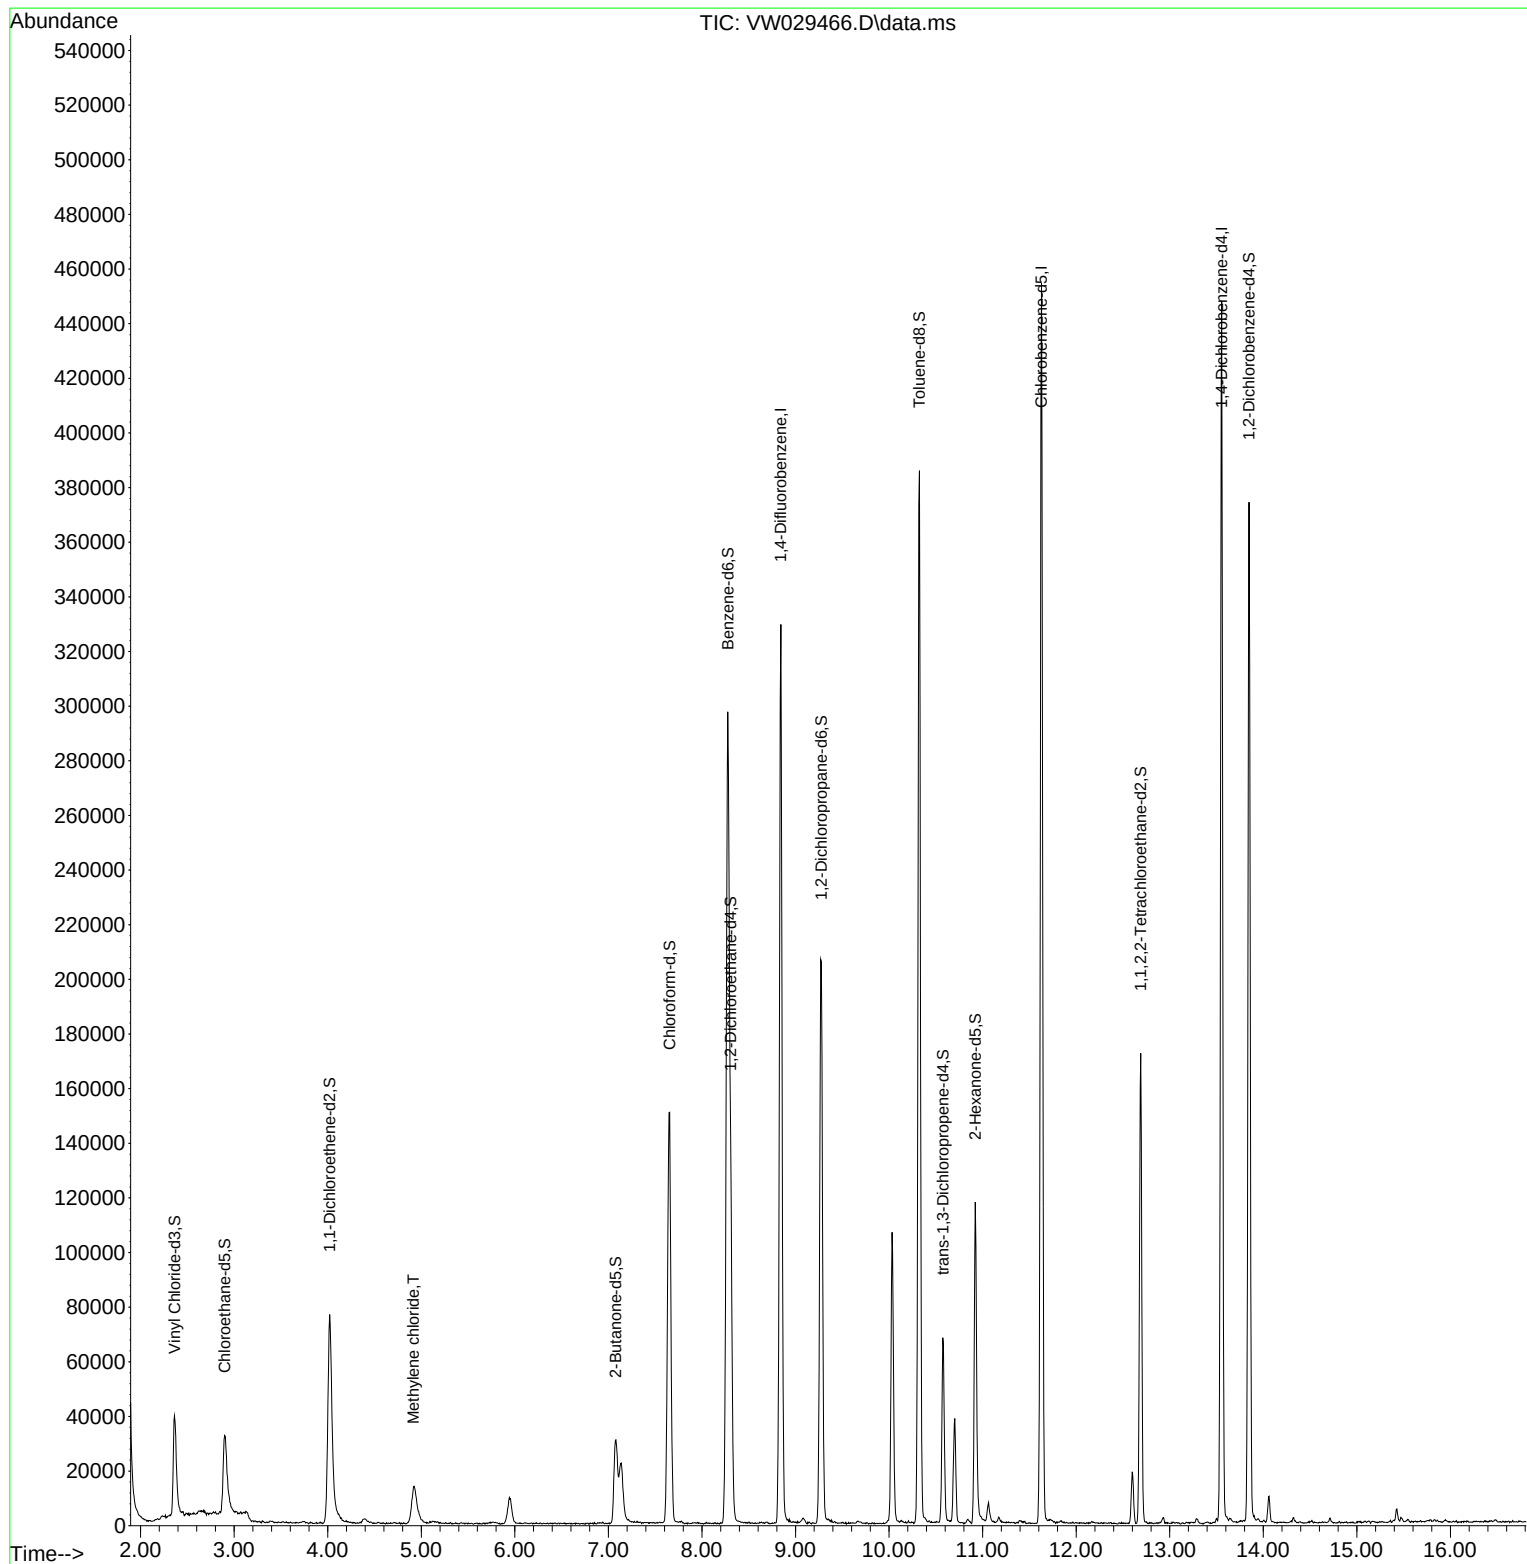

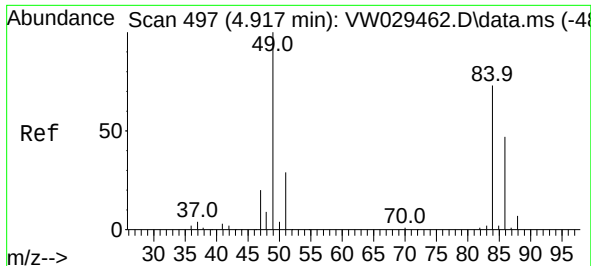

#16
Methylene chloride
Concen: 2.570 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW029466.D
Acq: 05 Jul 2024 11:55

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

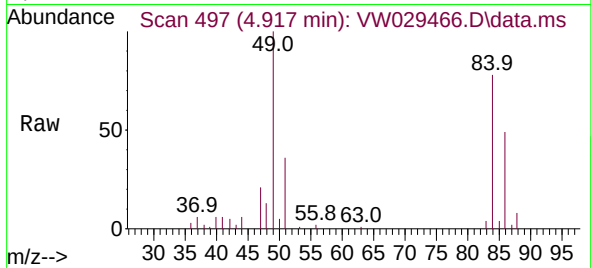

Tgt Ion:	84	Resp:	11291
Ion	Ratio	Lower	Upper
84	100		
86	63.3	41.4	77.0
49	128.4	95.7	177.7

