

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070524\
 Data File : VW029470.D
 Acq On : 05 Jul 2024 13:31
 Operator : SY/MD
 Sample : VIBLK493
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK493

Quant Time: Jul 06 00:24:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 06 00:21:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	243082	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	232187	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	105331	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	53834	16.000	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.000%
7) Chloroethane-d5	2.893	69	49779	17.520	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.080%
11) 1,1-Dichloroethene-d2	4.021	65	29843	18.371	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.480%
21) 2-Butanone-d5	7.075	46	66766	66.327	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	132.660%
24) Chloroform-d	7.648	84	167154	23.052	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.200%
26) 1,2-Dichloroethane-d4	8.306	65	102092	24.522	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.080%
32) Benzene-d6	8.276	84	309553	21.949	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	9.270	67	106956	23.858	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.440%
41) Toluene-d8	10.324	98	267061	21.403	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	10.580	79	41256	22.837	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.360%
47) 2-Hexanone-d5	10.922	63	44261	62.980	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.960%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	100606	28.197	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.800%
66) 1,2-Dichlorobenzene-d4	13.854	152	96658	26.437	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.760%
Target Compounds						
16) Methylene chloride	4.917	84	16957	3.967	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070524\
Data File : VW029470.D
Acq On : 05 Jul 2024 13:31
Operator : SY/MD
Sample : VIBLK493
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK493

Quant Time: Jul 06 00:24:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 06 00:21:19 2024
Response via : Initial Calibration

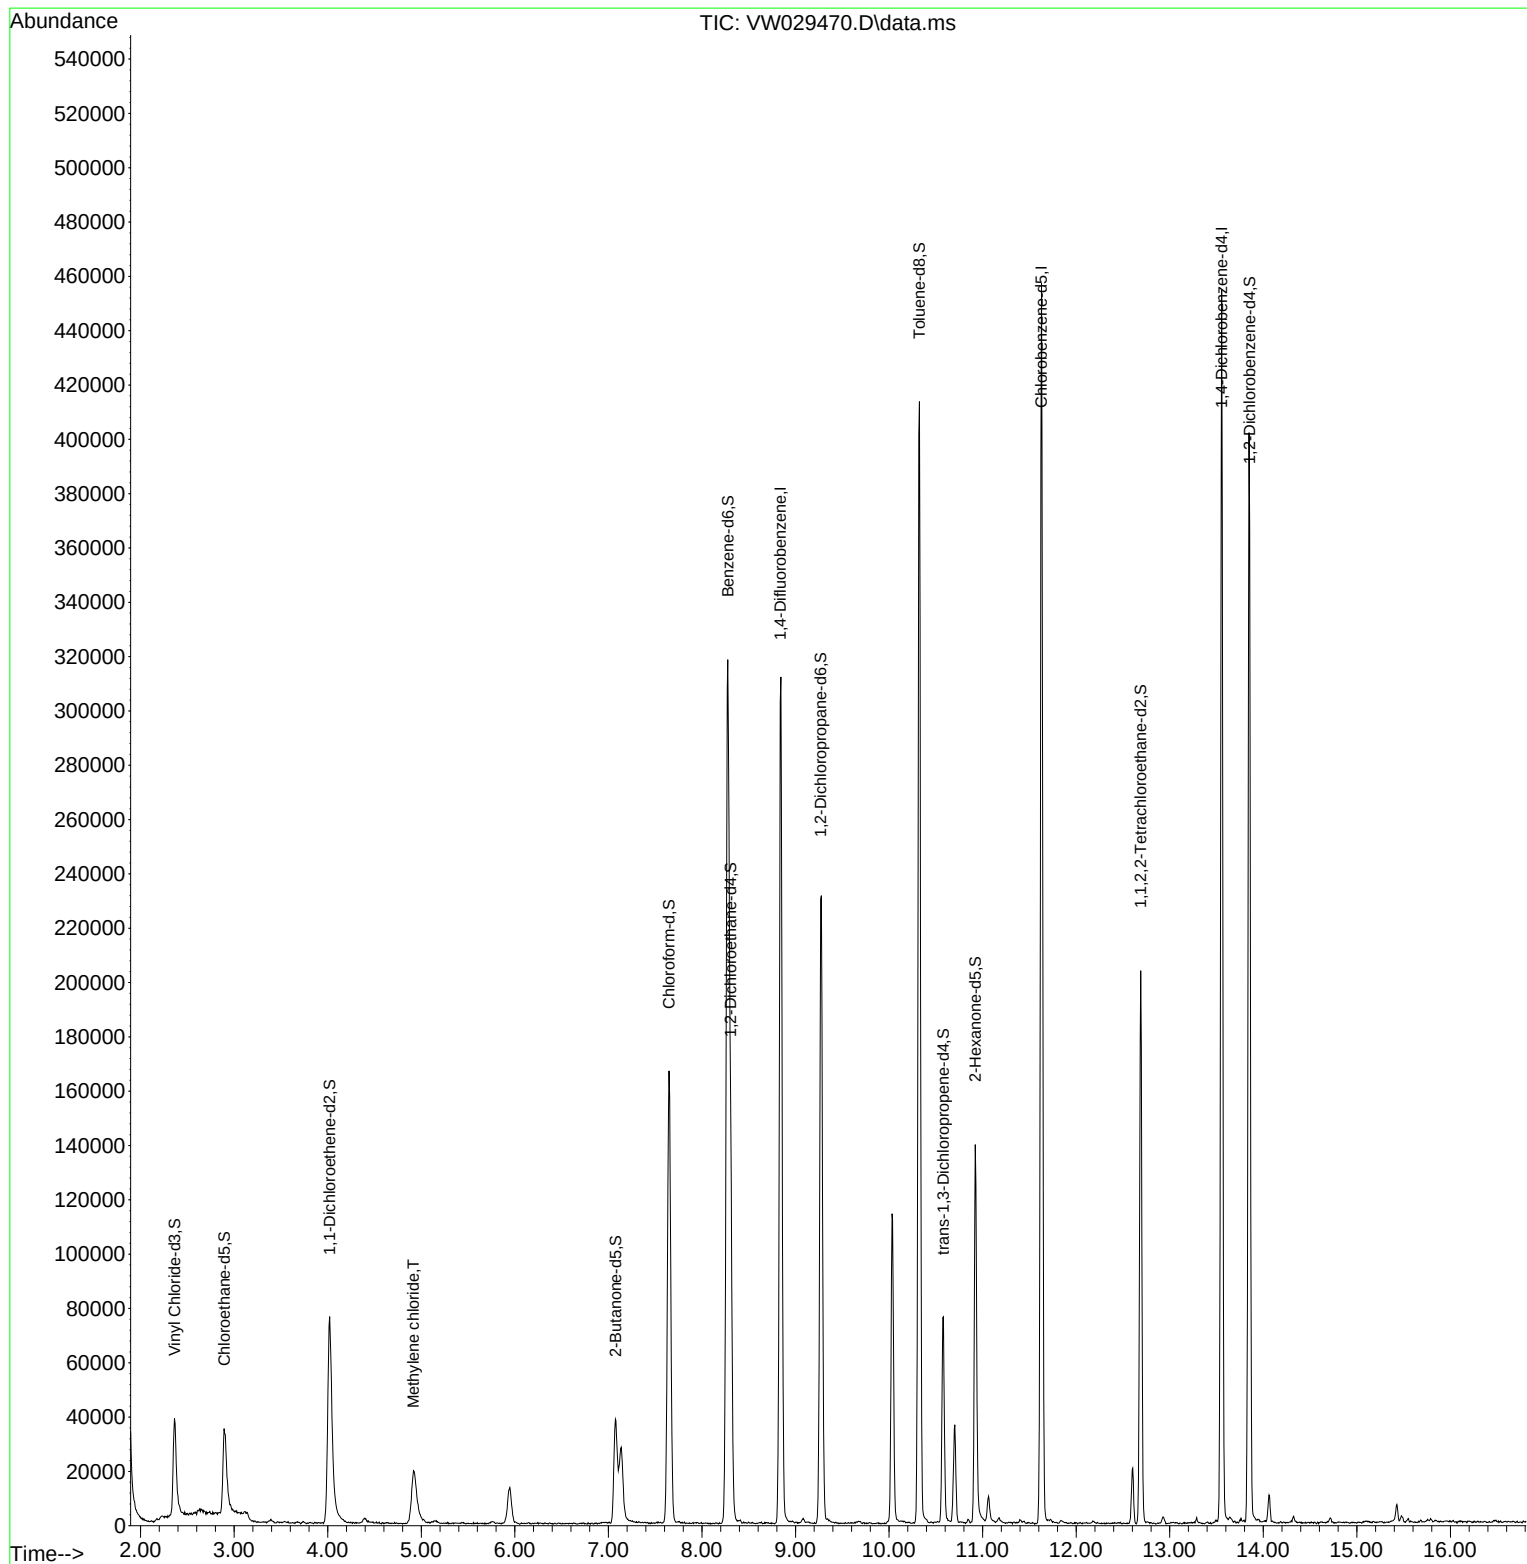

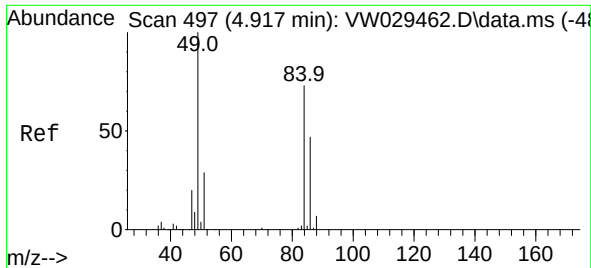

#16
Methylene chloride
Concen: 3.967 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW029470.D
Acq: 05 Jul 2024 13:31

Instrument :
MSVOA_W
ClientSampleId :
VIBLK493

Tgt Ion: 84 Resp: 16957
Ion Ratio Lower Upper
84 100
86 67.9 41.4 77.0
49 144.8 95.7 177.7

