

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070623\
Data File : VW026552.D
Acq On : 06 Jul 2023 19:19
Operator : SY/MD
Sample : 03534-20
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4739




Manual IntegrationsAPPROVED

Reviewed By :John
Carlone
07/07/2023

Supervised By :Semsetun
Yesilyurt

07/07/2023

Quant Time: Jul 07 02:36:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 04 13:17:14 2023
Response via : Initial Calibration

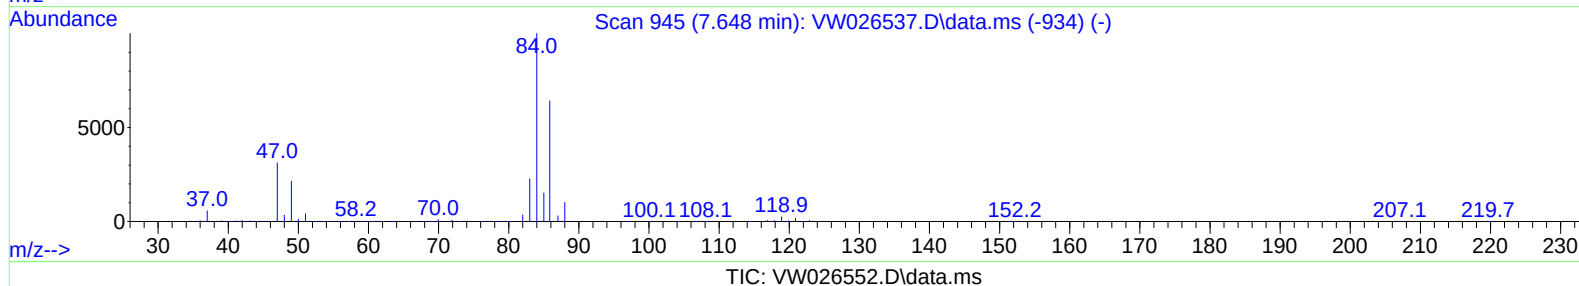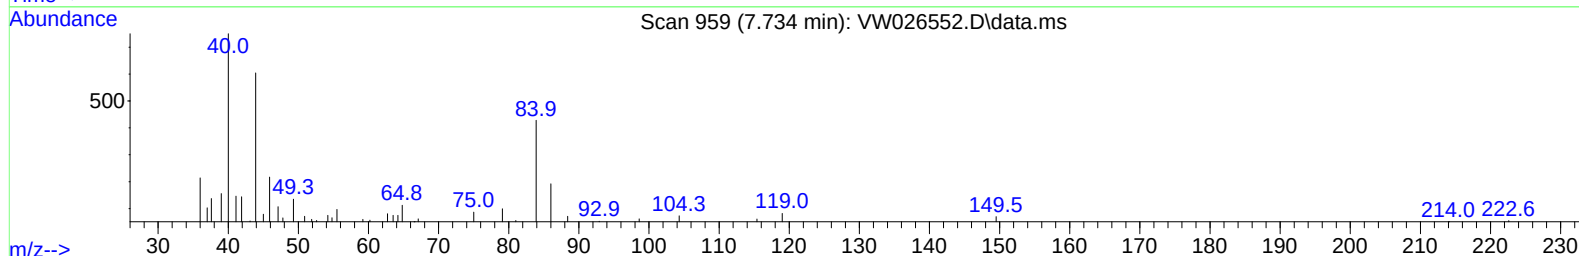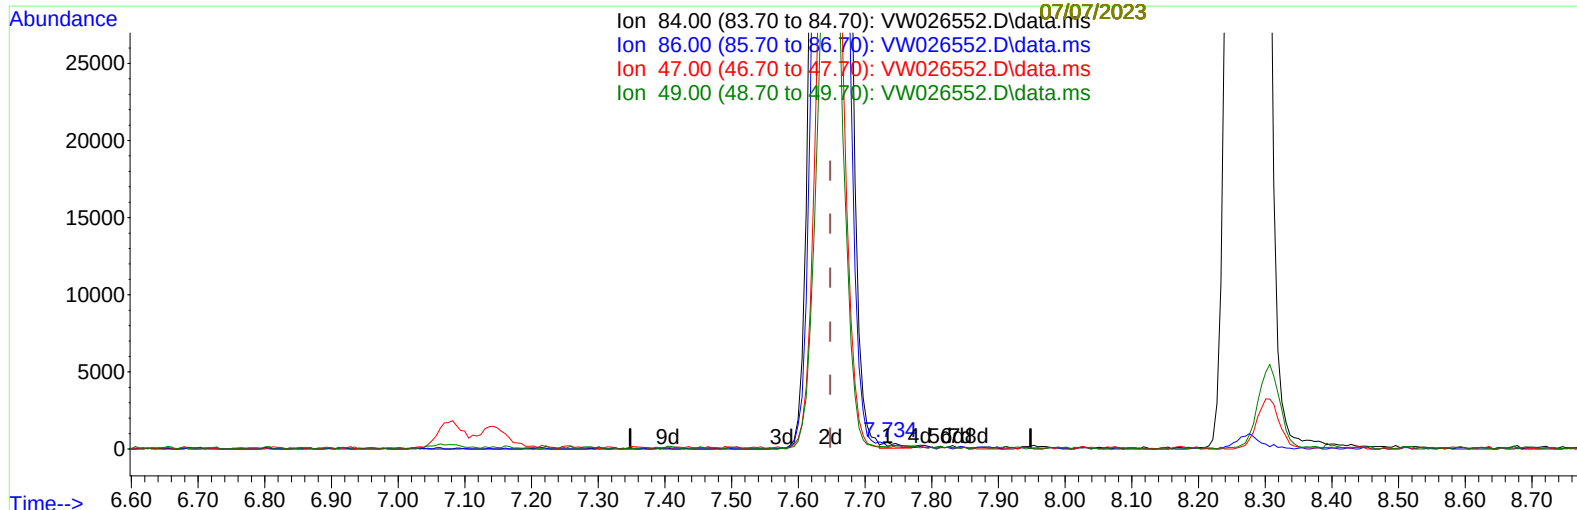

TIC: VW026552.D\data.ms

(24) Chloroform-d (S)

7.734min (+ 0.086) 0.03 ug/L

response 676

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	44.53
47.00	50.40	45.56
49.00	28.80	21.89

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070623\
 Data File : VW026552.D
 Acq On : 06 Jul 2023 19:19
 Operator : SY/MD
 Sample : 03534-20
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4739

Manual IntegrationsAPPROVED

Quant Time: Jul 07 02:36:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 04 13:17:14 2023
 Response via : Initial Calibration

Reviewed By :John




Carlone

07/07/2023

Supervised By :Semsetun

Yesilyurt

07/07/2023

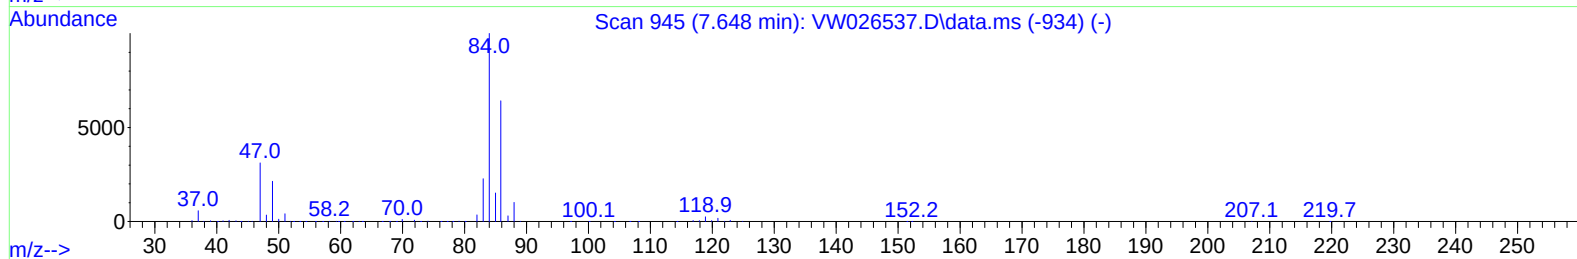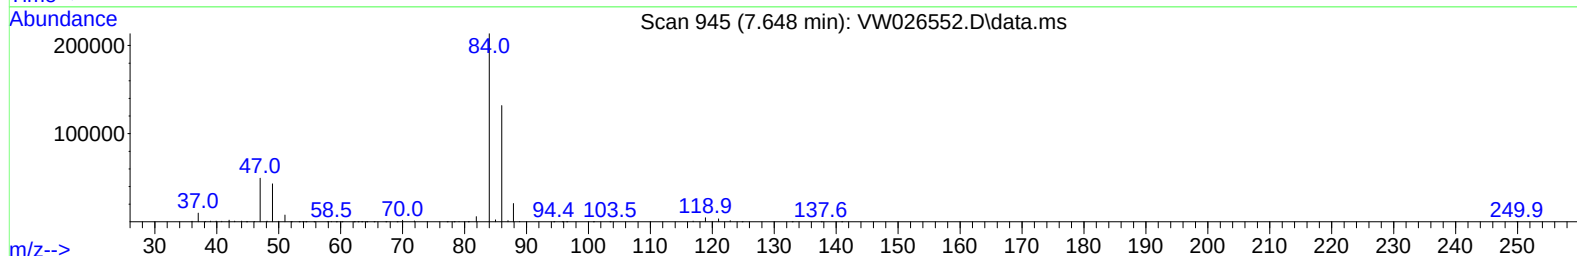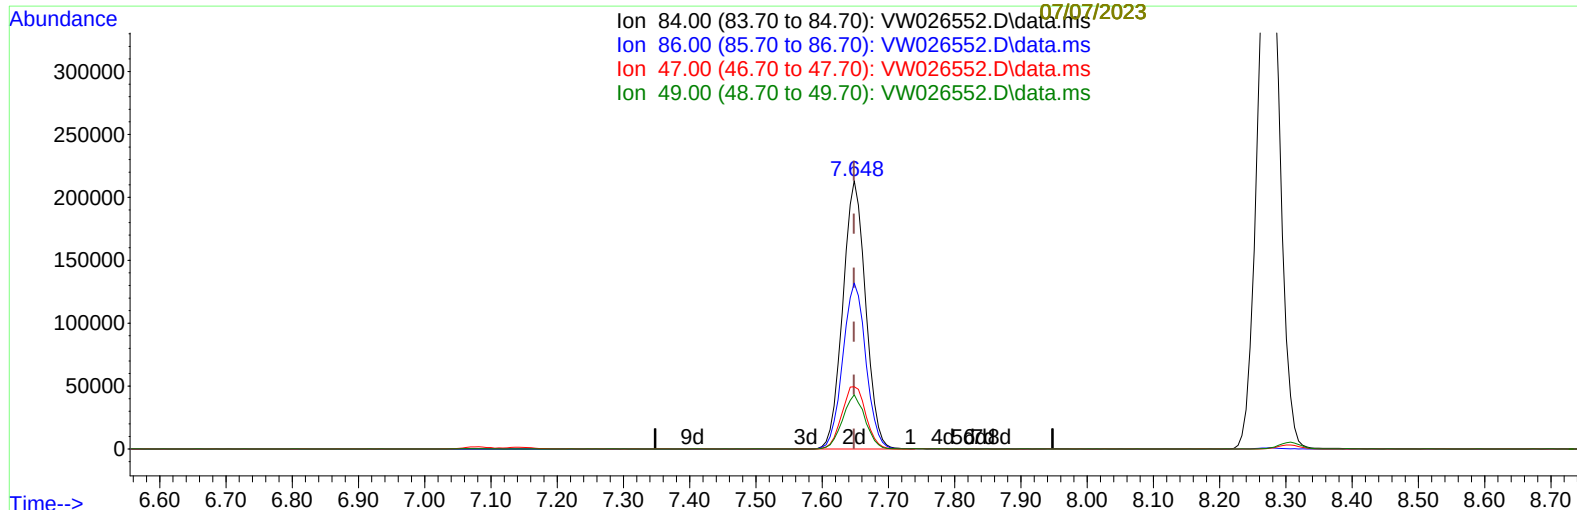

TIC: VW026552.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 21.79 ug/L m

response 509942

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.06#
47.00	50.40	0.06#
49.00	28.80	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070623\
 Data File : VW026552.D
 Acq On : 06 Jul 2023 19:19
 Operator : SY/MD
 Sample : 03534-20
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4739

Manual IntegrationsAPPROVED

Quant Time: Jul 07 02:36:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 04 13:17:14 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone
 07/07/2023

Supervised By :Semsetun
 Yesilyurt
 07/07/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		794256	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		724546	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		338038	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		239328	20.039	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.160%	
7) Chloroethane-d5	2.887	69		180572	18.275	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.120%	
11) 1,1-Dichloroethene-d2	4.021	65		118506	21.274	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.080%	
21) 2-Butanone-d5	7.075	46		192832	42.206	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.420%	
24) Chloroform-d	7.648	84		509942m	21.793	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.160%	
26) 1,2-Dichloroethane-d4	8.307	65		302922	22.258	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.040%	
32) Benzene-d6	8.270	84		1066846	23.094	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.360%	
36) 1,2-Dichloropropane-d6	9.270	67		343406	23.316	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.280%	
41) Toluene-d8	10.325	98		926764	22.346	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.400%	
43) trans-1,3-Dichloroprop...	10.575	79		129966	21.757	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.040%	
47) 2-Hexanone-d5	10.922	63		128021	43.656	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.320%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		284190	22.052	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.200%	
66) 1,2-Dichlorobenzene-d4	13.848	152		293403	21.854	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.400%	
Target Compounds						Qvalue	
13) Acetone	4.131	43		9812	3.463	ug/L	48

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070623\
Data File : VW026552.D
Acq On : 06 Jul 2023 19:19
Operator : SY/MD
Sample : 03534-20
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4739

Manual IntegrationsAPPROVED

Reviewed By :John
Carlone
07/07/2023

Supervised By :Semsetun
Yesilyurt
07/07/2023

Quant Time: Jul 07 02:36:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 04 13:17:14 2023
Response via : Initial Calibration

