

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070924\
 Data File : VW029485.D
 Acq On : 09 Jul 2024 15:45
 Operator : SY/MD
 Sample : P3177-03
 Misc : 5.73g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BS1

Quant Time: Jul 10 01:20:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 10 01:18:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	304609	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	235976	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	66671	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	107072	21.759	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.040%
7) Chloroethane-d5	2.899	69	78128	22.050	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.200%
11) 1,1-Dichloroethene-d2	4.021	65	47719	21.596	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.400%
21) 2-Butanone-d5	7.075	46	52410	35.481	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.960%
24) Chloroform-d	7.648	84	188970	21.459	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.840%
26) 1,2-Dichloroethane-d4	8.307	65	112248	21.732	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.920%
32) Benzene-d6	8.270	84	372391	26.343	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.360%
36) 1,2-Dichloropropane-d6	9.270	67	119678	26.478	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.920%
41) Toluene-d8	10.319	98	301870	24.281	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.120%
43) trans-1,3-Dichloroprop...	10.575	79	43980	22.978	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.920%
47) 2-Hexanone-d5	10.922	63	36344	44.251	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75956	20.698	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.800%
66) 1,2-Dichlorobenzene-d4	13.848	152	50090	21.573	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.280%
Target Compounds						
13) Acetone	4.125	43	6021	4.038	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070924\
Data File : VW029485.D
Acq On : 09 Jul 2024 15:45
Operator : SY/MD
Sample : P3177-03
Misc : 5.73g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BS1

Quant Time: Jul 10 01:20:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 10 01:18:26 2024
Response via : Initial Calibration

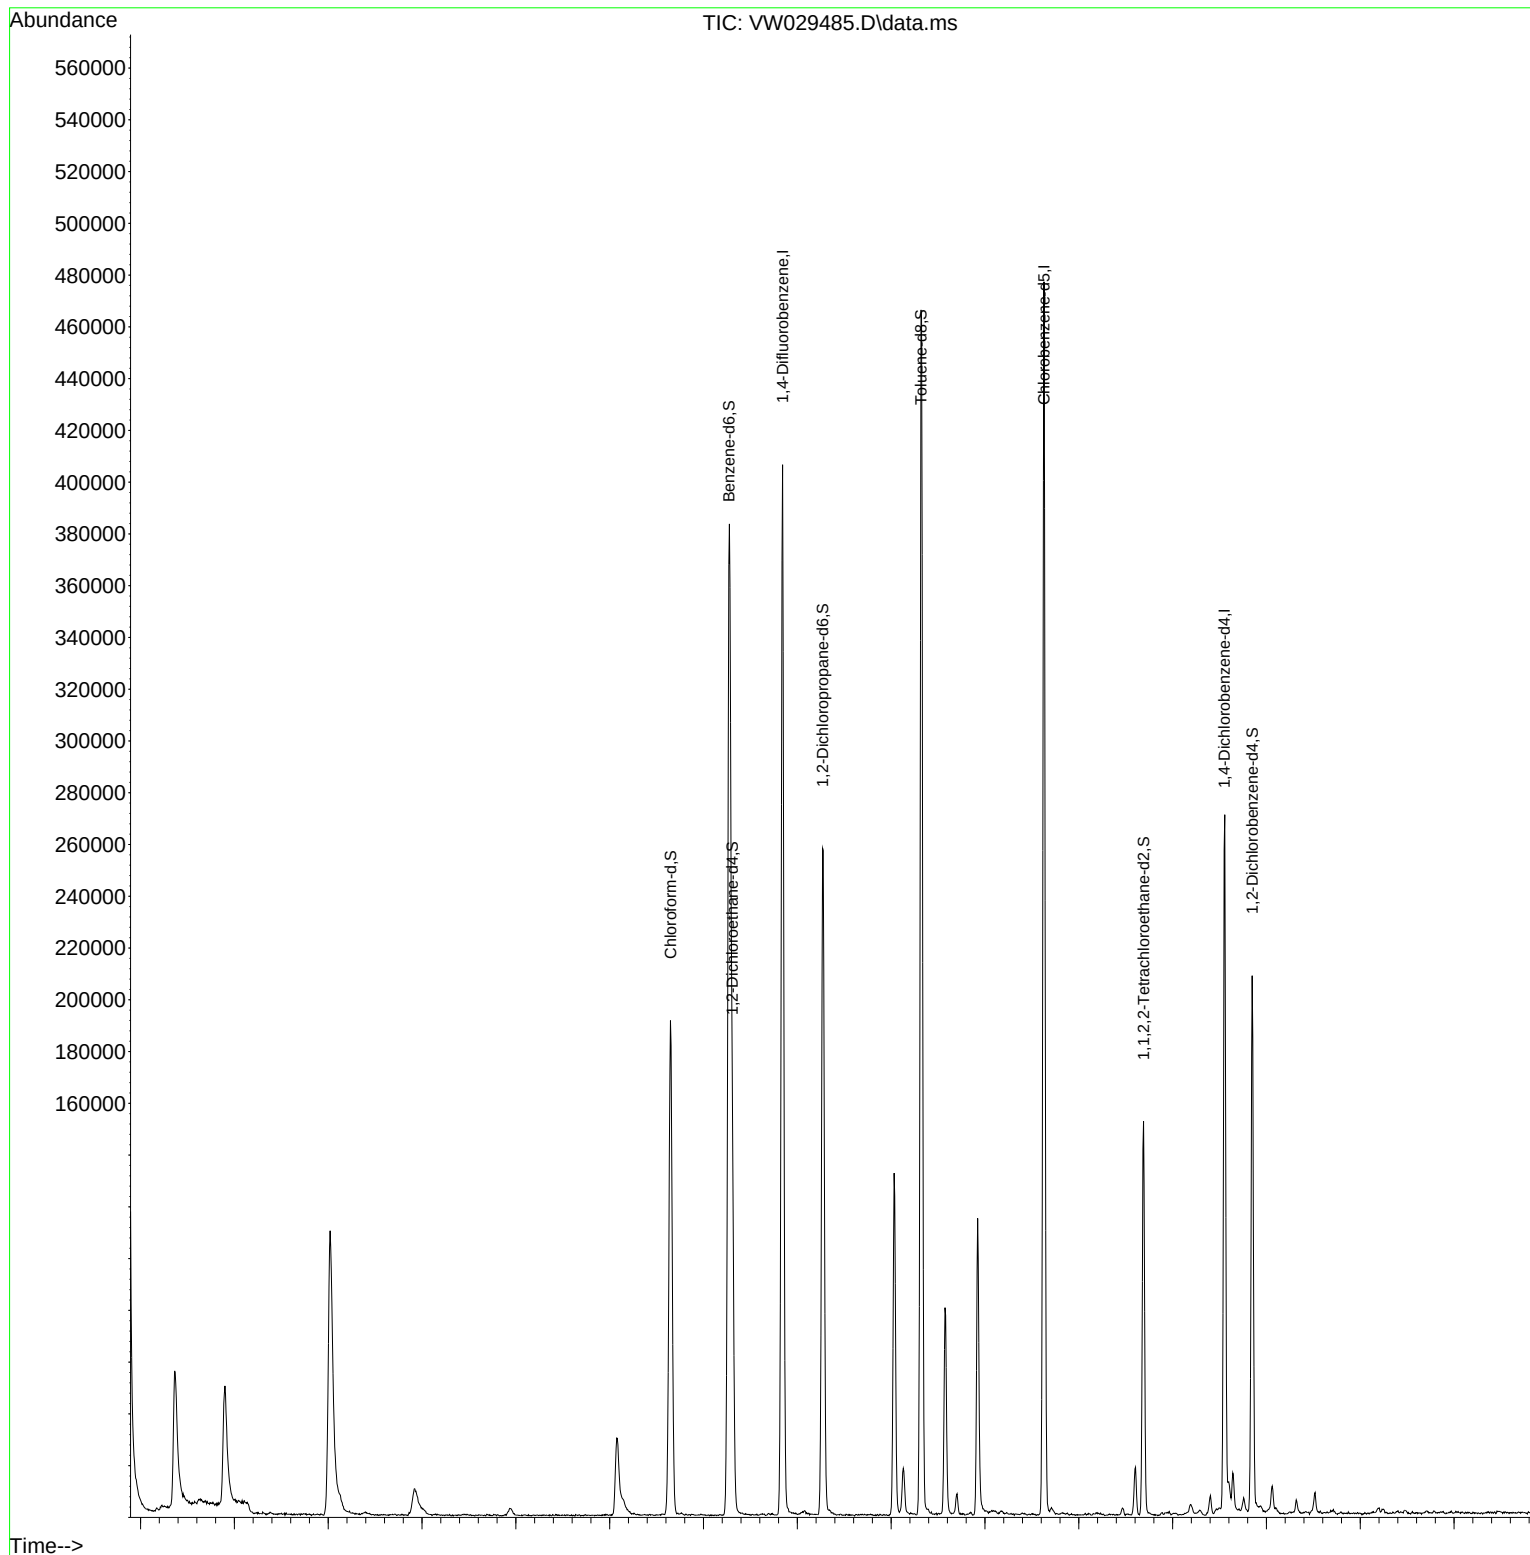

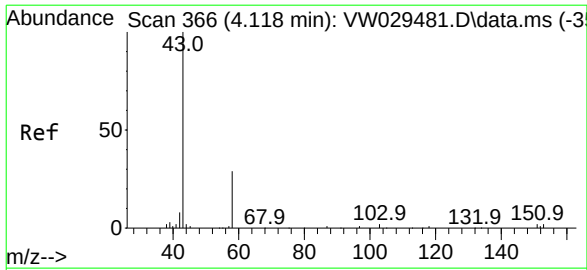

#13
 Acetone
 Concen: 4.038 ug/L
 RT: 4.125 min Scan# 36
 Delta R.T. 0.006 min
 Lab File: VW029485.D
 Acq: 09 Jul 2024 15:45

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BS1

Tgt Ion: 43 Resp: 6021
 Ion Ratio Lower Upper
 43 100
 58 29.7 0.0 55.6

