
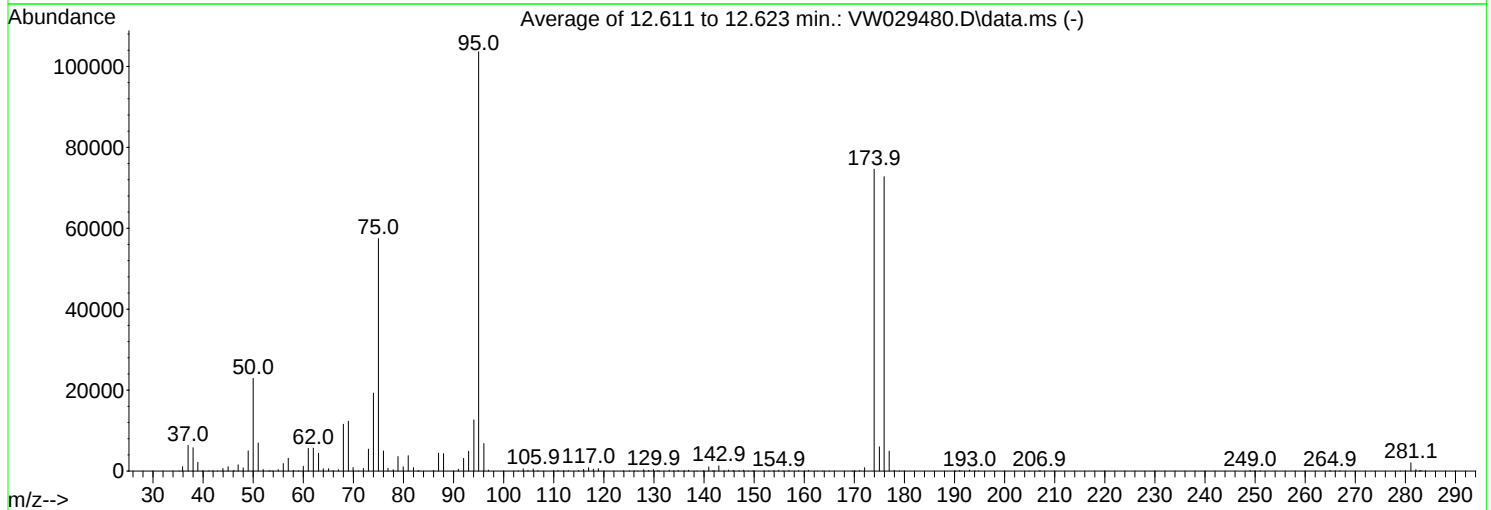


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070924\
Data File : VW029480.D
Acq On : 09 Jul 2024 09:25
Operator : SY/MD
Sample : BFB520
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB520

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Title : SFAM01.0
Last Update : Fri Jul 12 04:31:40 2024

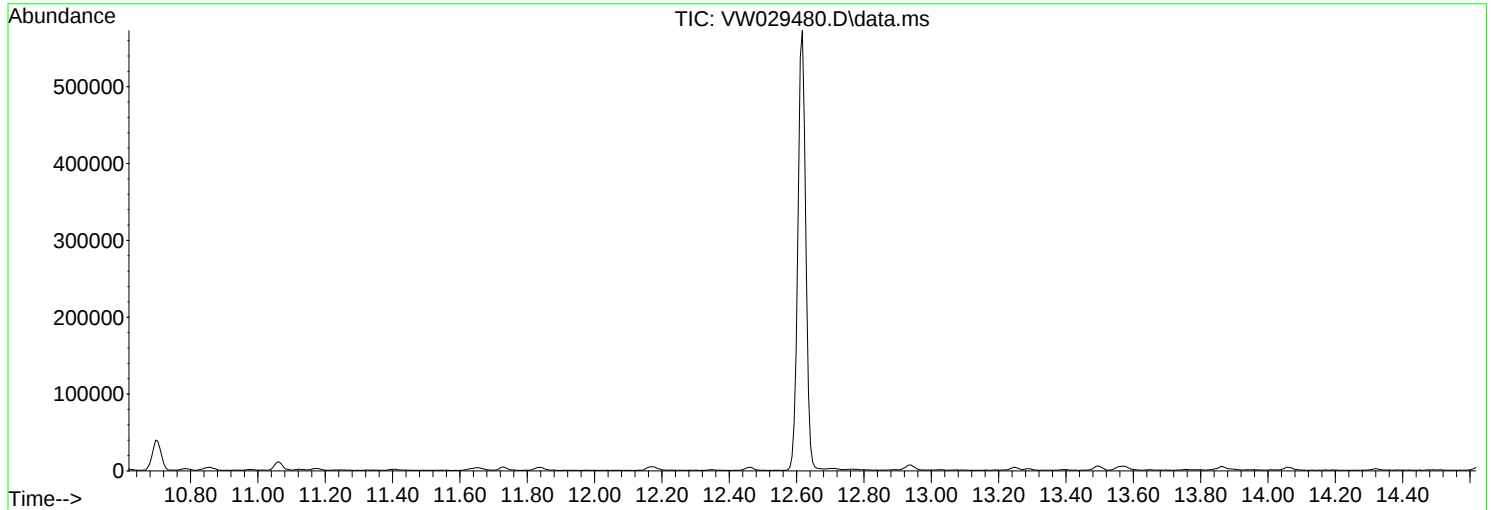

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	22931	PASS
75	95	30	80	55.4	57453	PASS
95	95	100	100	100.0	103632	PASS
96	95	5	9	6.6	6814	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.0	74597	PASS
175	174	5	9	8.0	5992	PASS
176	174	95	101	97.5	72765	PASS
177	176	5	9	6.8	4931	PASS

m/z	Abundance
35.80	53.0
37.30	52.0
38.90	86.0
39.90	313.0
43.00	77.0
43.90	224.0

Instrument :
MSVOA_W
ClientSampleId :
BFB520

m/z	Abundance
36.00	1286.0
37.00	6842.0
38.00	6423.0
39.00	2643.0
40.00	457.0
41.10	81.0
42.90	178.0
44.00	964.0
45.00	1401.0
46.10	207.0
47.00	1657.0
48.00	920.0
49.00	5390.0
50.00	24752.0
51.00	7881.0
52.00	472.0
53.20	151.0
53.80	104.0
54.90	357.0
56.00	1917.0
57.00	3382.0
58.00	152.0
59.10	96.0
60.00	1161.0
61.00	5975.0
62.00	6303.0
63.00	4299.0
64.00	747.0
65.10	672.0
66.00	173.0
67.10	341.0
68.00	12032.0
69.00	13191.0
70.00	866.0
72.00	698.0
73.00	5882.0
74.00	21080.0
75.00	61600.0
76.00	5542.0
76.90	616.0
78.90	3910.0
79.90	1069.0
80.90	4251.0
82.00	1010.0
82.90	127.0
83.10	128.0
86.00	209.0
87.00	4740.0
88.00	4825.0
90.90	466.0
92.00	3063.0
93.00	4901.0
94.00	13100.0
95.00	107584.0
96.00	7083.0
96.90	306.0
102.90	114.0
104.00	670.0
104.90	191.0
105.90	509.0
106.90	120.0
110.00	128.0
110.90	197.0
111.90	93.0
112.90	137.0
115.00	154.0
115.90	381.0
116.90	827.0
117.90	505.0
118.90	722.0
125.20	103.0
126.80	50.0
128.00	406.0
129.10	200.0
129.80	376.0
130.80	164.0
133.00	428.0
134.00	113.0
134.90	260.0
136.10	70.0
137.00	207.0
139.80	96.0
141.00	891.0
142.10	158.0
142.90	1495.0
144.00	89.0
144.90	272.0
145.80	190.0
147.00	132.0
147.90	225.0
148.90	106.0
149.90	151.0

Instrument :
MSVOA_W
ClientSampleId :
BFB520

151.90	66.0
152.90	78.0
154.00	146.0
154.90	173.0
156.90	162.0
158.80	124.0
160.90	167.0
162.70	52.0
163.70	67.0
165.00	62.0
170.10	58.0
171.10	237.0
172.10	980.0
173.90	71032.0
175.00	5736.0
176.00	70656.0
176.90	4615.0
178.00	194.0
179.00	125.0
190.20	76.0
191.00	250.0
193.00	408.0
194.10	88.0
194.90	69.0
204.90	59.0
206.90	174.0
249.10	282.0
250.00	79.0
251.00	106.0
265.00	362.0
266.00	74.0
267.00	88.0
279.00	82.0
280.00	109.0
281.10	3130.0
282.10	849.0
283.10	468.0
284.00	144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB520

m/z	Abundance
35.20	55.0
35.90	1235.0
37.00	7445.0
38.00	6668.0
39.00	2341.0
40.00	349.0
41.10	53.0
42.10	50.0
42.90	118.0
44.00	970.0
45.00	1025.0
46.20	202.0
47.00	1573.0
48.00	960.0
49.00	5703.0
50.00	25616.0
51.00	7578.0
52.00	425.0
53.00	115.0
53.40	79.0
55.00	444.0
56.00	2076.0
57.00	3352.0
58.10	217.0
59.00	68.0
60.00	1351.0
61.00	6110.0
62.00	6033.0
63.00	5193.0
64.00	679.0
65.00	685.0
66.00	78.0
67.00	381.0
68.00	13207.0
69.00	14070.0
70.00	1079.0
71.00	71.0
72.00	703.0
73.00	6174.0
74.00	20320.0
75.00	63704.0
76.00	5293.0
76.90	941.0
77.90	578.0
78.90	3928.0
79.90	1078.0
81.00	4153.0
82.00	1032.0
83.00	192.0
86.00	175.0
87.00	5056.0
88.00	4473.0
91.00	481.0
92.00	3402.0
93.00	5629.0
94.10	14466.0
95.00	111544.0
96.00	7486.0
97.00	286.0
102.90	137.0
103.80	510.0
104.80	226.0
106.00	635.0
106.90	181.0
109.90	110.0
110.80	151.0
112.00	80.0
112.90	110.0
114.90	142.0
116.00	437.0
117.00	952.0
117.90	554.0
118.90	613.0
123.90	119.0
125.00	101.0
126.10	66.0
127.90	327.0
128.90	159.0
129.90	447.0
131.00	154.0
133.10	181.0
133.90	76.0
134.80	181.0
136.00	103.0
136.90	213.0
139.90	112.0
141.00	1248.0
141.90	189.0
143.00	1262.0
144.00	106.0
144.90	352.0
145.90	208.0

Instrument :
MSVOA_W
ClientSampleId :
BFB520

147.10	124.0
148.00	277.0
148.70	73.0
149.80	112.0
152.00	100.0
153.00	54.0
153.90	75.0
154.90	236.0
155.80	67.0
157.00	250.0
158.90	144.0
160.80	116.0
170.20	67.0
171.00	133.0
172.00	873.0
174.00	88048.0
175.00	7188.0
176.00	76168.0
177.00	5666.0
177.90	170.0
191.00	146.0
193.00	236.0
194.80	59.0
207.10	233.0
248.90	204.0
251.00	90.0
264.90	168.0
266.10	62.0
266.90	126.0
281.10	2220.0
282.80	227.0
284.10	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB520

m/z	Abundance
36.00	868.0
37.00	4874.0
38.00	4260.0
39.00	1798.0
40.00	287.0
41.20	61.0
41.90	90.0
42.90	83.0
44.00	655.0
45.00	850.0
46.10	144.0
47.00	1446.0
48.00	557.0
49.00	3952.0
50.00	18424.0
51.00	5399.0
52.00	255.0
53.20	106.0
55.10	301.0
56.00	1591.0
57.00	2798.0
58.10	137.0
59.10	53.0
60.00	1049.0
61.00	4748.0
62.00	4680.0
63.10	3756.0
64.00	333.0
65.00	413.0
65.80	66.0
66.90	342.0
68.00	9495.0
69.00	9690.0
69.90	702.0
71.00	60.0
72.00	471.0
73.00	4251.0
74.00	16400.0
75.00	47056.0
76.00	4076.0
77.00	514.0
78.00	481.0
78.90	2954.0
80.00	1029.0
80.90	2983.0
81.90	498.0
83.00	121.0
86.10	108.0
87.00	3500.0
88.00	3646.0
90.90	501.0
92.00	2946.0
93.00	4228.0
94.00	10408.0
95.00	91768.0
96.10	5874.0
97.00	183.0
103.90	501.0
104.90	176.0
105.80	460.0
106.80	110.0
110.00	82.0
110.90	74.0
112.00	84.0
112.90	157.0
114.90	106.0
115.90	396.0
117.00	736.0
117.90	357.0
118.90	504.0
123.90	56.0
126.10	70.0
127.90	322.0
128.90	179.0
130.00	321.0
130.70	60.0
131.10	78.0
133.00	102.0
134.80	171.0
136.00	67.0
136.80	208.0
138.60	58.0
139.90	100.0
140.90	982.0
141.70	160.0
142.90	1147.0
145.00	195.0
145.90	144.0
146.90	73.0
147.80	208.0
149.70	119.0
152.90	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB520

154.00	89.0
154.90	250.0
156.90	203.0
158.80	146.0
160.90	100.0
169.60	71.0
172.00	651.0
174.00	64712.0
175.00	5051.0
175.90	71472.0
177.00	4512.0
177.90	190.0
191.30	71.0
192.90	121.0
206.90	116.0
249.00	77.0
264.90	85.0
267.00	86.0
281.00	787.0
282.00	268.0
283.10	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB520