

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071019\
 Data File : VW011191.D
 Acq On : 10 Jul 2019 13:04
 Operator : SY/VA
 Sample : K3724-06
 Misc : 5.13G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB8T3

Quant Time: Jul 11 06:54:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 11 05:38:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	279551	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	260448	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	121264	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	72036	16.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.52%
7) Chloroethane-d5	2.89	69	57954	19.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.40%
10) 1,1-Dichloroethene-d2	4.01	63	132719	14.68	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.72%
20) 2-Butanone-d5	7.07	46	84591	50.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.62%
24) Chloroform-d	7.65	84	177497	23.16	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.64%
26) 1,2-Dichloroethane-d4	8.31	65	115378	24.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.80%
29) Benzene-d6	8.27	84	357558	22.28	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.12%
33) 1,2-Dichloropropane-d6	9.27	67	123299	23.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.40%
37) Toluene-d8	10.32	98	313326	21.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.64%
38) trans-1,3-Dichloropropene-	10.58	79	47459	21.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.44%
39) 2-Hexanone-d5	10.93	63	53348	44.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.04%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	104698	24.23	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.92%
61) 1,2-Dichlorobenzene-d4	13.85	152	114426	24.58	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.32%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.13	43	3052	1.858	ug/L	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW071019\
Data File : VW011191.D
Acq On : 10 Jul 2019 13:04
Operator : SY/VA
Sample : K3724-06
Misc : 5.13G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB8T3

Quant Time: Jul 11 06:54:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 11 05:38:29 2019
Response via : Initial Calibration

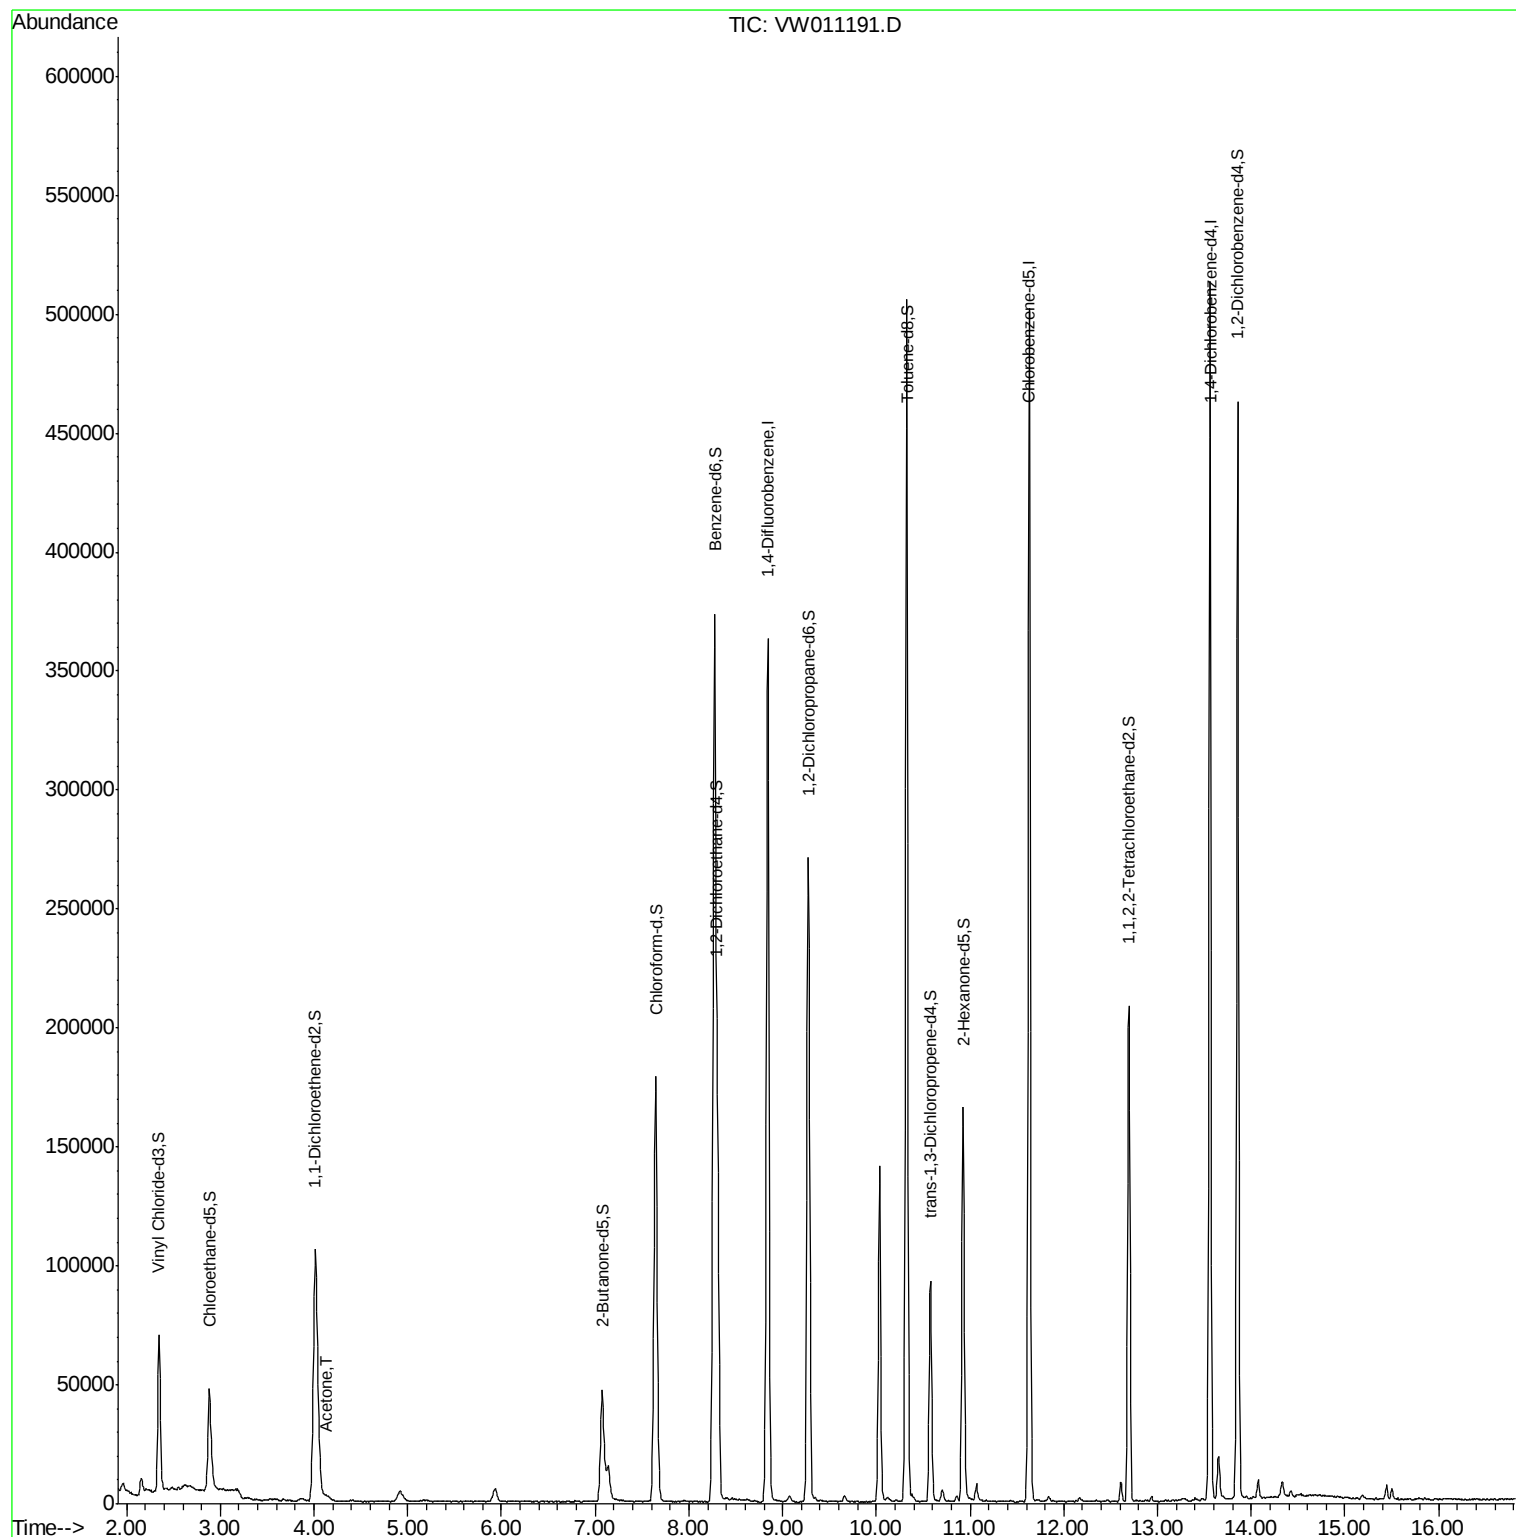

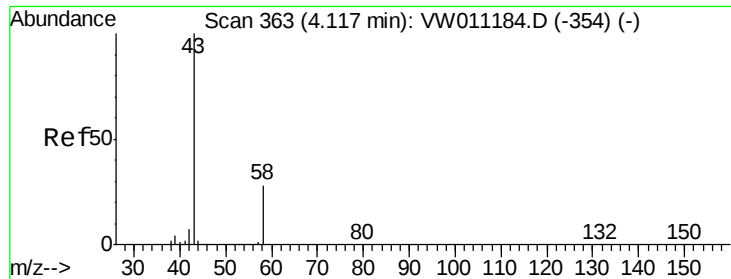

#13

Acetone

Concen: 1.858 ug/L

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW011191.D

Acq: 10 Jul 2019 13:04

Instrument :

MSVOA_W

ClientSampleId :

DB8T3

Tgt Ion: 43 Resp: 3052

Ion Ratio Lower Upper

43 100

58 11.3 0.0 55.0

