

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071024\
 Data File : VW029497.D
 Acq On : 10 Jul 2024 11:26
 Operator : SY/MD
 Sample : P3100-05
 Misc : 5.00g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 11 02:15:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 11 02:12:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	258908	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	239507	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	104363	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	100596	24.052	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.200%
7) Chloroethane-d5	2.899	69	74931	24.881	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.520%
11) 1,1-Dichloroethene-d2	4.027	65	45905	24.442	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	97.760%
21) 2-Butanone-d5	7.075	46	53320	42.468	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.940%
24) Chloroform-d	7.648	84	192648	25.738	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.960%
26) 1,2-Dichloroethane-d4	8.307	65	114615	26.107	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.440%
32) Benzene-d6	8.276	84	390176	27.194	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.760%
36) 1,2-Dichloropropane-d6	9.276	67	125743	27.410	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.640%
41) Toluene-d8	10.325	98	344493	27.301	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	109.200%
43) trans-1,3-Dichloroprop...	10.575	79	47022	24.205	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.840%
47) 2-Hexanone-d5	10.922	63	36038	43.231	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.460%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	89949	24.150	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	106404	29.276	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	117.120%
Target Compounds			Qvalue			
39) cis-1,3-Dichloropropene	10.032	75	3667	0.589	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071024\
Data File : VW029497.D
Acq On : 10 Jul 2024 11:26
Operator : SY/MD
Sample : P3100-05
Misc : 5.00g/10mL/MSVOA_W/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jul 11 02:15:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 11 02:12:03 2024
Response via : Initial Calibration

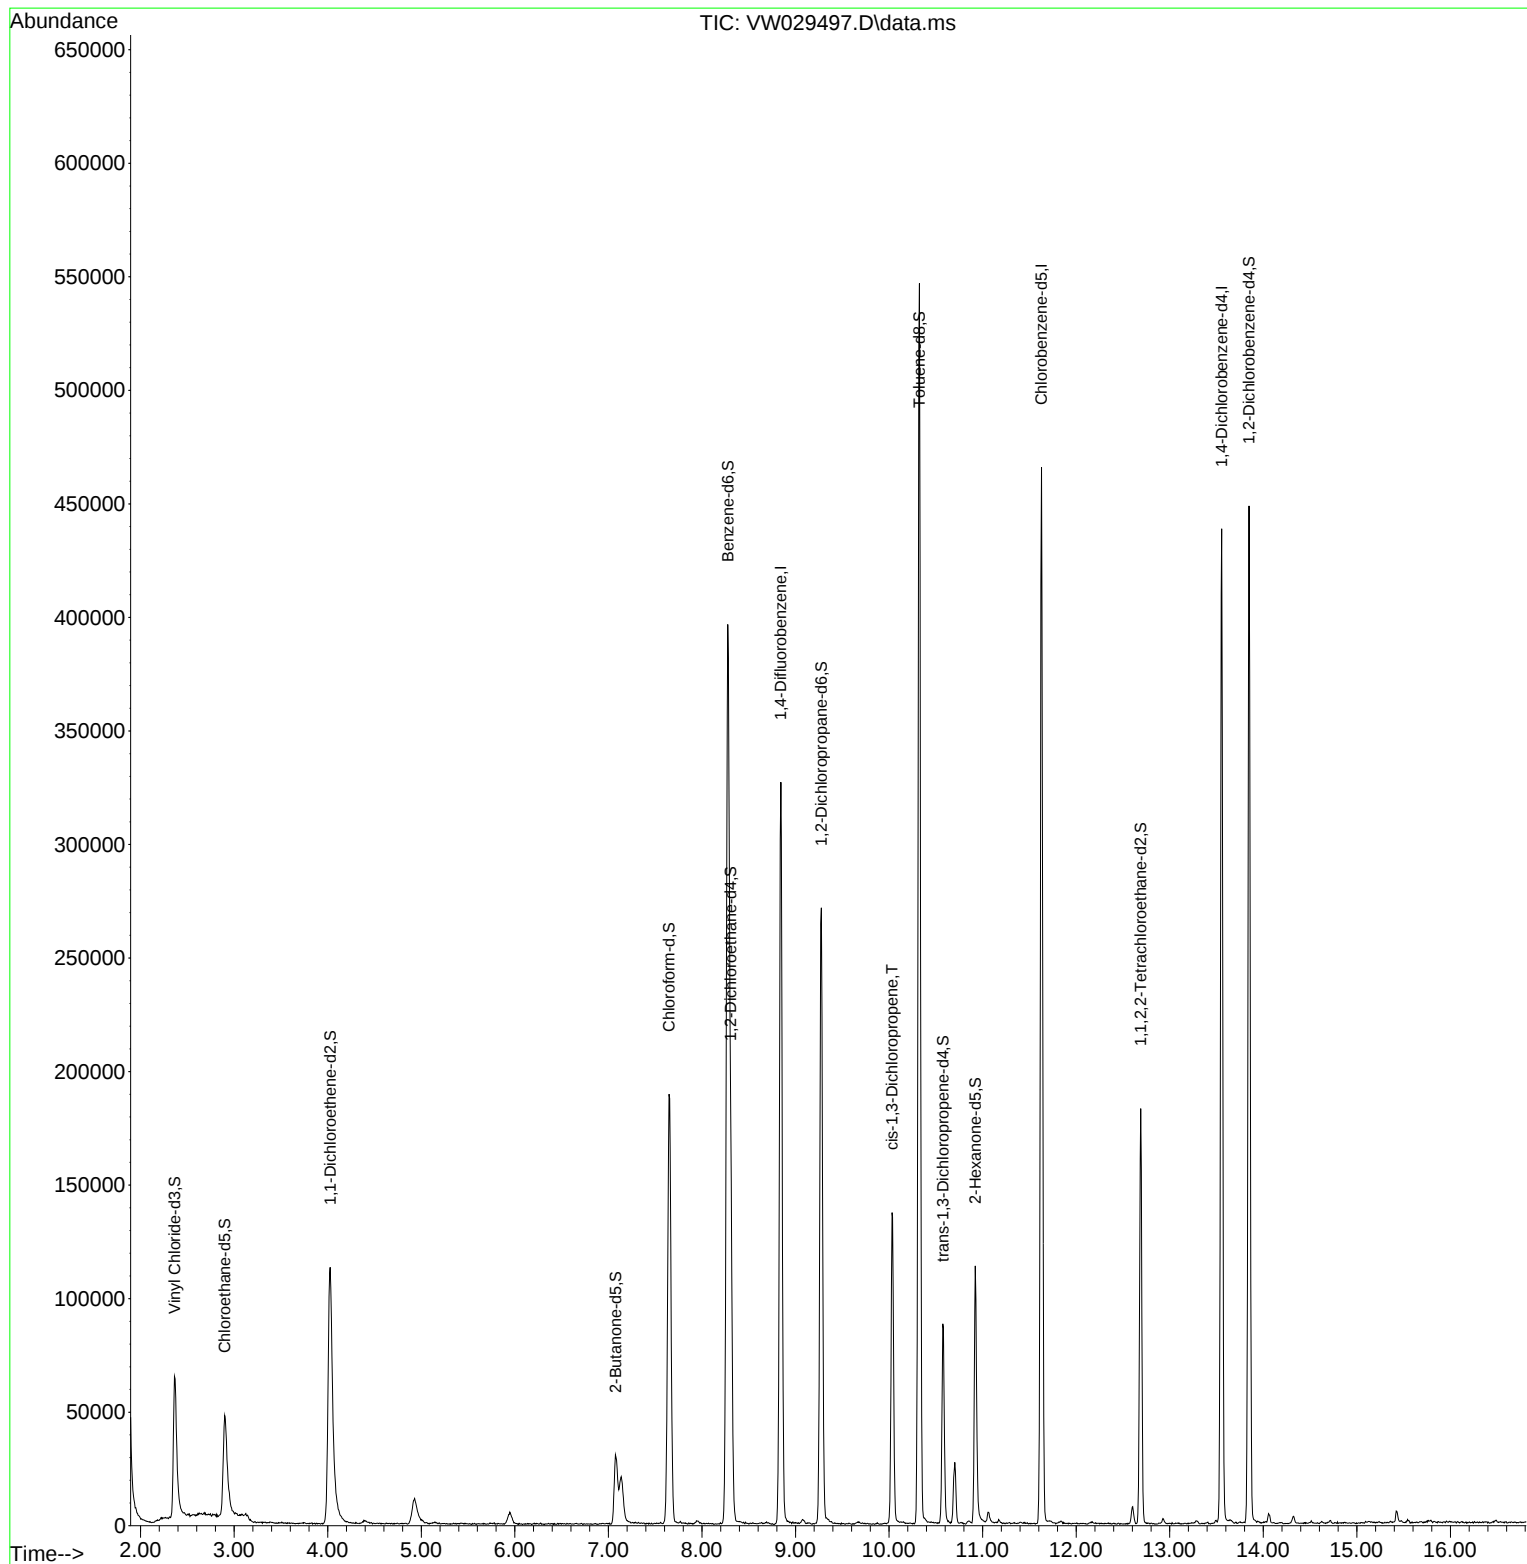

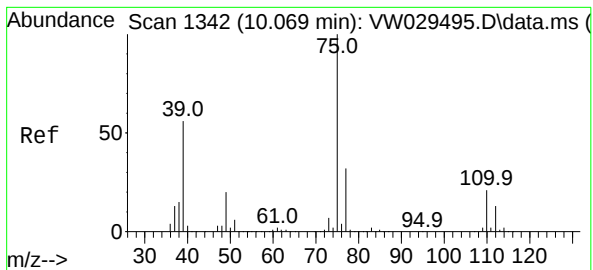

#39
 cis-1,3-Dichloropropene
 Concen: 0.589 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029497.D
 Acq: 10 Jul 2024 11:26

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3667
 Ion Ratio Lower Upper
 75 100
 77 50.8 22.2 41.2#

