

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071025\
 Data File : VW031792.D
 Acq On : 10 Jul 2025 10:15
 Operator : SY/MD
 Sample : VW0710SBL01
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0710SBL01

Quant Time: Jul 11 02:15:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:35:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.959	168	178449	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	403423	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.635	117	368923	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	171872	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	143086	55.872	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	111.740%
35) Dibromofluoromethane	7.898	113	121172	46.029	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	92.060%
50) Toluene-d8	10.325	98	445433	45.468	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	90.940%
62) 4-Bromofluorobenzene	12.617	95	164288	45.570	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	91.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071025\
Data File : VW031792.D
Acq On : 10 Jul 2025 10:15
Operator : SY/MD
Sample : VW0710SBL01
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0710SBL01

Quant Time: Jul 11 02:15:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:35:17 2025
Response via : Initial Calibration




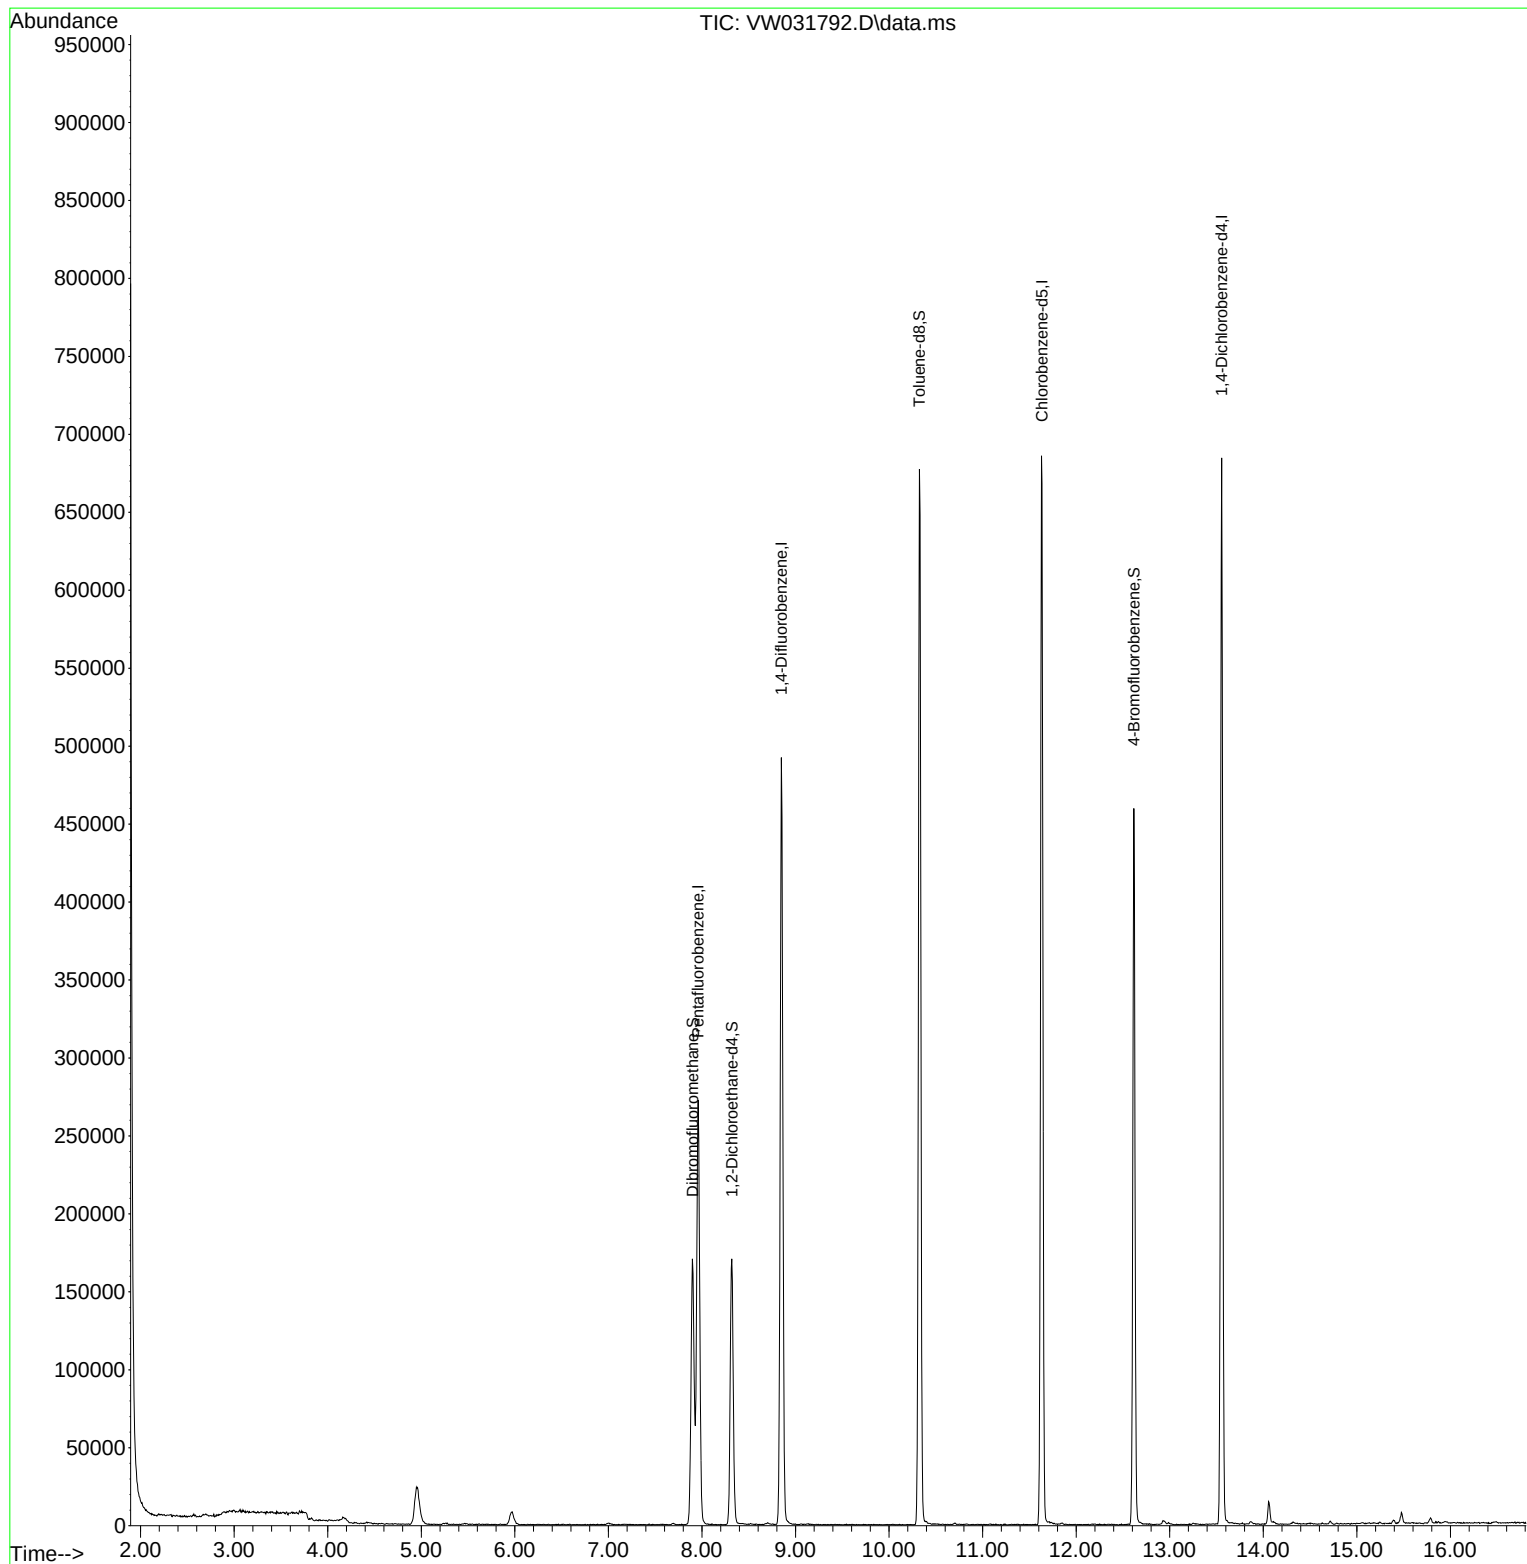


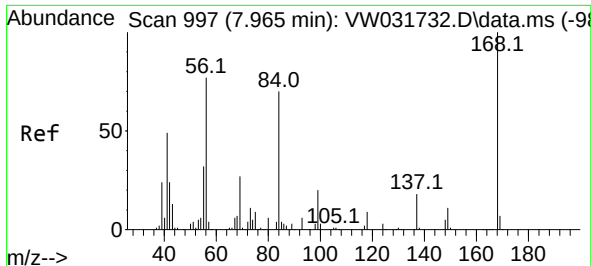

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 996
Delta R.T. -0.006 min
Lab File: VW031792.D
Acq: 10 Jul 2025 10:15




Instrument :
MSVOA_W
ClientSampleId :
VW0710SBL01


Tgt Ion:168 Resp: 178449
Ion Ratio Lower Upper
168 100
99 67.2 49.4 74.2

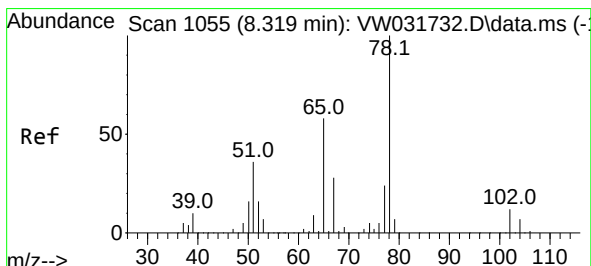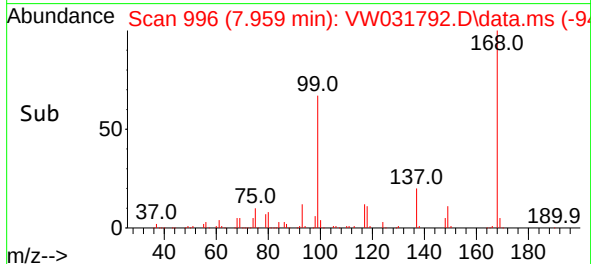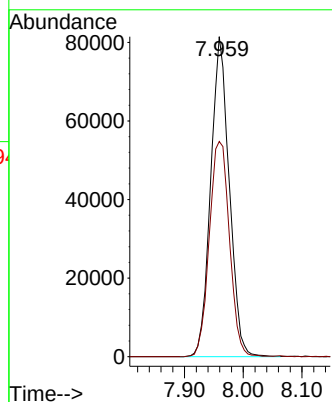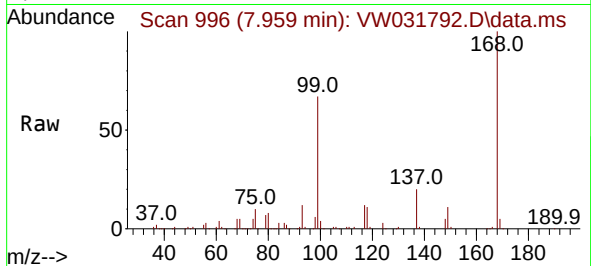

#33
1,2-Dichloroethane-d4
Concen: 55.872 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW031792.D
Acq: 10 Jul 2025 10:15

Tgt Ion: 65 Resp: 143086
Ion Ratio Lower Upper
65 100
67 50.7 0.0 99.4


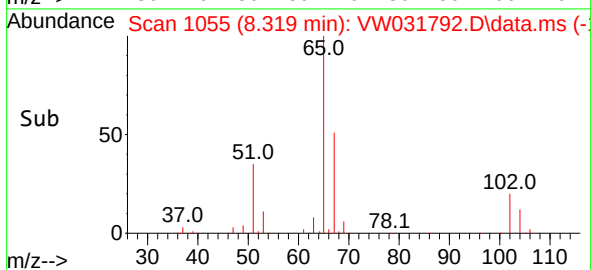
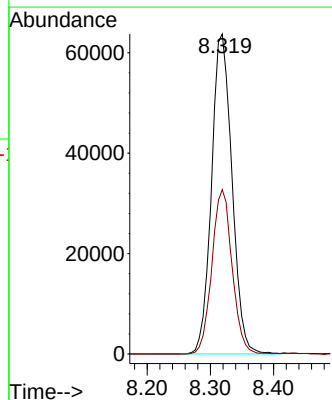
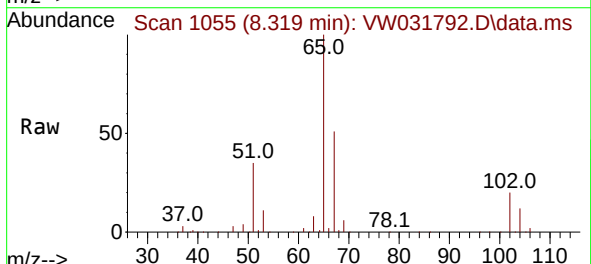


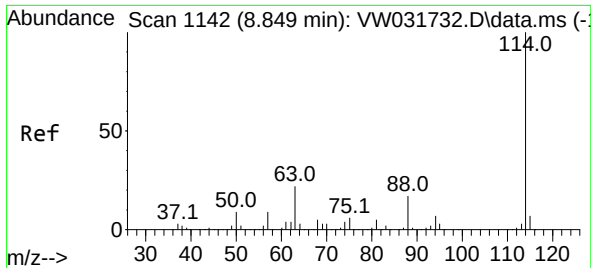

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.849 min Scan# 1142
 Delta R.T. 0.000 min
 Lab File: VW031792.D
 Acq: 10 Jul 2025 10:15




Instrument :
 MSVOA_W
 ClientSampleId :
 VW0710SBL01


Tgt Ion:114 Resp: 403423
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 43.6
 88 15.7 0.0 34.2

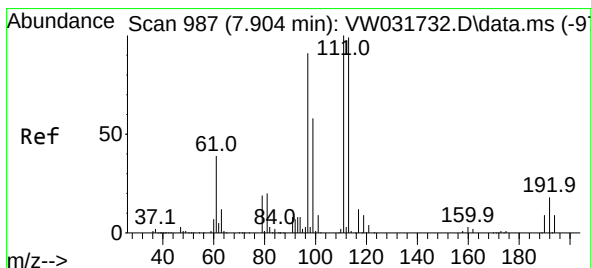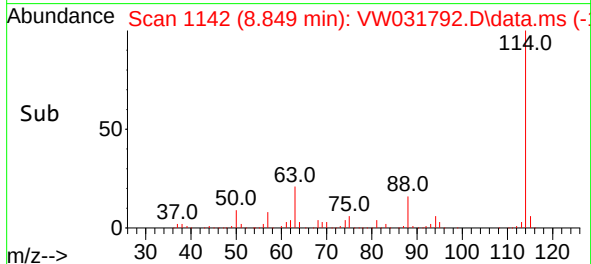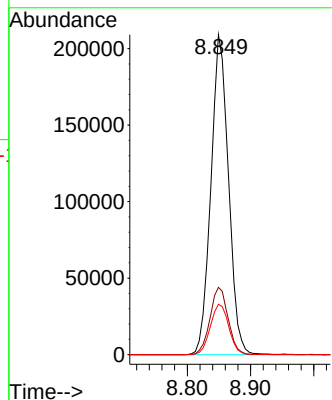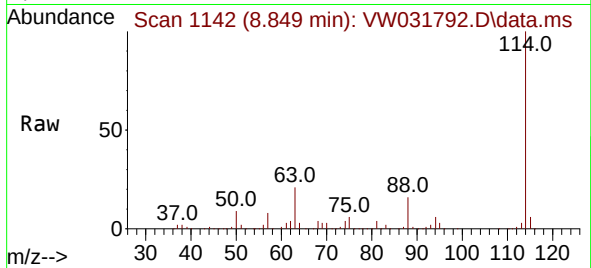

#35
 Dibromofluoromethane
 Concen: 46.029 ug/l
 RT: 7.898 min Scan# 986
 Delta R.T. -0.006 min
 Lab File: VW031792.D
 Acq: 10 Jul 2025 10:15

Tgt Ion:113 Resp: 121172
 Ion Ratio Lower Upper
 113 100
 111 105.3 82.1 123.1
 192 16.5 13.8 20.6


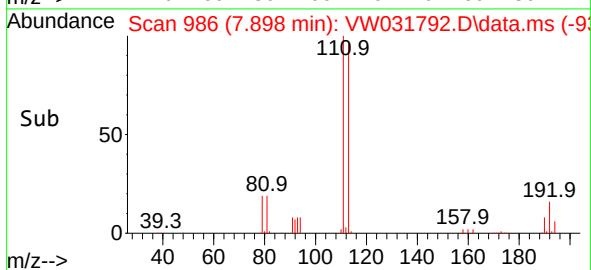
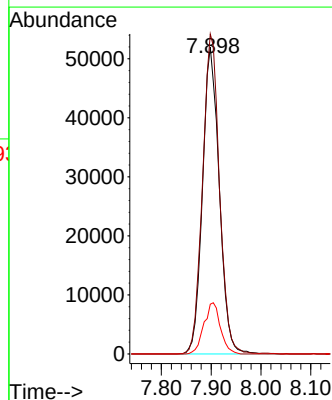
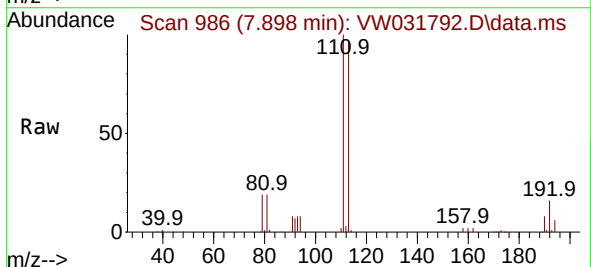


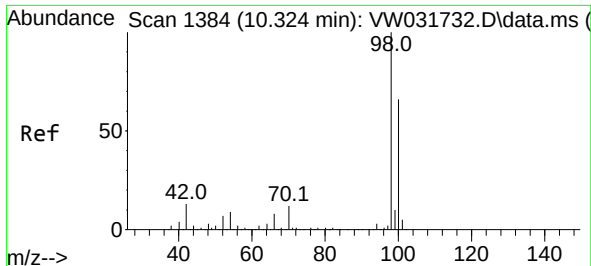

#50
Toluene-d8
Concen: 45.468 ug/l
RT: 10.325 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW031792.D
Acq: 10 Jul 2025 10:15




Instrument :
MSVOA_W
ClientSampleId :
VW0710SBL01


Tgt Ion: 98 Resp: 445433
Ion Ratio Lower Upper
98 100
100 66.6 53.0 79.4

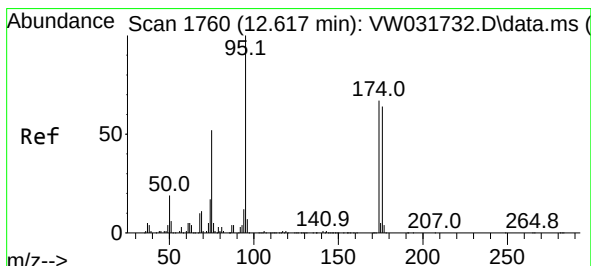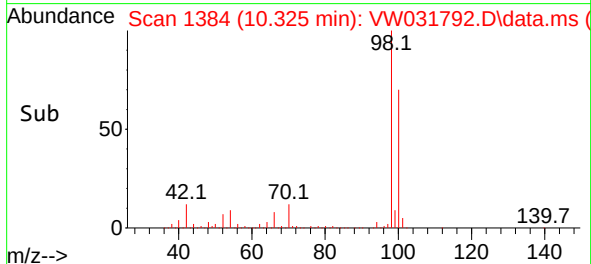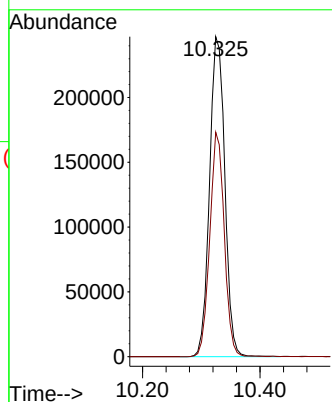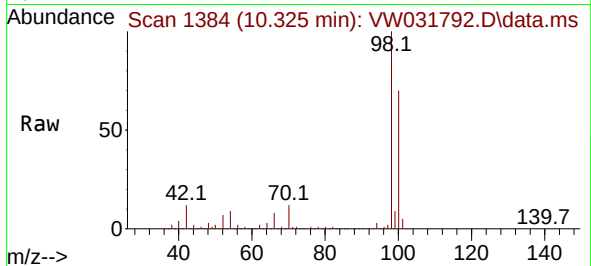

#62
4-Bromofluorobenzene
Concen: 45.570 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW031792.D
Acq: 10 Jul 2025 10:15

Tgt Ion: 95 Resp: 164288
Ion Ratio Lower Upper
95 100
174 59.0 0.0 133.8
176 59.7 0.0 126.0


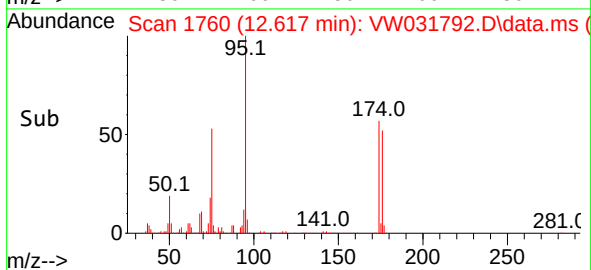
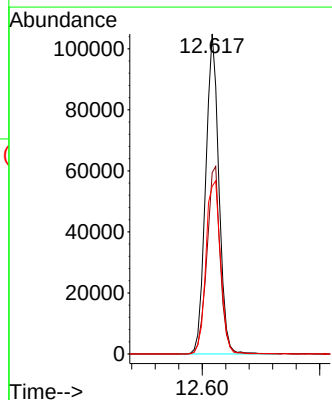
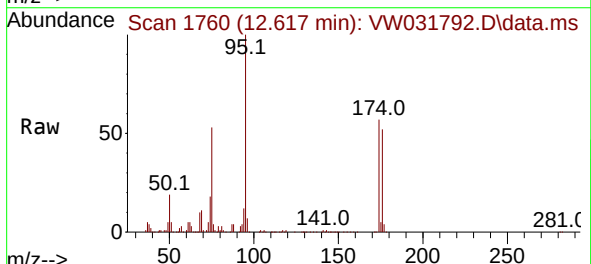


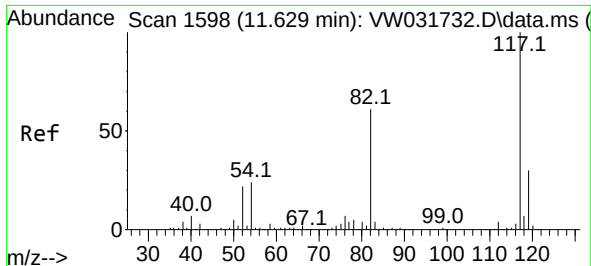

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.635 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW031792.D
Acq: 10 Jul 2025 10:15

Instrument :
MSVOA_W
ClientSampleId :
VW0710SBL01

Tgt Ion:117 Resp: 368923
Ion Ratio Lower Upper
117 100
82 57.6 48.6 72.8
119 32.7 23.9 35.9

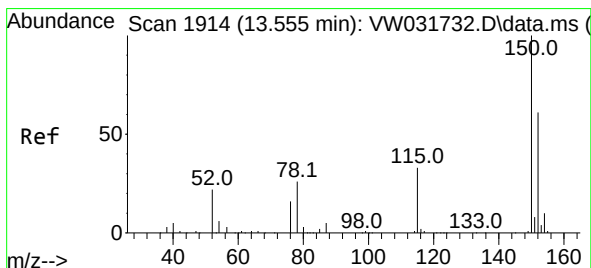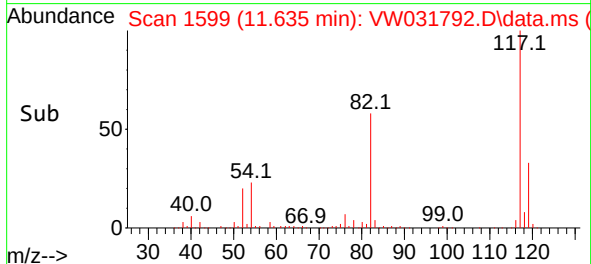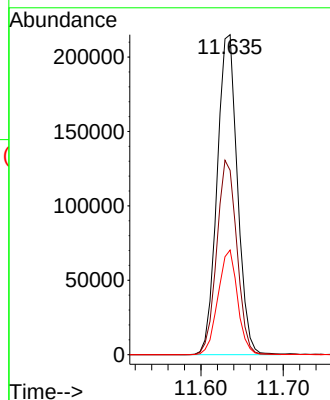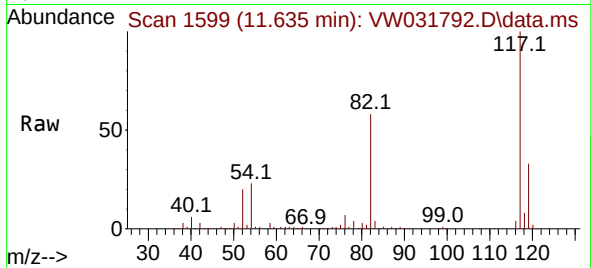

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. 0.000 min
Lab File: VW031792.D
Acq: 10 Jul 2025 10:15

Tgt Ion:152 Resp: 171872
Ion Ratio Lower Upper
152 100
115 64.8 31.9 95.7
150 150.4 0.0 356.4

