

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071025\
 Data File : VW031801.D
 Acq On : 10 Jul 2025 14:30
 Operator : SY/MD
 Sample : Q2529-08
 Misc : 3.89g/5mL/MSVOA_W/SOIL/B
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 TP-89

Quant Time: Jul 11 02:21:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:35:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.965	168	174642	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	393151	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.635	117	366298	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	174003	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	138054	55.083	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	110.160%
35) Dibromofluoromethane	7.904	113	116738	45.503	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	91.000%
50) Toluene-d8	10.325	98	428866	44.921	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	89.840%
62) 4-Bromofluorobenzene	12.617	95	171272	48.749	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	97.500%
Target Compounds						
					Qvalue	
16) Acetone	4.167	43	7296	11.778	ug/l	93
20) Methylene Chloride	4.960	84	25745	6.489	ug/l	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071025\
Data File : VW031801.D
Acq On : 10 Jul 2025 14:30
Operator : SY/MD
Sample : Q2529-08
Misc : 3.89g/5mL/MSVOA_W/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
TP-89

Quant Time: Jul 11 02:21:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:35:17 2025
Response via : Initial Calibration




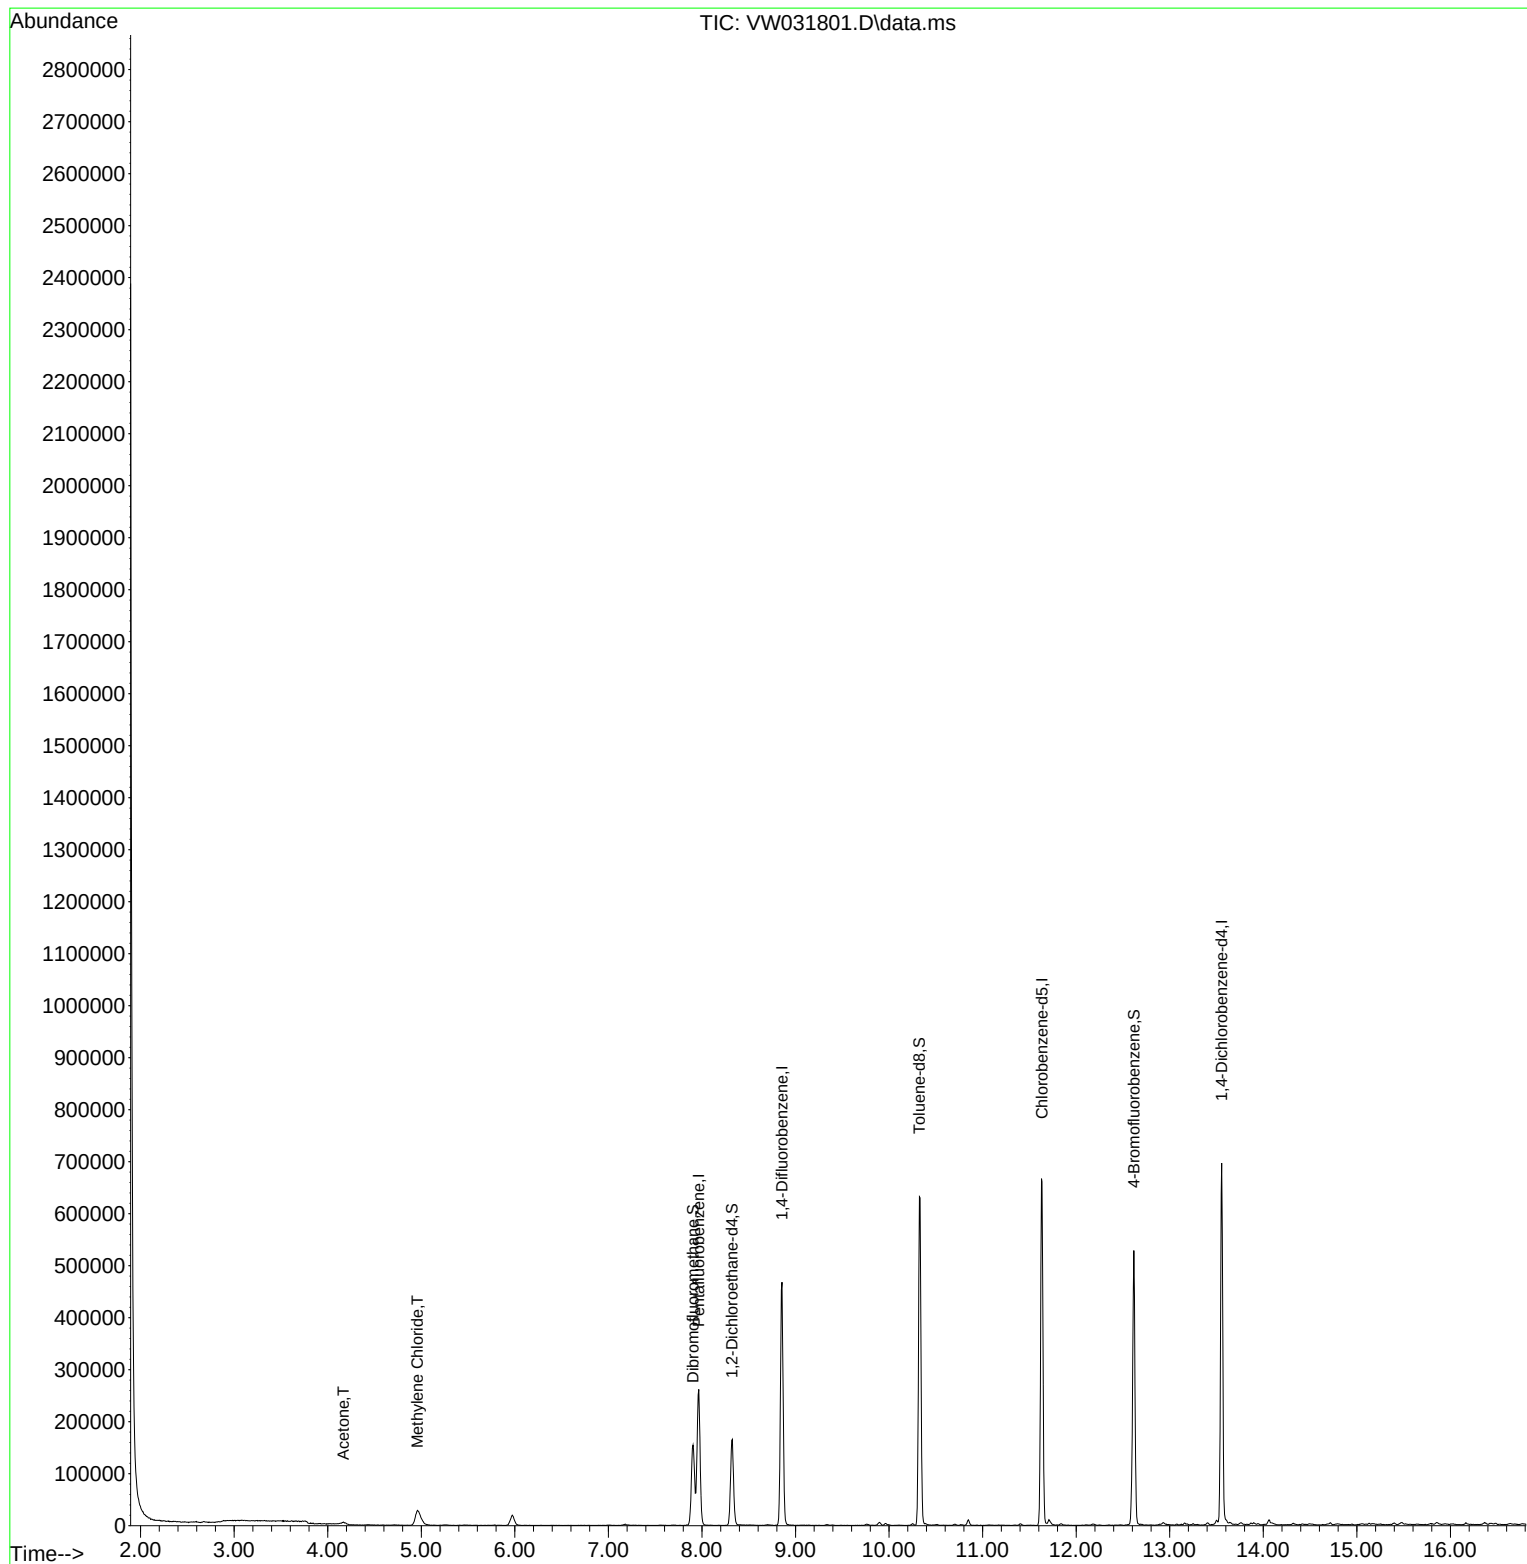


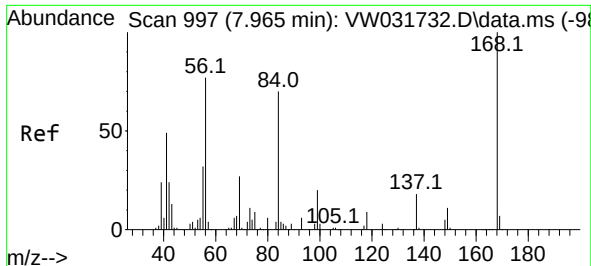

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.965 min Scan# 997
Delta R.T. 0.000 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30




Instrument :
MSVOA_W
ClientSampleId :
TP-89


Tgt Ion:168 Resp: 174642
Ion Ratio Lower Upper
168 100
99 67.7 49.4 74.2

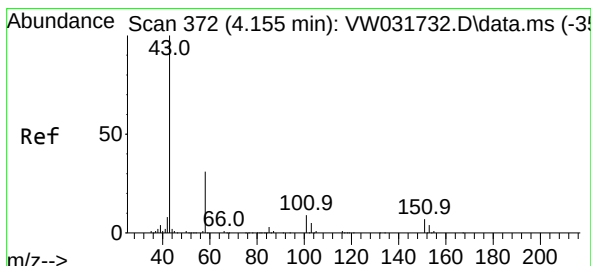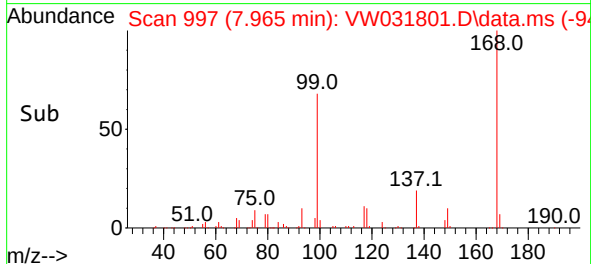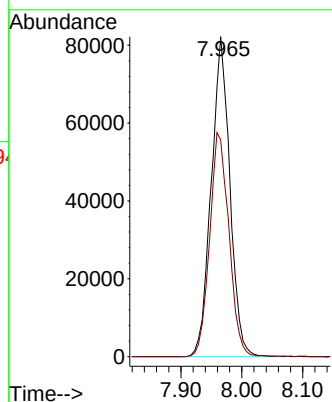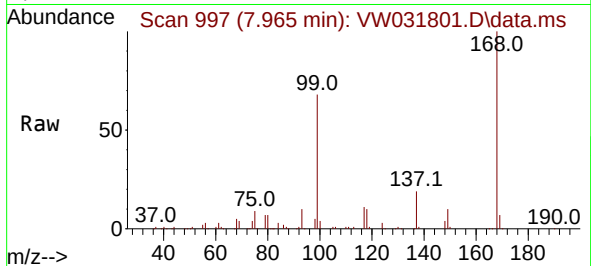

#16
Acetone
Concen: 11.778 ug/l
RT: 4.167 min Scan# 374
Delta R.T. 0.013 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30

Tgt Ion: 43 Resp: 7296
Ion Ratio Lower Upper
43 100
58 34.9 24.8 37.2


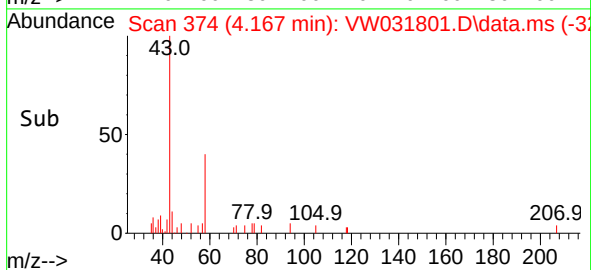
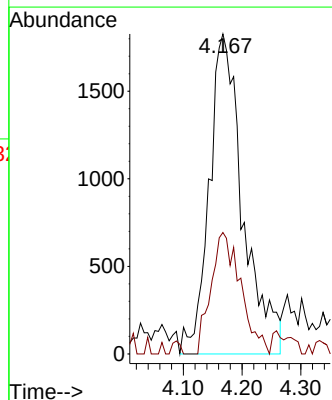
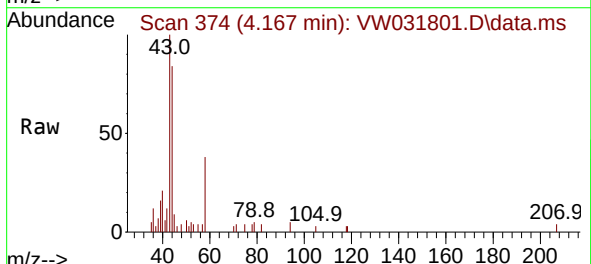


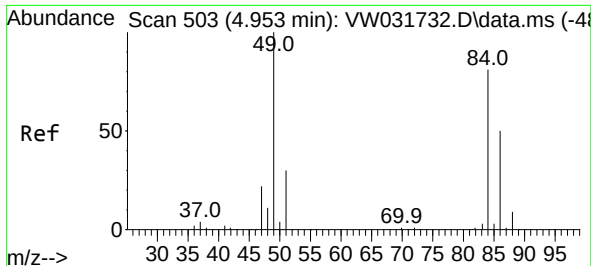

#20
Methylene Chloride
Concen: 6.489 ug/l
RT: 4.960 min Scan# 503
Delta R.T. 0.006 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30




Instrument :
MSVOA_W
ClientSampleId :
TP-89


Tgt Ion:	84	Resp:	25745
Ion	Ratio	Lower	Upper
84	100		
49	109.8	98.2	147.4
51	31.5	29.8	44.8
86	63.6	49.5	74.3

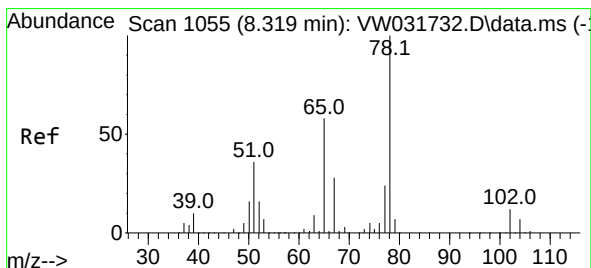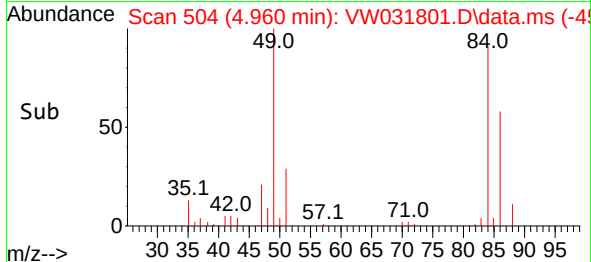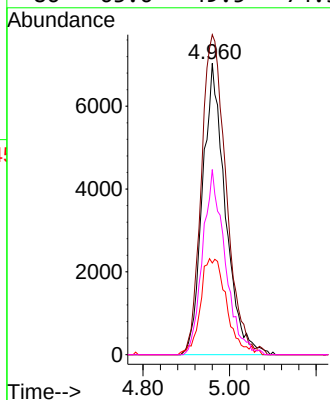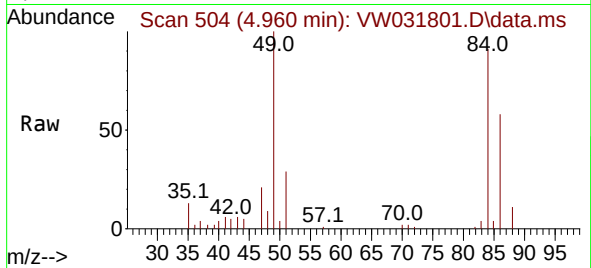

#33
1,2-Dichloroethane-d4
Concen: 55.083 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30

Tgt Ion:	65	Resp:	138054
Ion	Ratio	Lower	Upper
65	100		
67	51.1	0.0	99.4


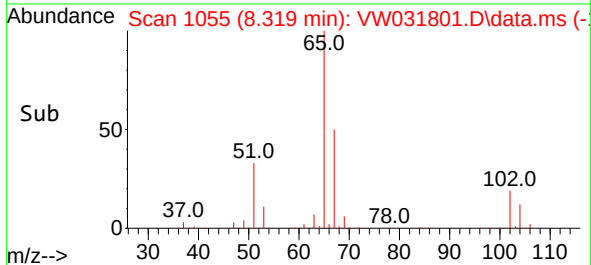
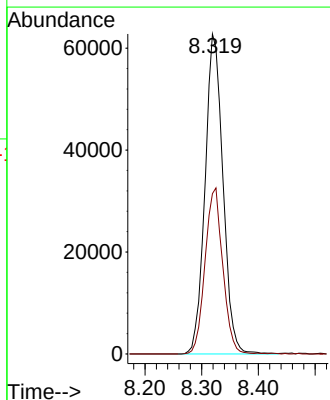
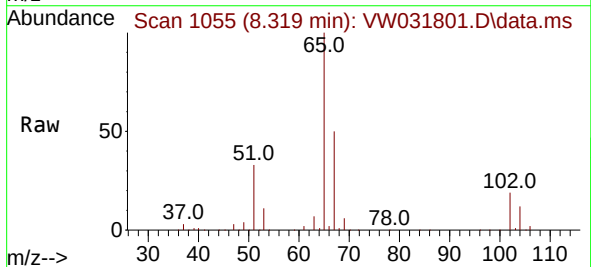


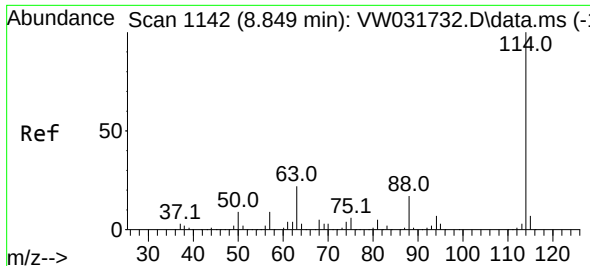

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.855 min Scan# 1143
 Delta R.T. 0.006 min
 Lab File: VW031801.D
 Acq: 10 Jul 2025 14:30




Instrument :
 MSVOA_W
 ClientSampleId :
 TP-89


Tgt	Ion:114	Resp:	393151
Ion	Ratio	Lower	Upper
114	100		
63	20.3	0.0	43.6
88	15.4	0.0	34.2

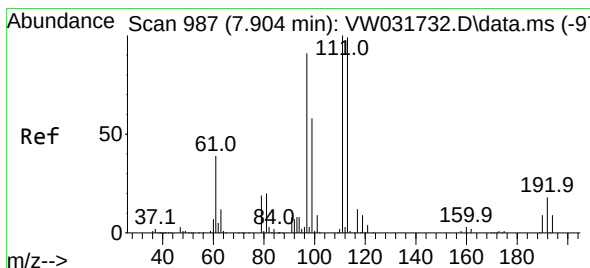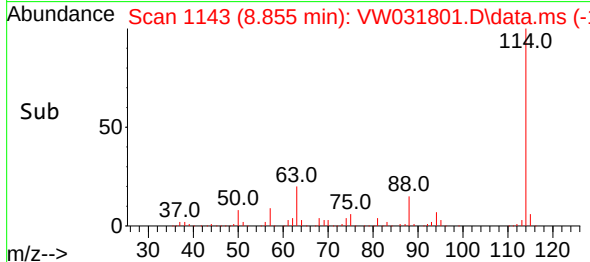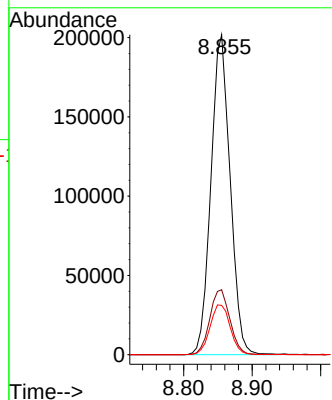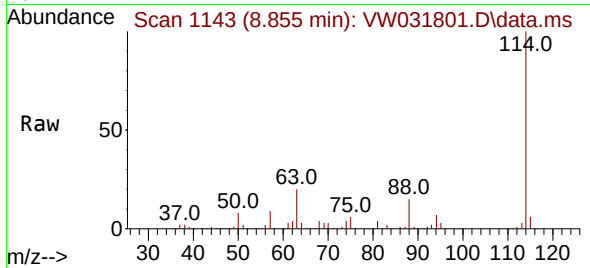

#35
 Dibromofluoromethane
 Concen: 45.503 ug/l
 RT: 7.904 min Scan# 987
 Delta R.T. 0.000 min
 Lab File: VW031801.D
 Acq: 10 Jul 2025 14:30

Tgt Ion:113	Resp:	116738	
Ion	Ratio	Lower	Upper
113	100		
111	103.3	82.1	123.1
192	15.3	13.8	20.6


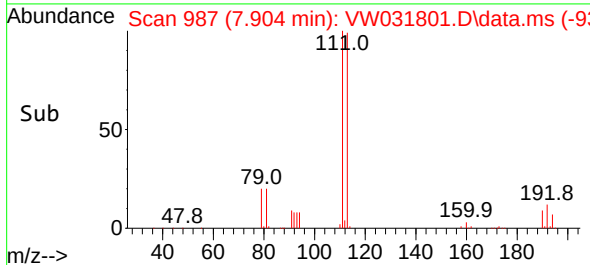
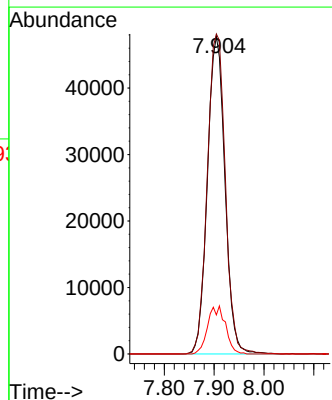
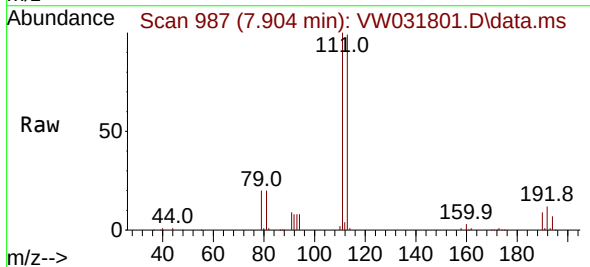


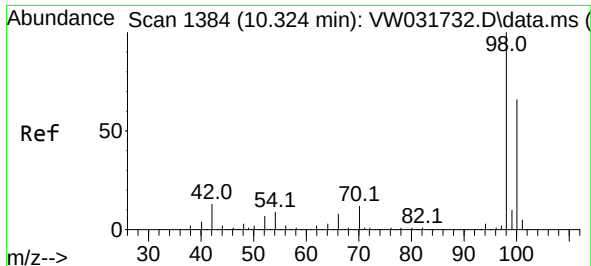

#50
Toluene-d8
Concen: 44.921 ug/l
RT: 10.325 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30




Instrument :
MSVOA_W
ClientSampleId :
TP-89


Tgt Ion: 98 Resp: 428866
Ion Ratio Lower Upper
98 100
100 64.8 53.0 79.4

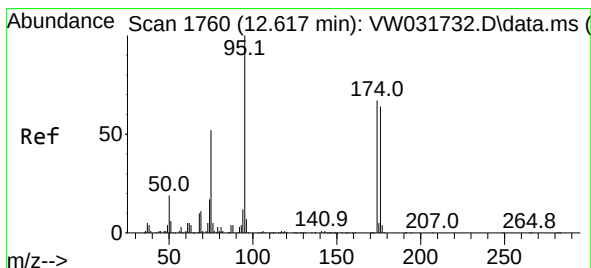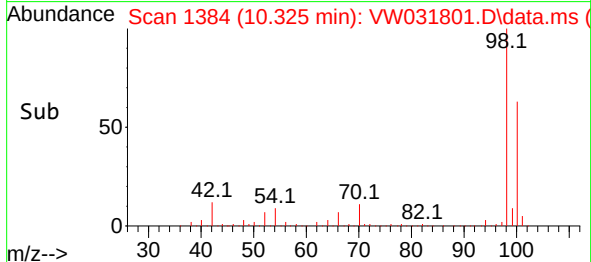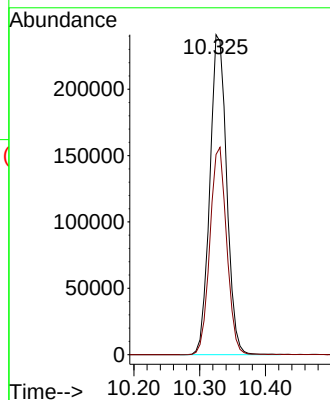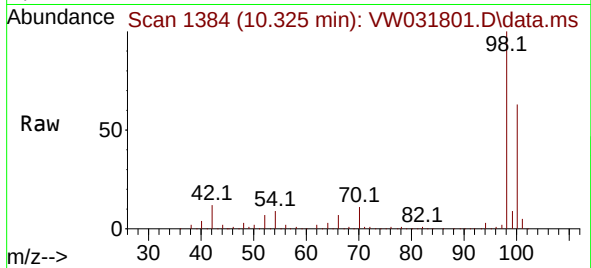

#62
4-Bromofluorobenzene
Concen: 48.749 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30

Tgt Ion: 95 Resp: 171272
Ion Ratio Lower Upper
95 100
174 63.8 0.0 133.8
176 65.6 0.0 126.0


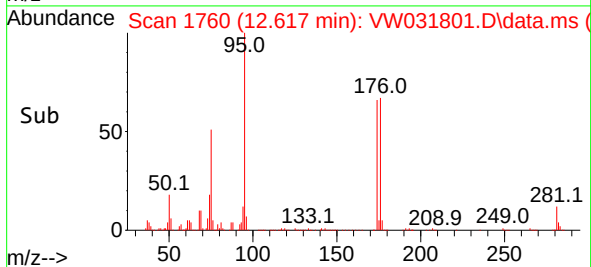
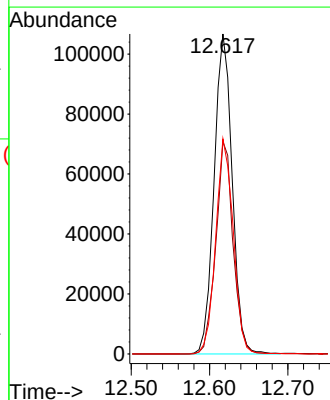
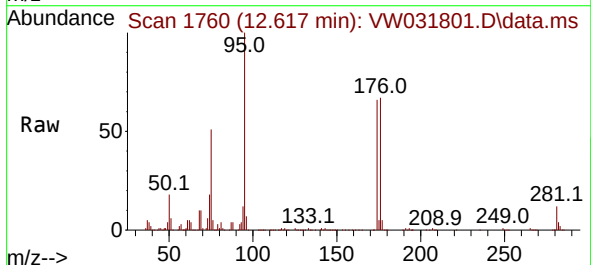


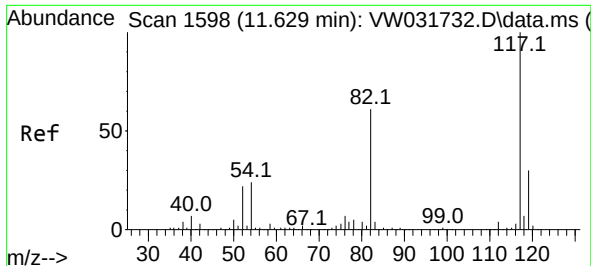

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.635 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30

Instrument :
MSVOA_W
ClientSampleId :
TP-89

Tgt Ion:117 Resp: 366298
Ion Ratio Lower Upper
117 100
82 56.5 48.6 72.8
119 29.3 23.9 35.9

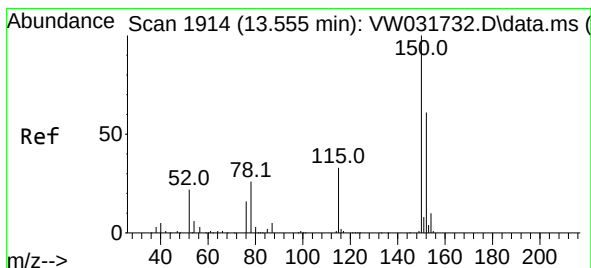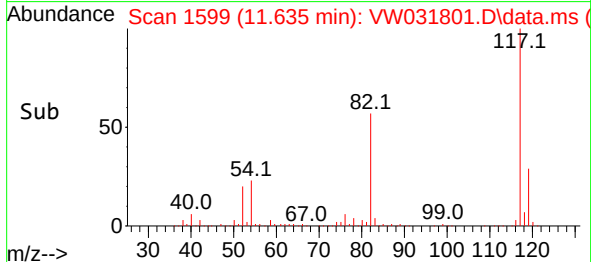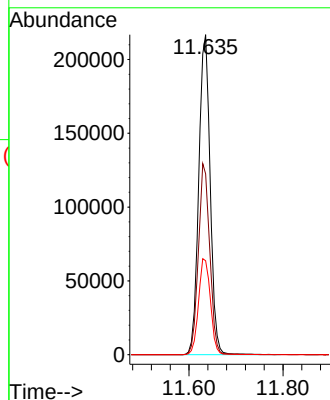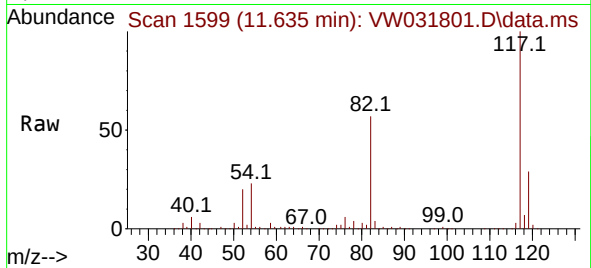

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. 0.000 min
Lab File: VW031801.D
Acq: 10 Jul 2025 14:30

Tgt Ion:152 Resp: 174003
Ion Ratio Lower Upper
152 100
115 64.4 31.9 95.7
150 158.2 0.0 356.4

