

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071122\
 Data File : VW023593.D
 Acq On : 11 Jul 2022 10:59
 Operator : SY/VA
 Sample : VW0711SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK540

Quant Time: Jul 12 01:42:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 12 01:39:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	318112	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	299360	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	140274	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	123363	21.423	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.680%
7) Chloroethane-d5	2.879	69	77066	23.400	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.600%
11) 1,1-Dichloroethene-d2	4.013	63	107237	16.518	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.080%
21) 2-Butanone-d5	7.080	46	53495	44.735	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.480%
24) Chloroform-d	7.653	84	209238	23.092	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.360%
26) 1,2-Dichloroethane-d4	8.519	65	62	0.012	ug/L	0.21
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.275	84	393737	23.771	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.080%
36) 1,2-Dichloropropane-d6	9.275	67	116342	23.991	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.960%
41) Toluene-d8	10.323	98	366553	22.831	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.320%
43) trans-1,3-Dichloroprop...	10.579	79	48318	22.321	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.280%
47) 2-Hexanone-d5	10.921	63	39664	41.820	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.640%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	104486	21.718	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	124996	24.698	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.800%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4456	0.643	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071122\
Data File : VW023593.D
Acq On : 11 Jul 2022 10:59
Operator : SY/VA
Sample : VW0711SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK540

Quant Time: Jul 12 01:42:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 12 01:39:48 2022
Response via : Initial Calibration

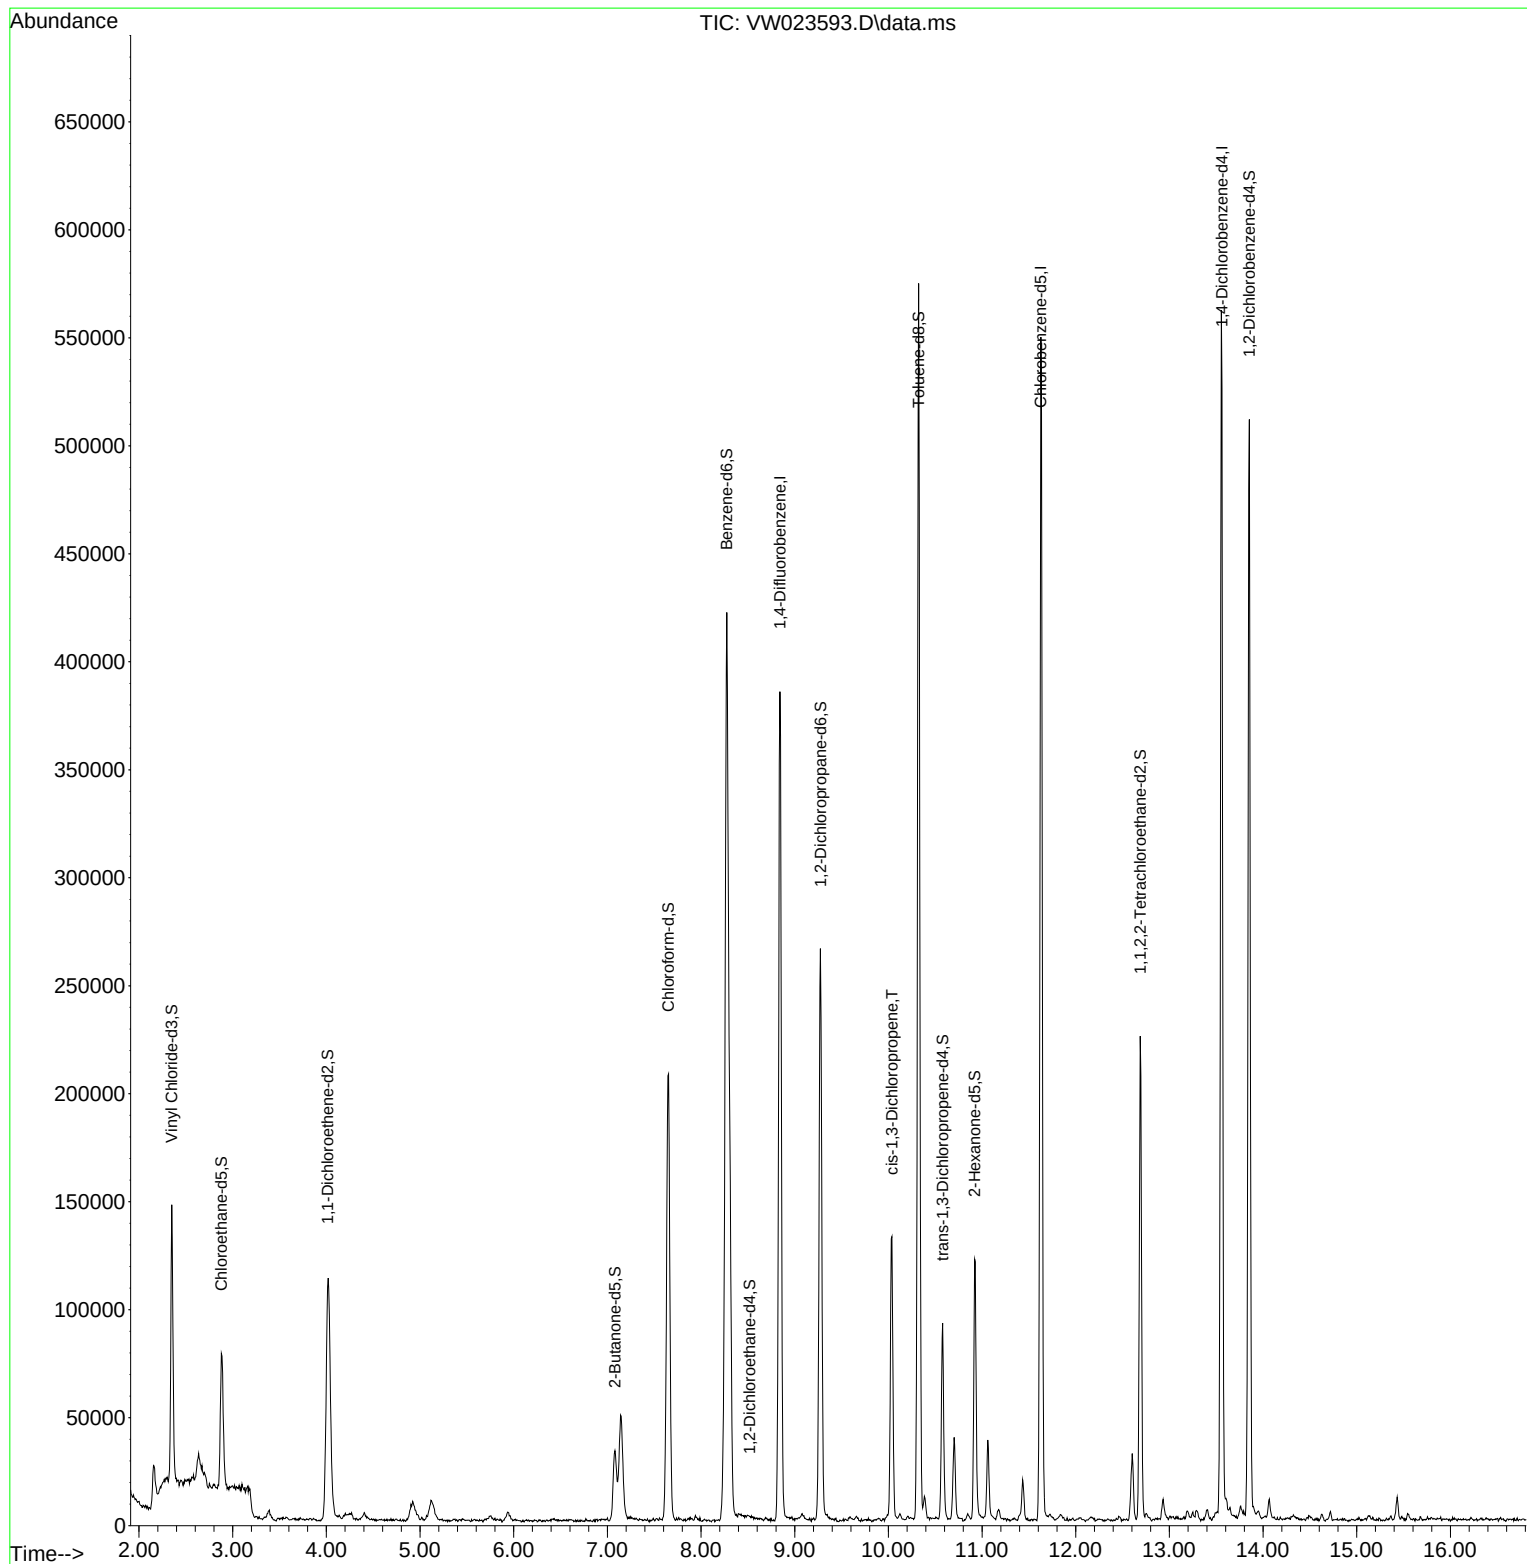

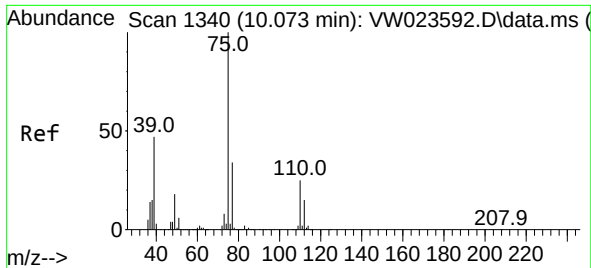

#39
 cis-1,3-Dichloropropene
 Concen: 0.643 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW023593.D
 Acq: 11 Jul 2022 10:59

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK540

Tgt Ion: 75 Resp: 4456
 Ion Ratio Lower Upper
 75 100
 77 53.2 23.0 42.6#

