

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071122\
 Data File : VW023594.D
 Acq On : 11 Jul 2022 11:23
 Operator : SY/VA
 Sample : N3626-07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 12 01:42:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 12 01:39:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	325183	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	311335	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	143132	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	121666	20.669	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.680%
7) Chloroethane-d5	2.879	69	64478	19.152	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.600%
11) 1,1-Dichloroethene-d2	4.129	63	346	0.052	ug/L	0.10
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.200%#
21) 2-Butanone-d5	7.080	46	48914	40.015	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.040%
24) Chloroform-d	7.647	84	199636	21.553	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.200%
26) 1,2-Dichloroethane-d4	8.494	65	189	0.036	ug/L	0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.275	84	381262	22.133	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.520%
36) 1,2-Dichloropropane-d6	9.275	67	110746	21.959	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.840%
41) Toluene-d8	10.323	98	349278	20.918	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.680%
43) trans-1,3-Dichloroprop...	10.579	79	45425	20.178	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.720%
47) 2-Hexanone-d5	10.921	63	36534	37.039	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.080%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	95940	19.175	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.680%
66) 1,2-Dichlorobenzene-d4	13.853	152	119351	23.112	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.440%
Target Compounds						
39) cis-1,3-Dichloropropene	10.037	75	4180	0.580	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071122\
Data File : VW023594.D
Acq On : 11 Jul 2022 11:23
Operator : SY/VA
Sample : N3626-07
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Jul 12 01:42:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 12 01:39:48 2022
Response via : Initial Calibration

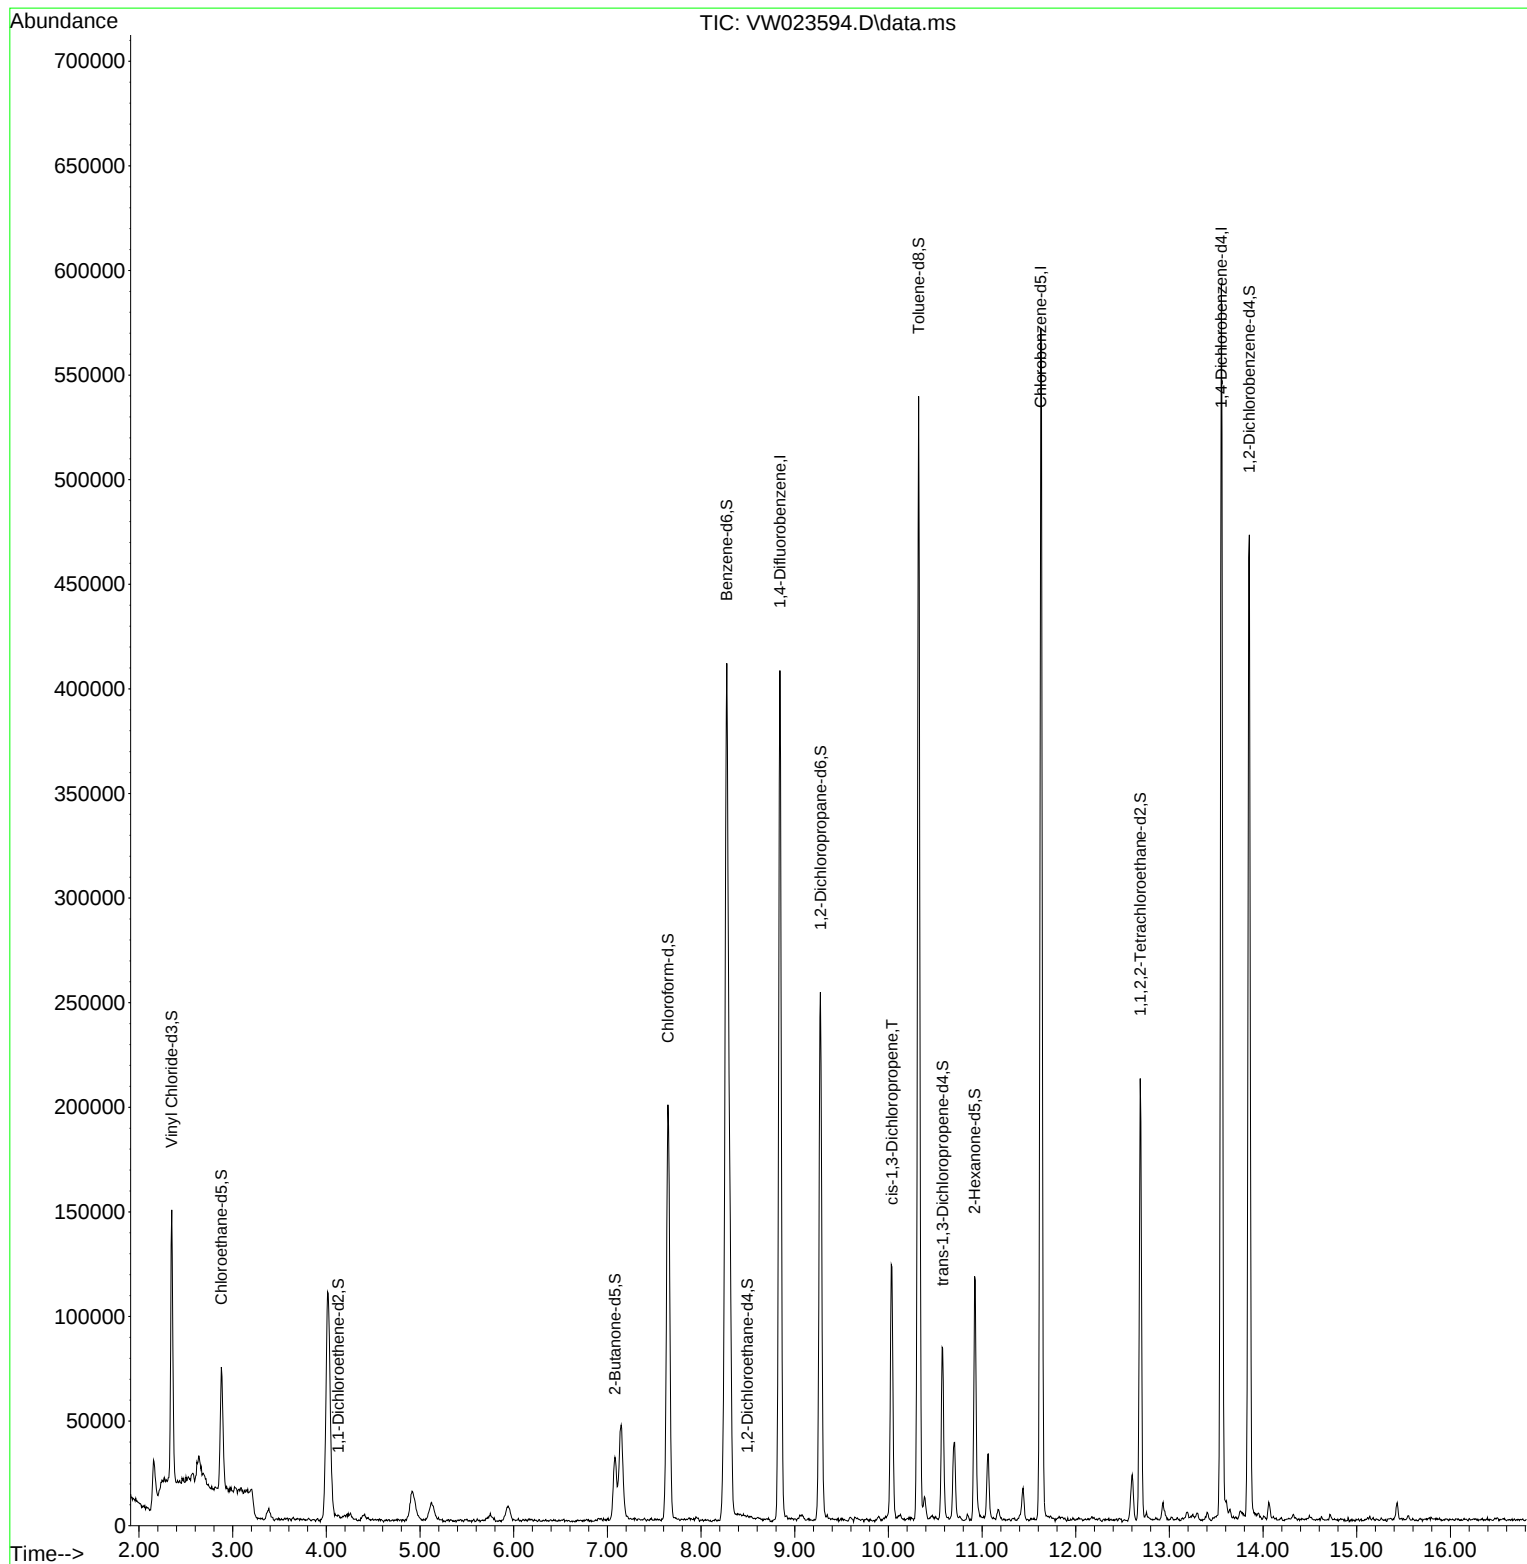

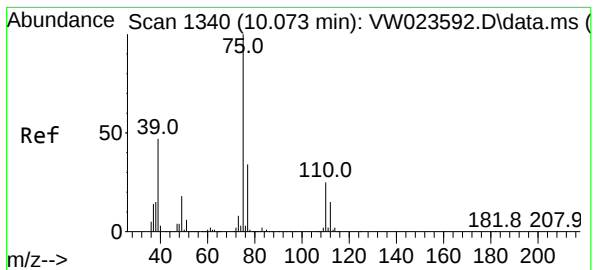

#39
 cis-1,3-Dichloropropene
 Concen: 0.580 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW023594.D
 Acq: 11 Jul 2022 11:23

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion:	75	Resp:	4180
Ion	Ratio	Lower	Upper
75	100		
77	42.6	23.0	42.6

