

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071125\
 Data File : VW031822.D
 Acq On : 11 Jul 2025 16:10
 Operator : SY/MD
 Sample : Q2542-01
 Misc : 5.00g/5mL/MSVOA_W/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VNJ-245

Quant Time: Jul 11 22:49:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:35:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.965	168	167452	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	360619	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.636	117	343947	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	165000	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	139262	57.950	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	115.900%
35) Dibromofluoromethane	7.904	113	116912	49.682	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	99.360%
50) Toluene-d8	10.331	98	411542	46.995	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	93.980%
62) 4-Bromofluorobenzene	12.617	95	152271	47.250	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	94.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071125\
Data File : VW031822.D
Acq On : 11 Jul 2025 16:10
Operator : SY/MD
Sample : Q2542-01
Misc : 5.00g/5mL/MSVOA_W/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VNJ-245

Quant Time: Jul 11 22:49:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:35:17 2025
Response via : Initial Calibration




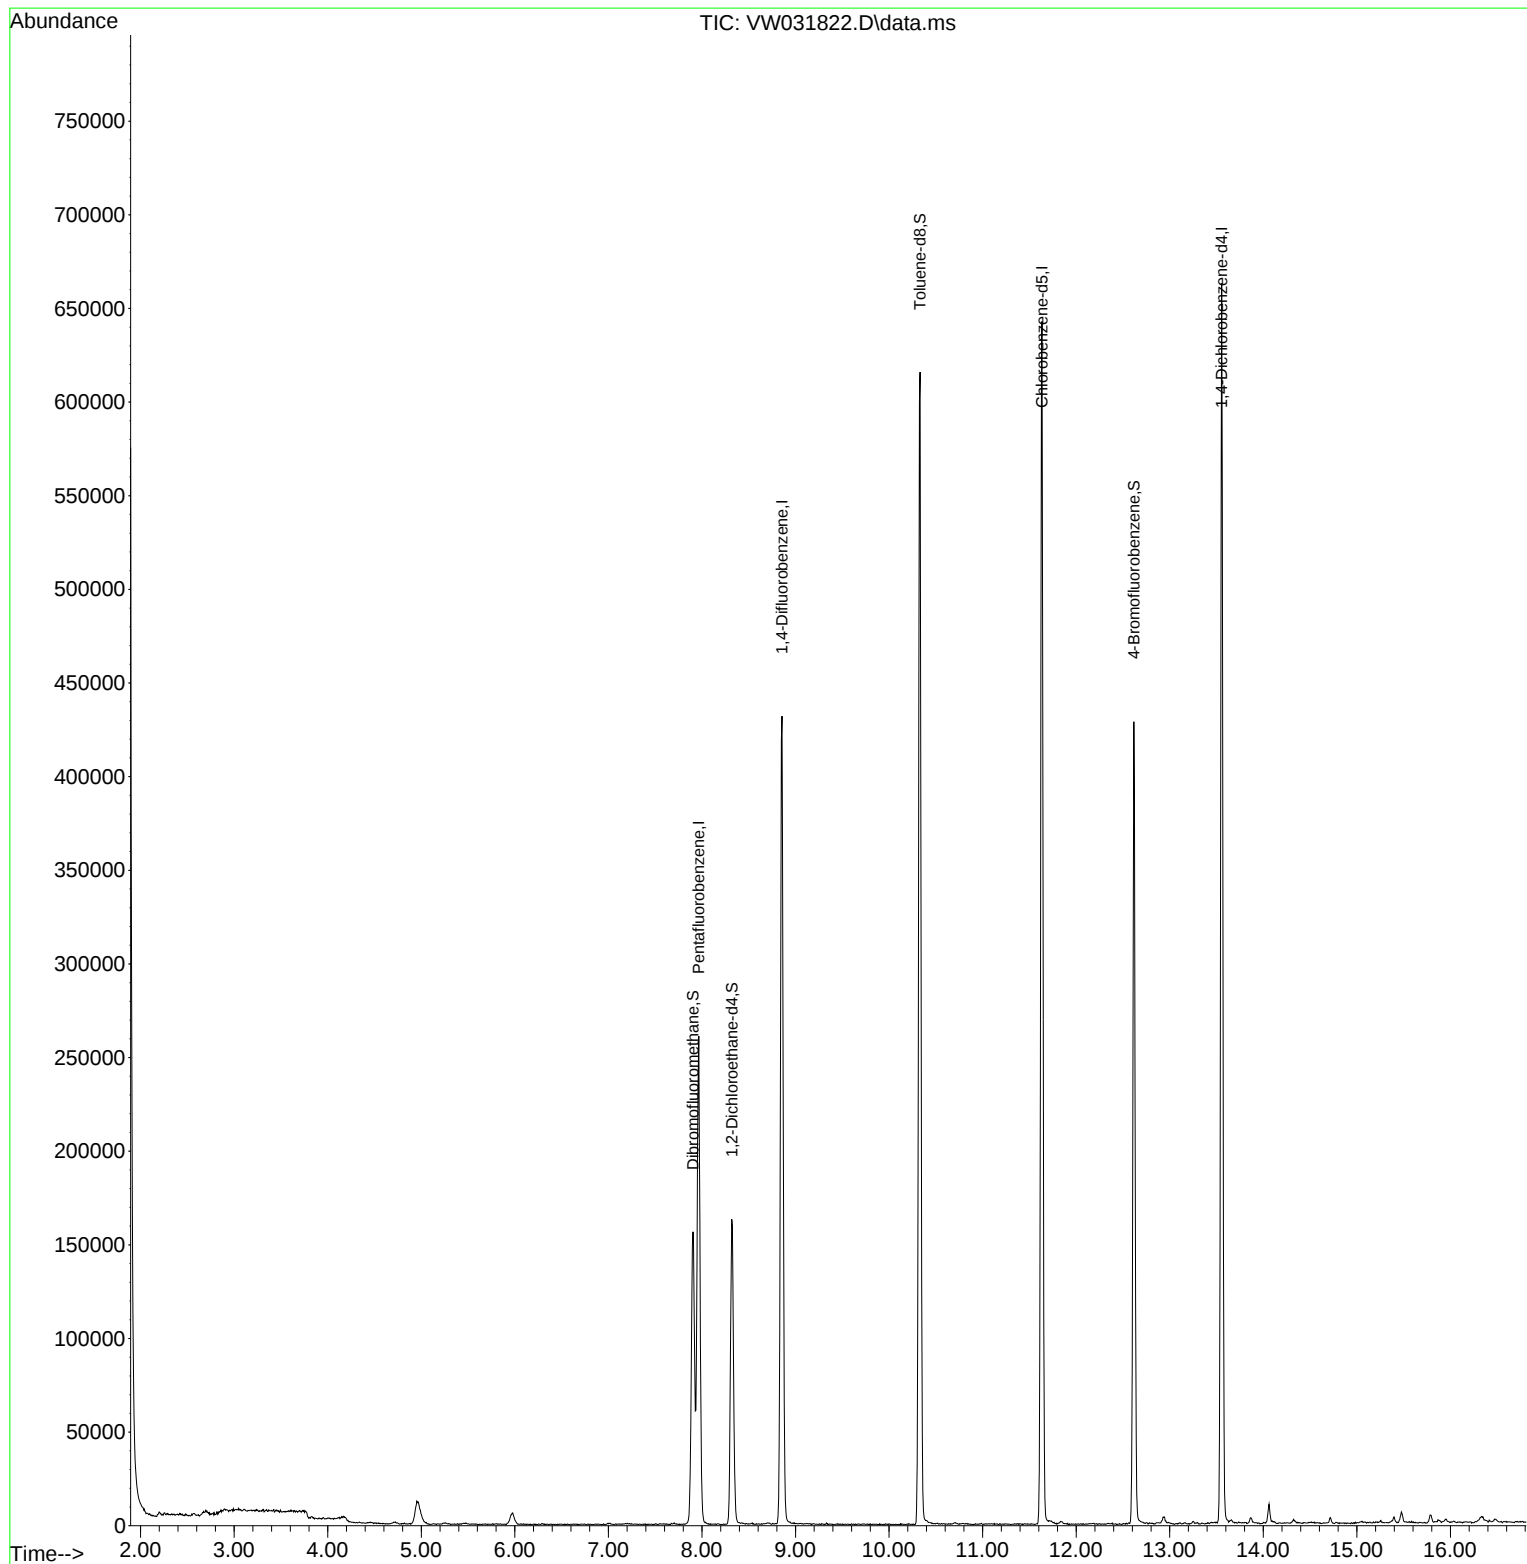


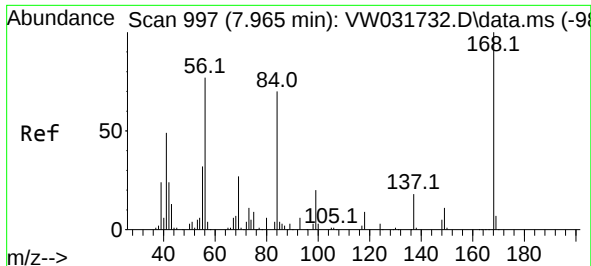

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.965 min Scan# 997
Delta R.T. 0.000 min
Lab File: VW031822.D
Acq: 11 Jul 2025 16:10




Instrument :
MSVOA_W
ClientSampleId :
VNJ-245


Tgt Ion:168 Resp: 167452
Ion Ratio Lower Upper
168 100
99 63.6 49.4 74.2

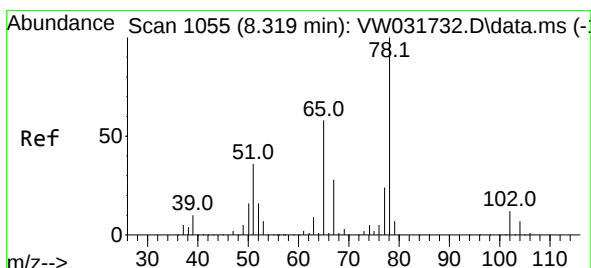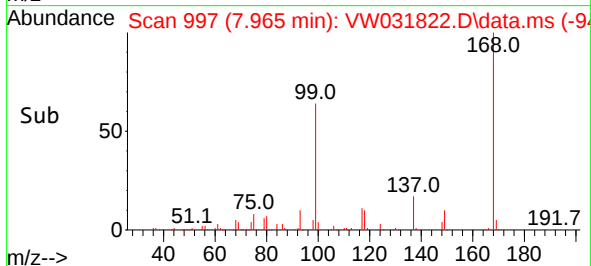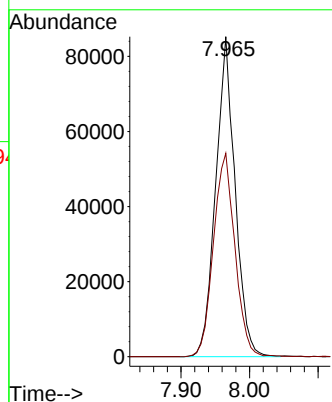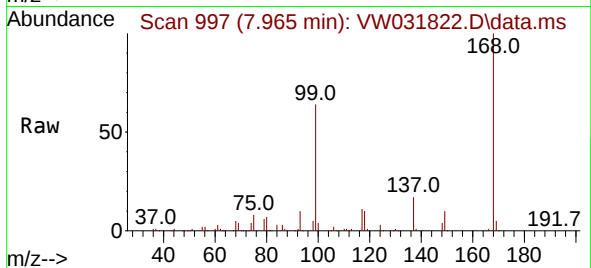

#33
1,2-Dichloroethane-d4
Concen: 57.950 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW031822.D
Acq: 11 Jul 2025 16:10

Tgt Ion: 65 Resp: 139262
Ion Ratio Lower Upper
65 100
67 49.2 0.0 99.4

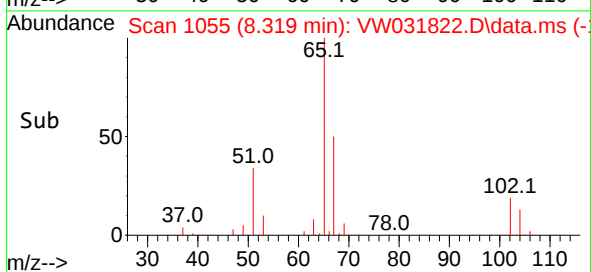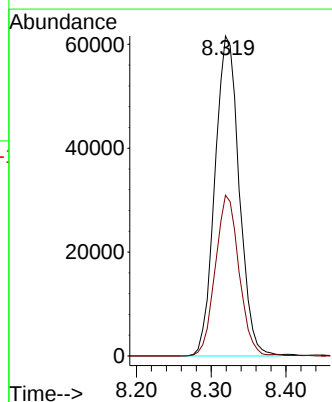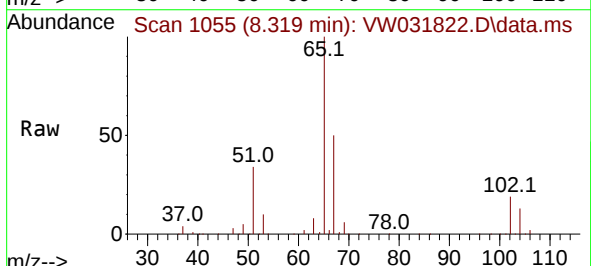

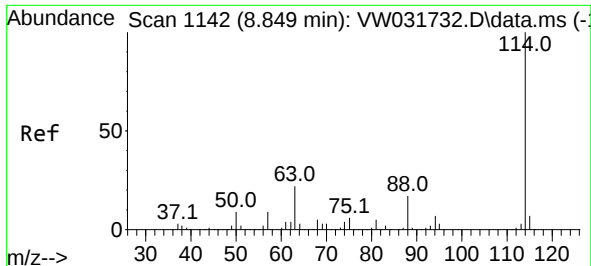

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1142

Delta R.T. 0.006 min

Lab File: VW031822.D

Acq: 11 Jul 2025 16:10

Instrument :

MSVOA_W

ClientSampleId :

VNJ-245





Tgt Ion:114 Resp: 360619

Ion Ratio Lower Upper

114 100

63 21.6 0.0 43.6

88 17.3 0.0 34.2

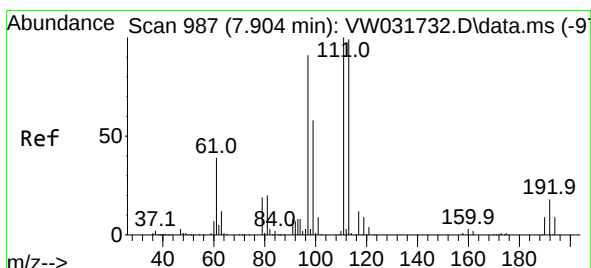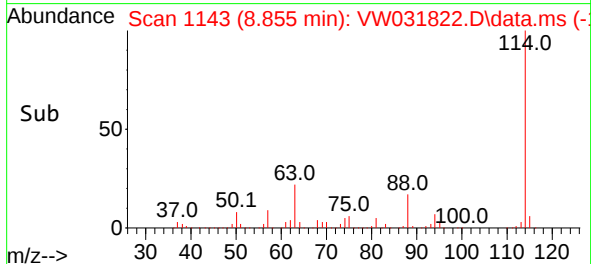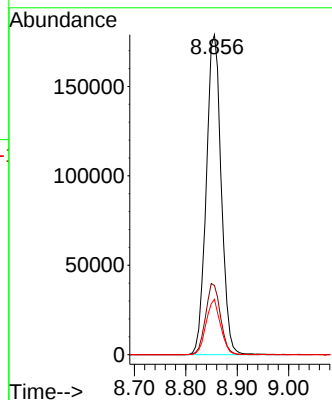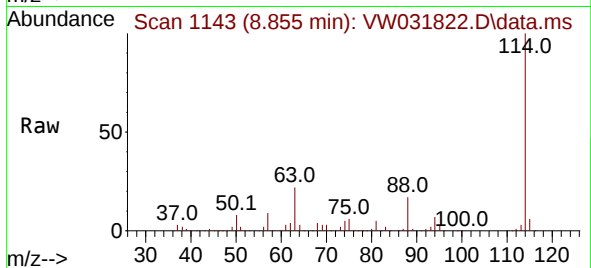

#35

Dibromofluoromethane

Concen: 49.682 ug/l

RT: 7.904 min Scan# 987

Delta R.T. 0.000 min

Lab File: VW031822.D

Acq: 11 Jul 2025 16:10




Tgt Ion:113 Resp: 116912


Ion Ratio Lower Upper

113 100

111 103.1 82.1 123.1

192 15.8 13.8 20.6


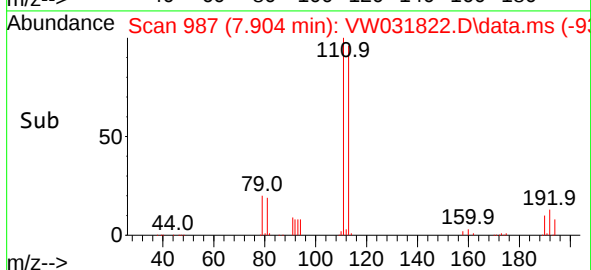
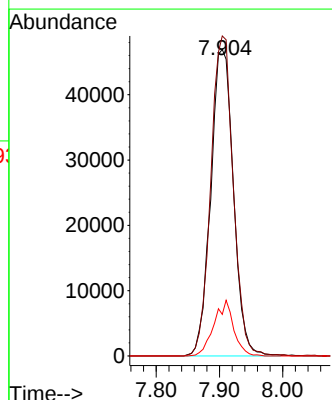
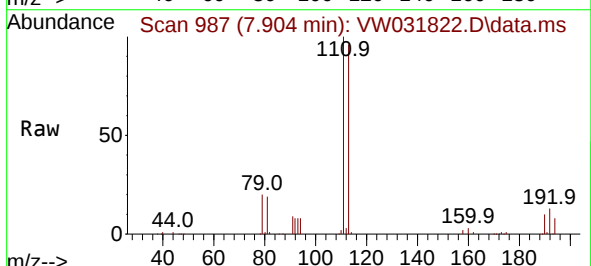


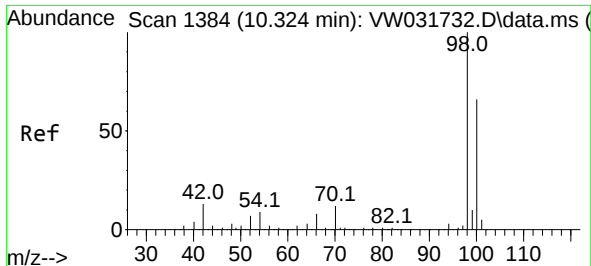

#50
Toluene-d8
Concen: 46.995 ug/l
RT: 10.331 min Scan# 1
Delta R.T. 0.006 min
Lab File: VW031822.D
Acq: 11 Jul 2025 16:10




Instrument :
MSVOA_W
ClientSampleId :
VNJ-245


Tgt Ion: 98 Resp: 411542
Ion Ratio Lower Upper
98 100
100 63.8 53.0 79.4

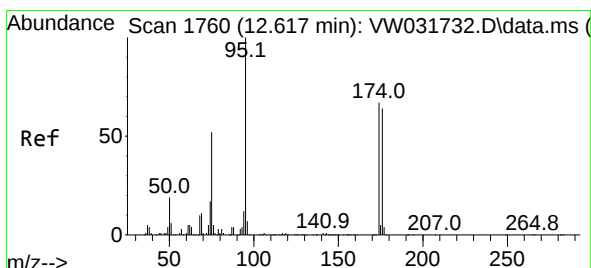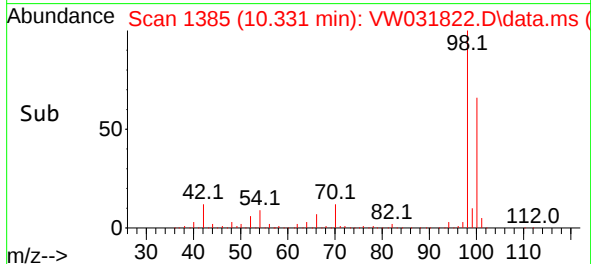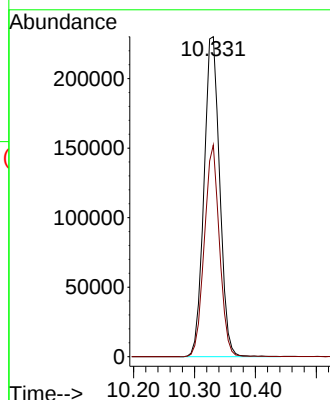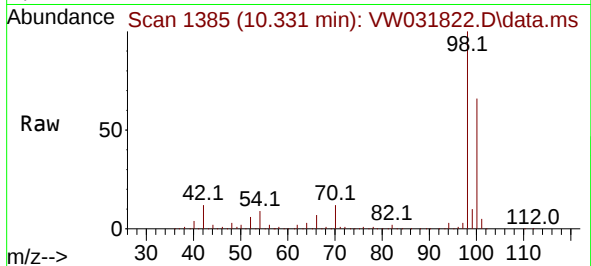

#62
4-Bromofluorobenzene
Concen: 47.250 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW031822.D
Acq: 11 Jul 2025 16:10

Tgt Ion: 95 Resp: 152271
Ion Ratio Lower Upper
95 100
174 65.9 0.0 133.8
176 59.6 0.0 126.0


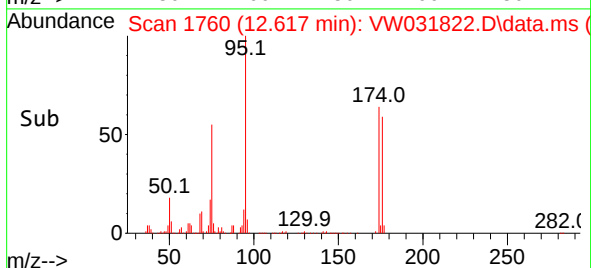
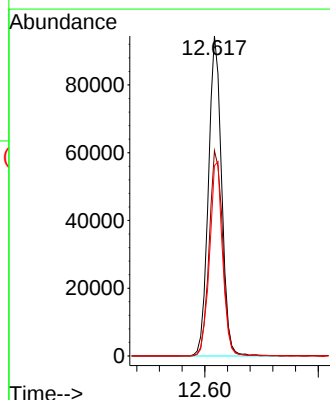
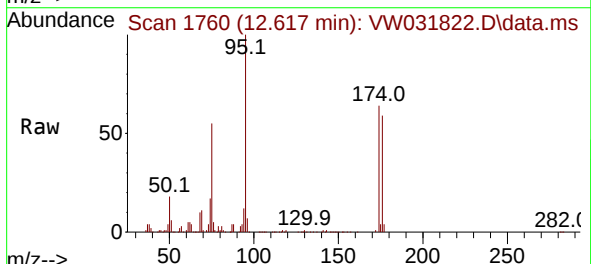


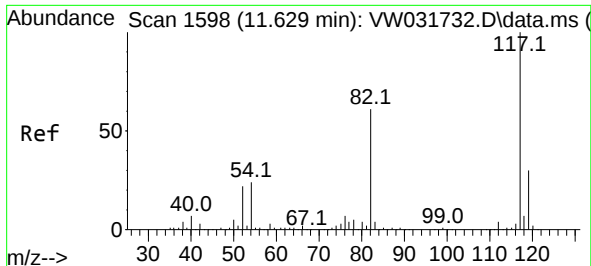

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.636 min Scan# 11
Delta R.T. 0.007 min
Lab File: VW031822.D
Acq: 11 Jul 2025 16:10

Instrument :
MSVOA_W
ClientSampleId :
VNJ-245

Tgt Ion:117 Resp: 343947
Ion Ratio Lower Upper
117 100
82 57.4 48.6 72.8
119 30.9 23.9 35.9

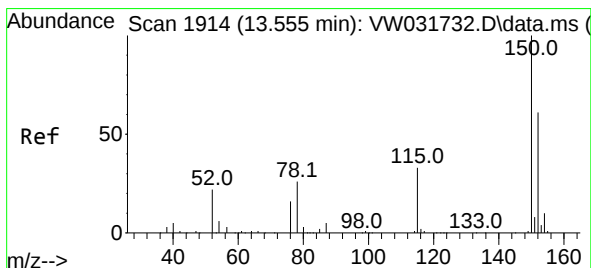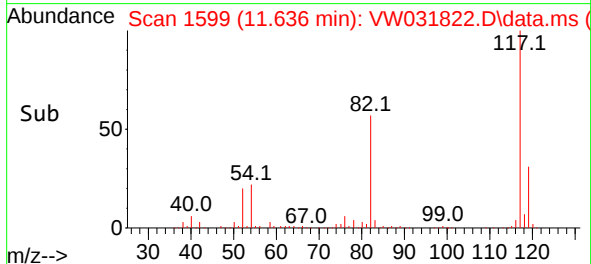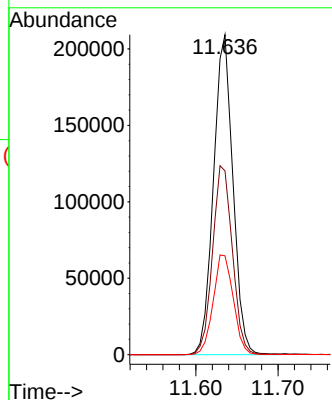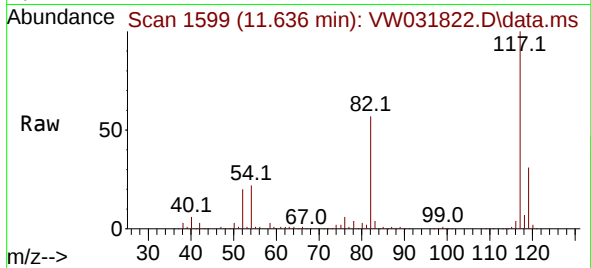

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. 0.000 min
Lab File: VW031822.D
Acq: 11 Jul 2025 16:10

Tgt Ion:152 Resp: 165000
Ion Ratio Lower Upper
152 100
115 65.4 31.9 95.7
150 151.3 0.0 356.4

