

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023613.D
 Acq On : 12 Jul 2022 18:16
 Operator : SY/VA
 Sample : N3676-13
 Misc : 4.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B12

Quant Time: Jul 13 01:35:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 01:31:49 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	81466	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	76230	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	28682	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.343	65	37783	25.621	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.480%	
7) Chloroethane-d5		2.879	69	26051	30.888	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	123.560%	
11) 1,1-Dichloroethene-d2		4.001	63	36256	21.807	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.240%	
21) 2-Butanone-d5		7.080	46	21541	70.341	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	140.680%#	
24) Chloroform-d		7.647	84	60287	25.981	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.920%	
26) 1,2-Dichloroethane-d4		8.451	65	95	0.072	ug/L	0.15
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.280%#	
32) Benzene-d6		8.275	84	105369	24.982	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.920%	
36) 1,2-Dichloropropane-d6		9.274	67	34023	27.552	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.200%	
41) Toluene-d8		10.323	98	86823	21.237	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.960%	
43) trans-1,3-Dichloroprop...		10.579	79	12091	21.935	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.760%	
47) 2-Hexanone-d5		10.927	63	12508	51.790	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.580%	
56) 1,1,2,2-Tetrachloroeth...		12.695	84	37354	30.491	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.960%#	
66) 1,2-Dichlorobenzene-d4		13.853	152	27491	26.566	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.280%	
Target Compounds							Qvalue
13) Acetone		4.135	43	12455	55.185	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023613.D
Acq On : 12 Jul 2022 18:16
Operator : SY/VA
Sample : N3676-13
Misc : 4.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B12


Quant Time: Jul 13 01:35:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 01:31:49 2022
Response via : Initial Calibration

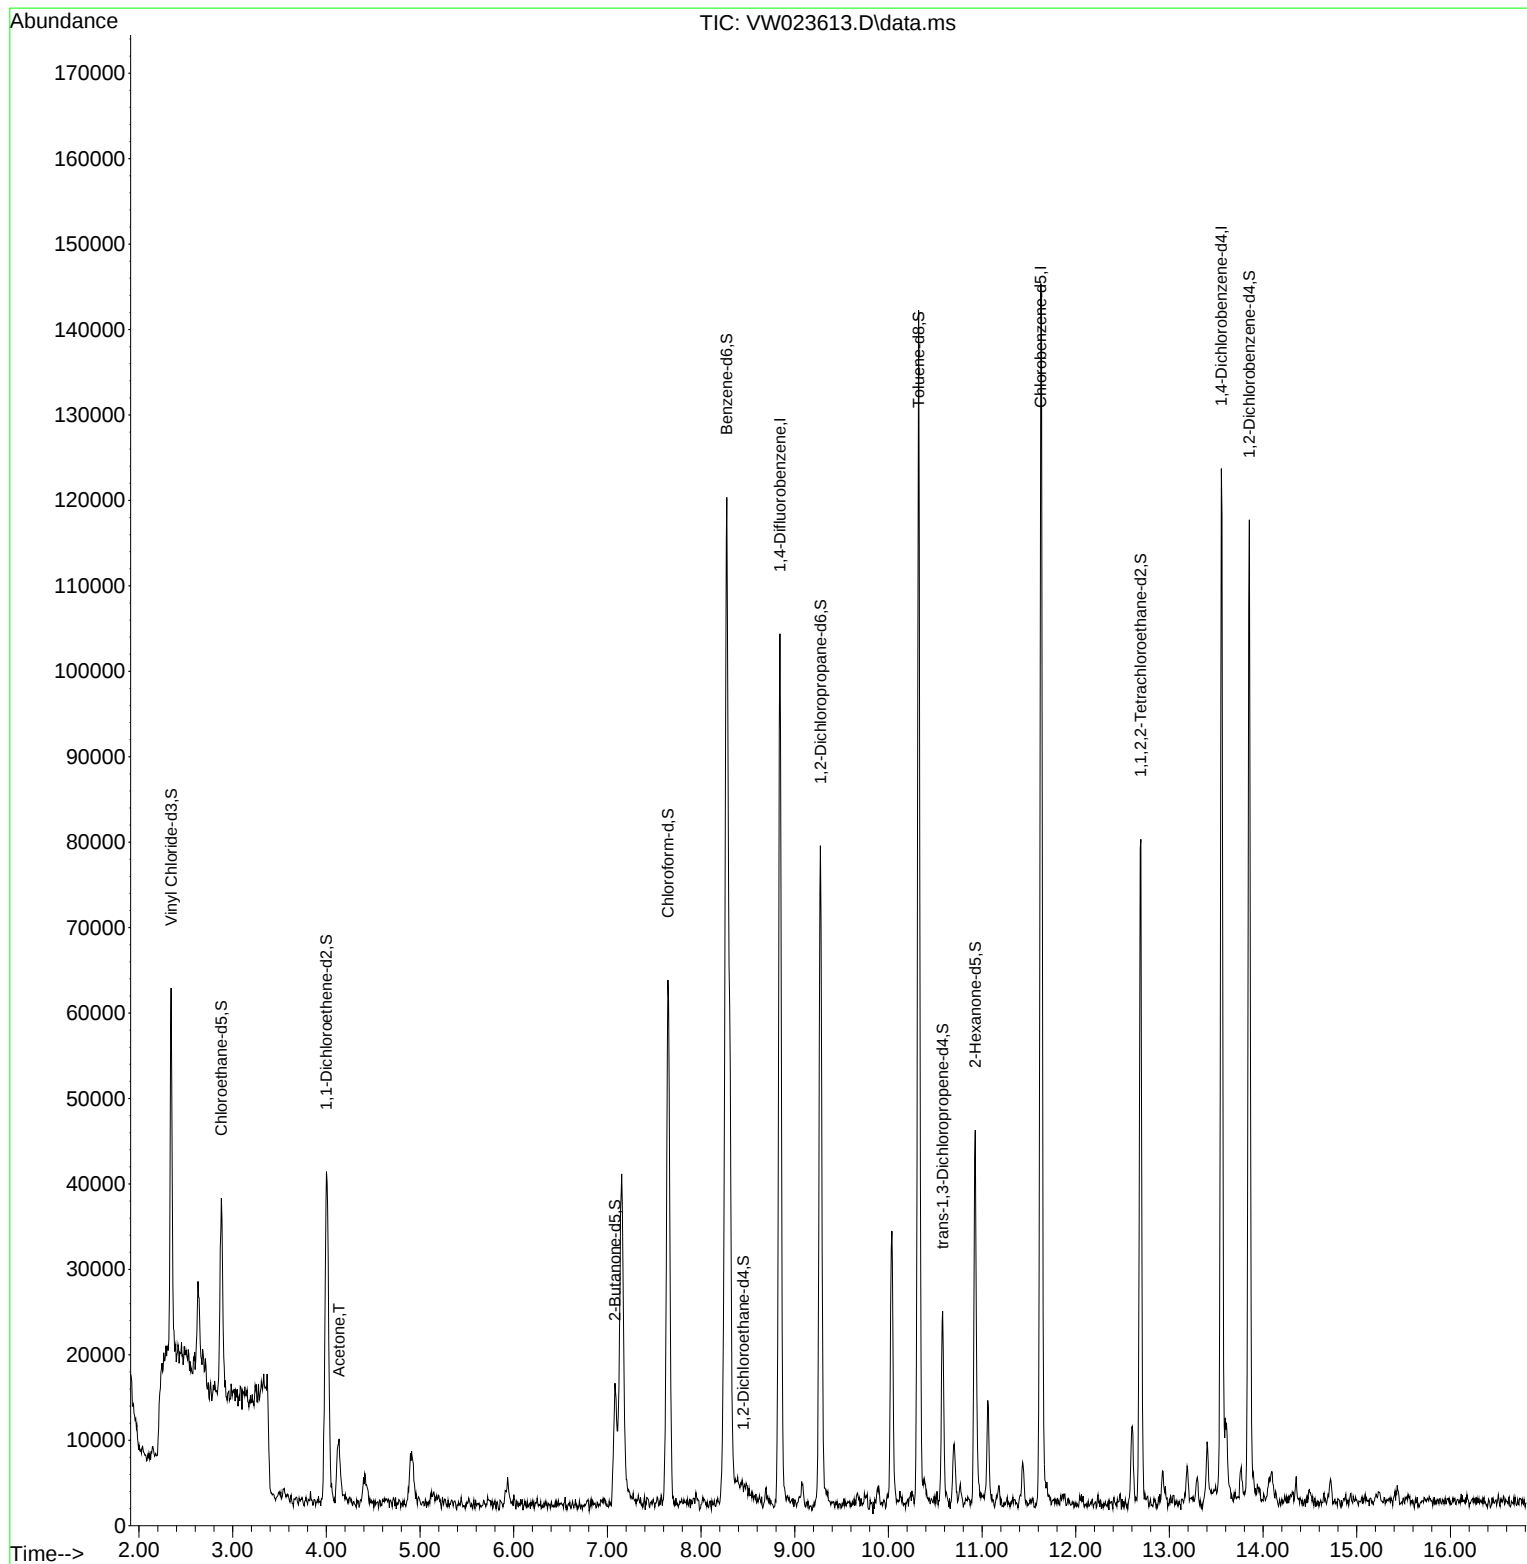

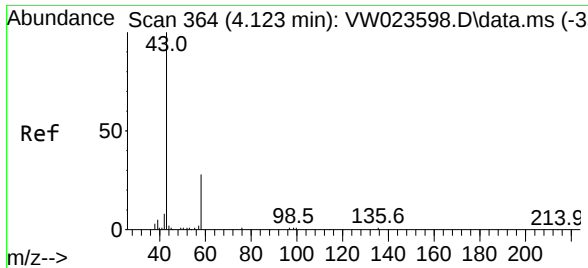

#13
 Acetone
 Concen: 55.185 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023613.D
 Acq: 12 Jul 2022 18:16

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B12

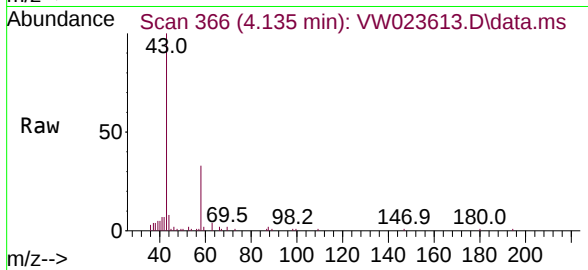

Tgt Ion: 43 Resp: 12455
 Ion Ratio Lower Upper
 43 100
 58 20.0 0.0 61.2

