

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023620.D
 Acq On : 12 Jul 2022 22:11
 Operator : SY/VA
 Sample : N3676-18
 Misc : 6.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B17

Quant Time: Jul 13 06:12:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 02:42:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	367595	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	339334	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	146296	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	131956	19.831	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.320%
7) Chloroethane-d5	2.879	69	88282	23.198	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.800%
11) 1,1-Dichloroethene-d2	4.013	63	108646	14.482	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.920%
21) 2-Butanone-d5	7.080	46	72101	52.178	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.360%
24) Chloroform-d	7.647	84	234840	22.429	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.720%
26) 1,2-Dichloroethane-d4	8.415	65	291	0.049	ug/L	0.11
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	435406	23.190	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.760%
36) 1,2-Dichloropropane-d6	9.275	67	137226	24.964	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.840%
41) Toluene-d8	10.323	98	394196	21.660	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.640%
43) trans-1,3-Dichloroprop...	10.579	79	46985	19.149	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.600%
47) 2-Hexanone-d5	10.927	63	58327	54.253	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.500%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	136438	25.019	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	129915	24.614	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.440%
Target Compounds					Qvalue	
13) Acetone	4.135	43	13074	12.838	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023620.D
Acq On : 12 Jul 2022 22:11
Operator : SY/VA
Sample : N3676-18
Misc : 6.61g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B17

Quant Time: Jul 13 06:12:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 02:42:59 2022
Response via : Initial Calibration

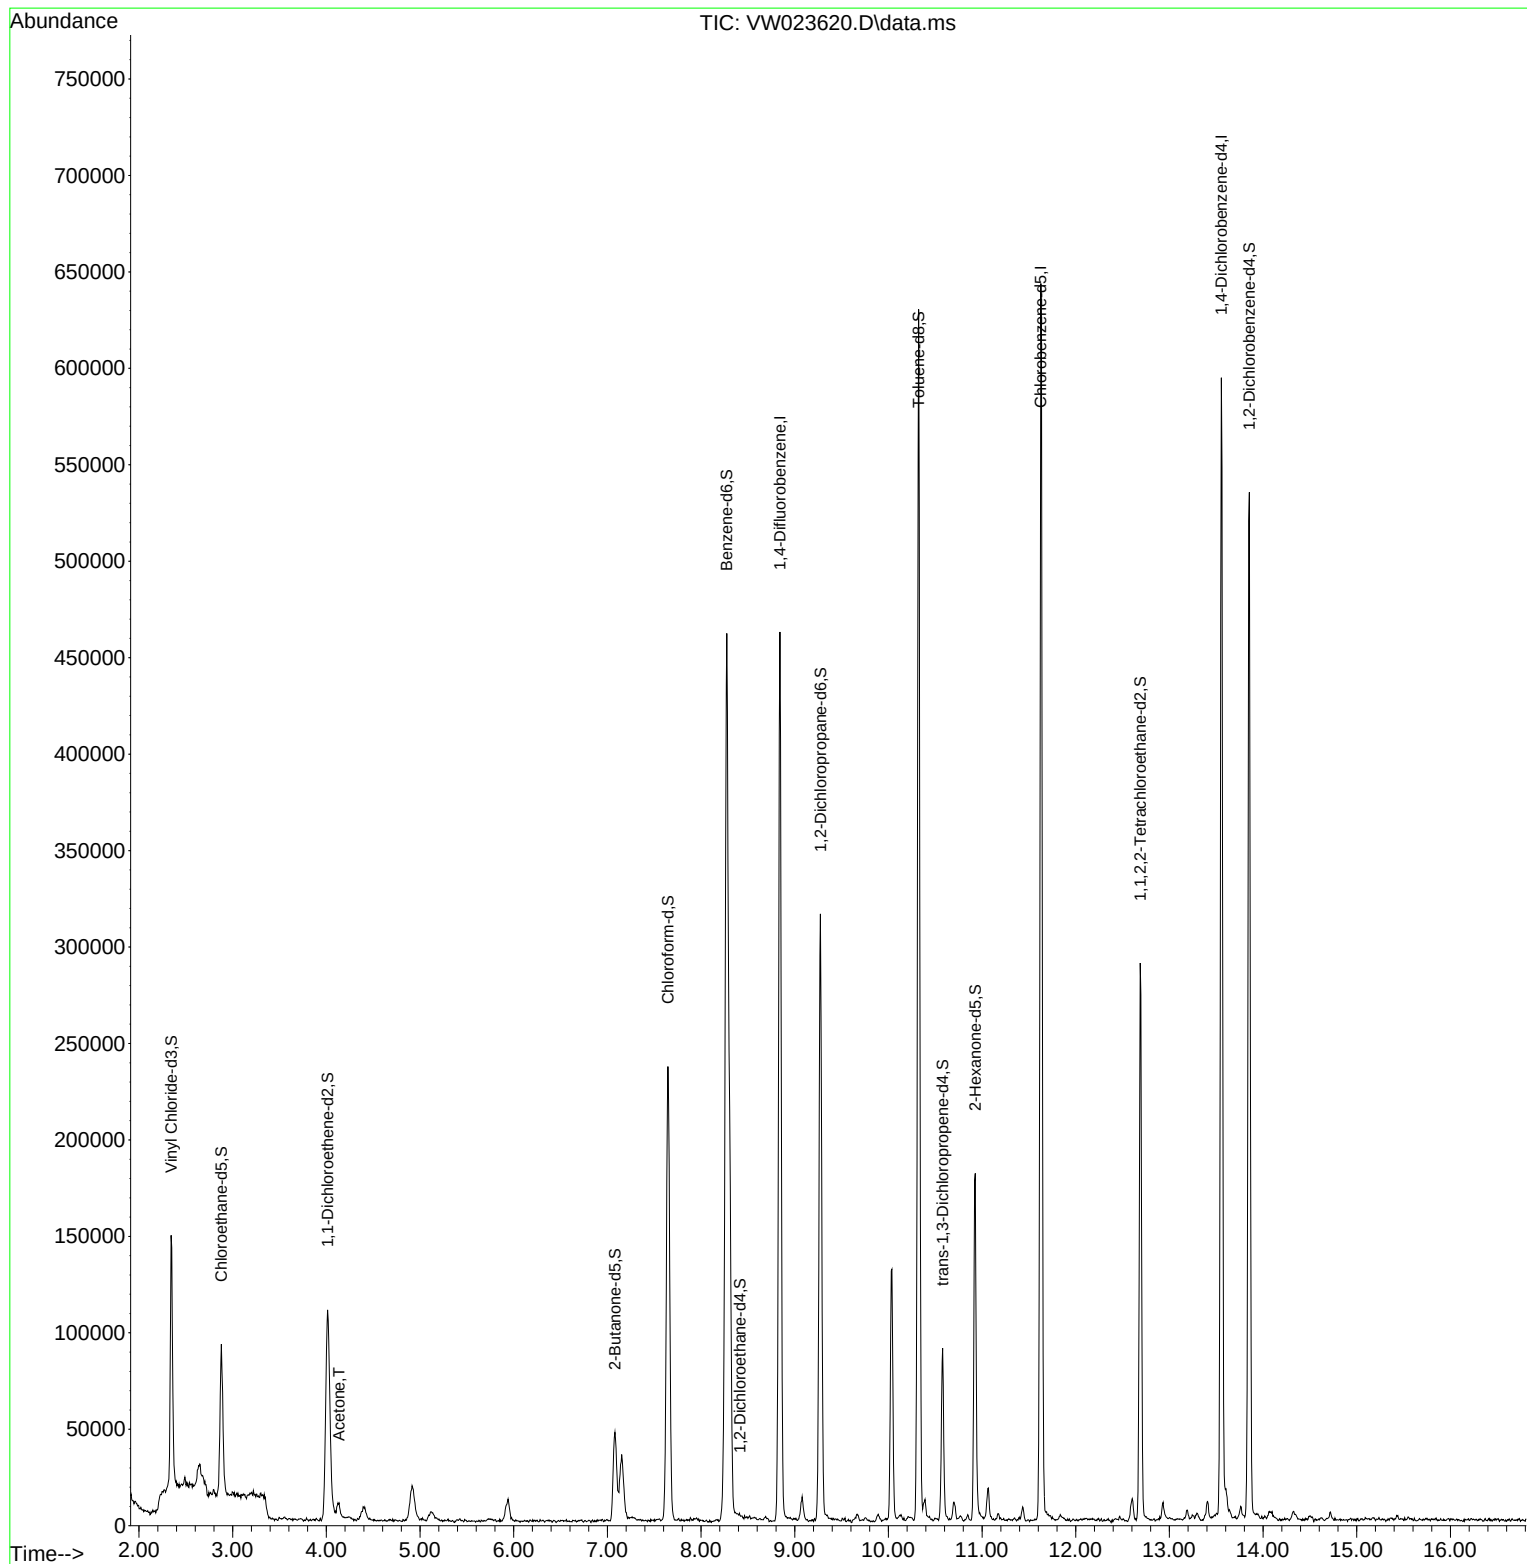

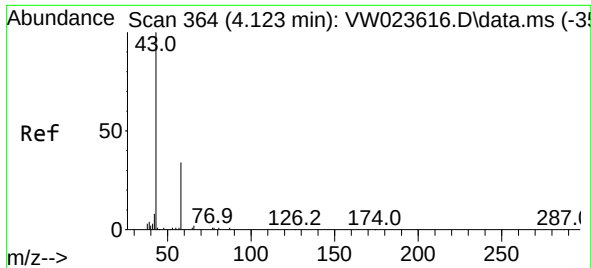

#13

Acetone

Concen: 12.838 ug/L

RT: 4.135 min Scan# 3

Delta R.T. 0.012 min

Lab File: VW023620.D


Acq: 12 Jul 2022 22:11

Instrument :

MSVOA_W

ClientSampleId :

F5B17

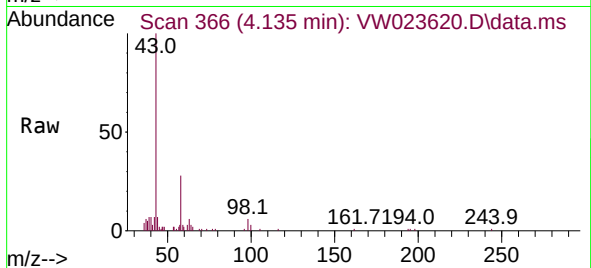

Tgt Ion: 43 Resp: 13074

Ion Ratio Lower Upper

43 100

58 35.6 0.0 61.2

