

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023630.D
 Acq On : 13 Jul 2022 02:19
 Operator : SY/VA
 Sample : N3678-08
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B27

Quant Time: Jul 13 06:15:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 02:42:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	367054	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	328085	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	126124	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	134290	20.211	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.840%
7) Chloroethane-d5	2.873	69	96558	25.410	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.640%
11) 1,1-Dichloroethene-d2	4.007	63	108480	14.481	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.920%
21) 2-Butanone-d5	7.080	46	60483	43.835	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.680%
24) Chloroform-d	7.647	84	248202	23.740	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.960%
26) 1,2-Dichloroethane-d4	8.384	65	331	0.056	ug/L	0.08
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.240%#
32) Benzene-d6	8.275	84	460320	25.358	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.440%
36) 1,2-Dichloropropane-d6	9.275	67	144021	27.099	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.400%
41) Toluene-d8	10.323	98	407236	23.144	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.560%
43) trans-1,3-Dichloroprop...	10.573	79	45088	19.006	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.040%
47) 2-Hexanone-d5	10.927	63	45988	44.243	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.480%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	119906	22.741	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	120069	26.387	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.560%
Target Compounds						
					Qvalue	
5) Vinyl chloride	2.355	62	22178	2.683	ug/L #	81
13) Acetone	4.129	43	9046	8.896	ug/L	94
17) trans-1,2-Dichloroethene	5.415	96	9763	1.858	ug/L	90
39) cis-1,3-Dichloropropene	10.037	75	4105	0.540	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023630.D
Acq On : 13 Jul 2022 02:19
Operator : SY/VA
Sample : N3678-08
Misc : 6.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B27

Quant Time: Jul 13 06:15:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 02:42:59 2022
Response via : Initial Calibration




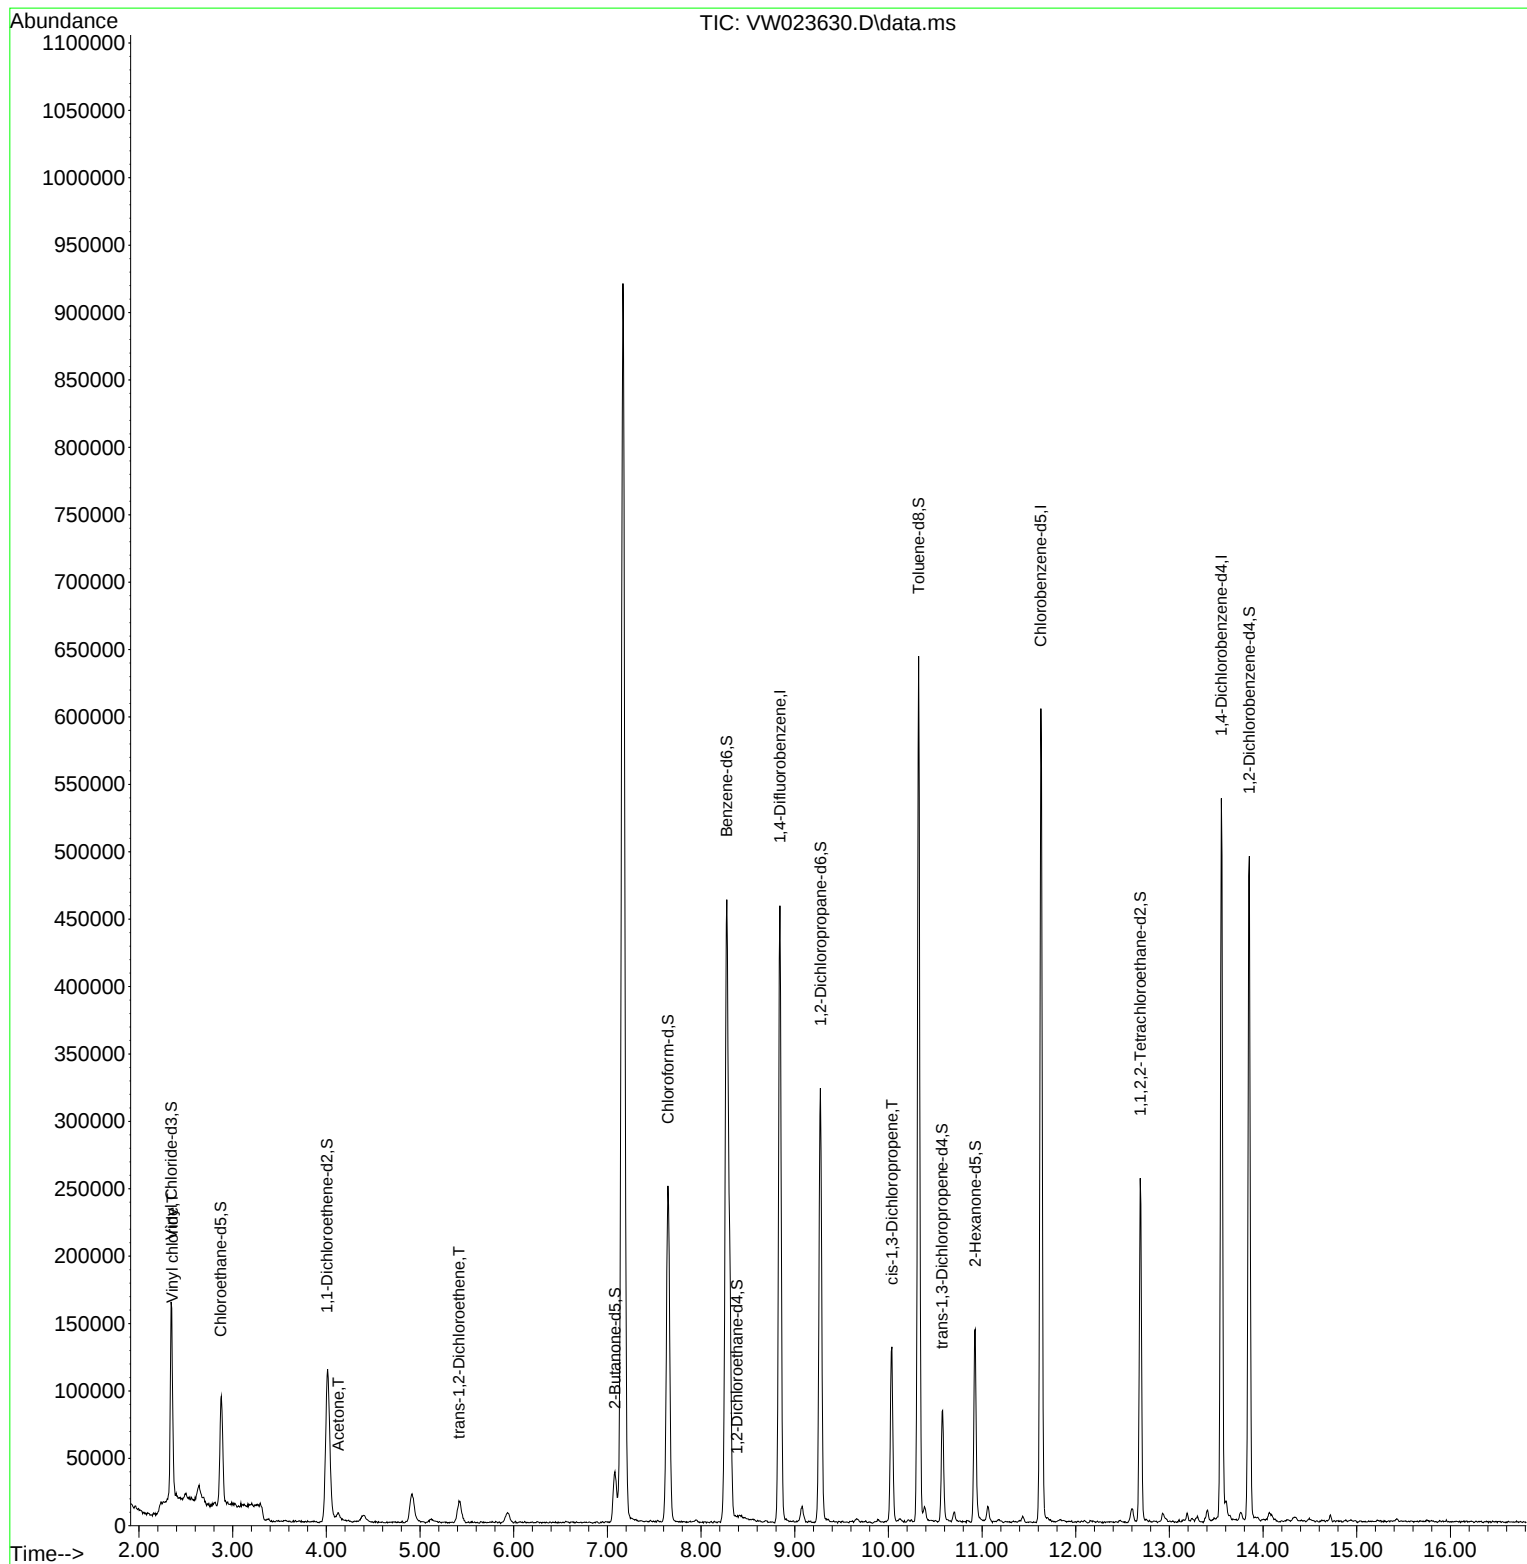


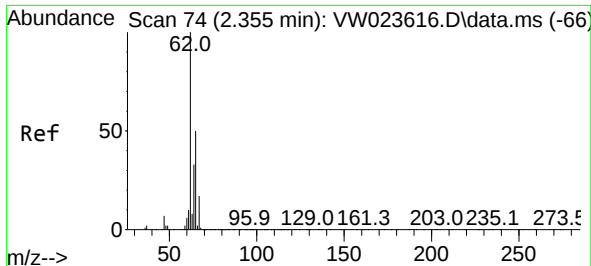

#5
 Vinyl chloride
 Concen: 2.683 ug/L
 RT: 2.355 min Scan# 74
 Delta R.T. 0.000 min
 Lab File: VW023630.D
 Acq: 13 Jul 2022 02:19




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B27


Tgt Ion: 62 Resp: 22178
 Ion Ratio Lower Upper
 62 100
 64 47.9 25.8 47.8#

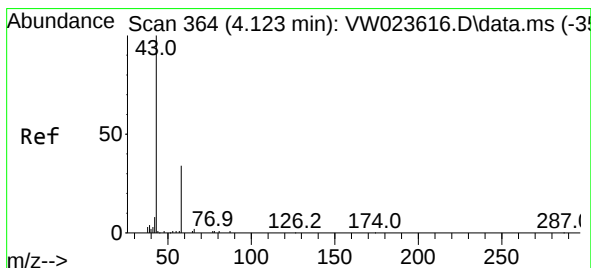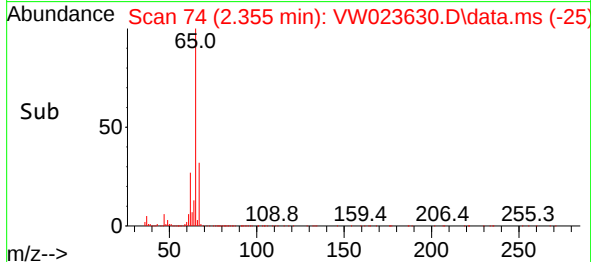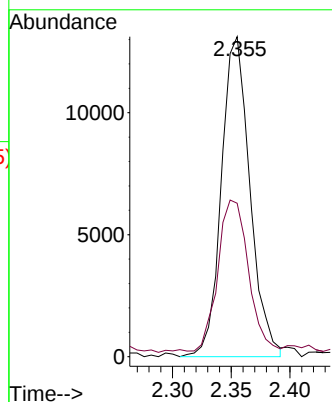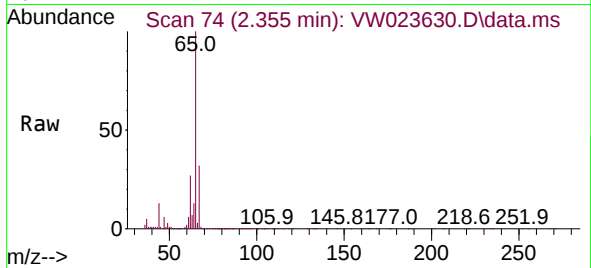

#13
 Acetone
 Concen: 8.896 ug/L
 RT: 4.129 min Scan# 365
 Delta R.T. 0.006 min
 Lab File: VW023630.D
 Acq: 13 Jul 2022 02:19

Tgt Ion: 43 Resp: 9046
 Ion Ratio Lower Upper
 43 100
 58 27.1 0.0 61.2


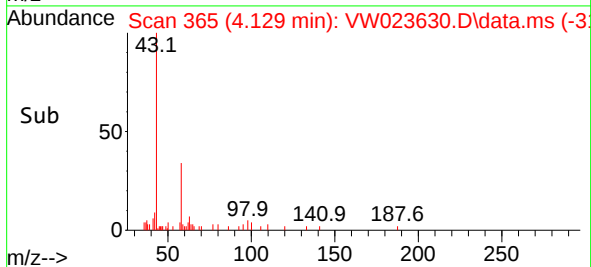
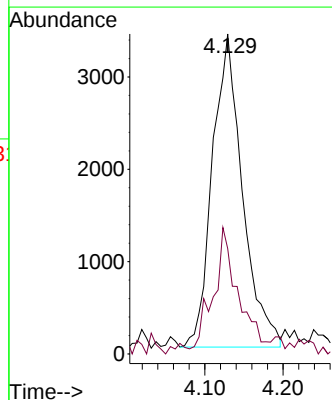
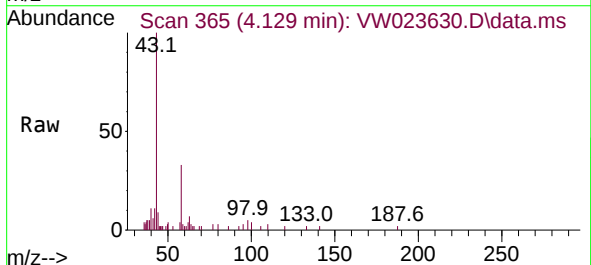


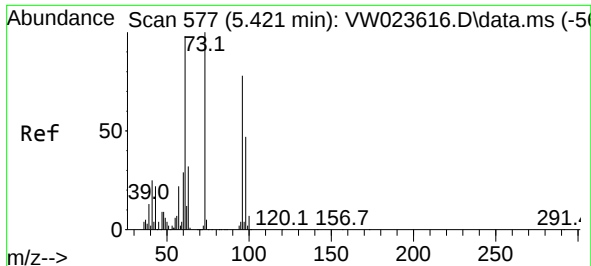

#17
trans-1,2-Dichloroethene
Concen: 1.858 ug/L
RT: 5.415 min Scan# 51
Delta R.T. -0.006 min
Lab File: VW023630.D
Acq: 13 Jul 2022 02:19

Instrument :
MSVOA_W
ClientSampleId :
F5B27

Tgt Ion: 96 Resp: 9763
Ion Ratio Lower Upper
96 100
61 115.5 92.3 171.5
98 63.5 45.5 84.5

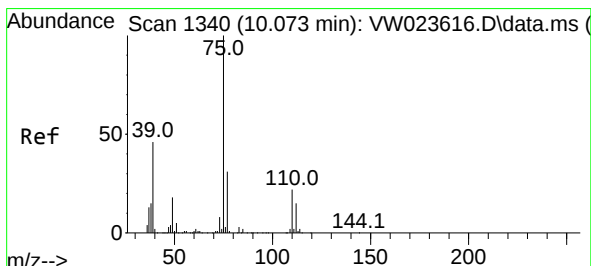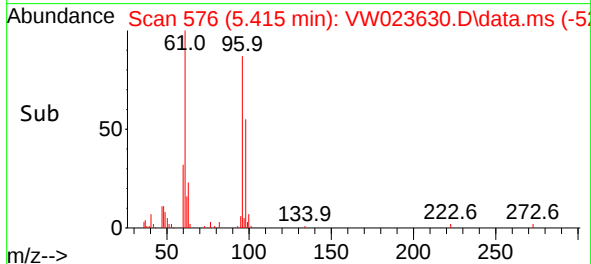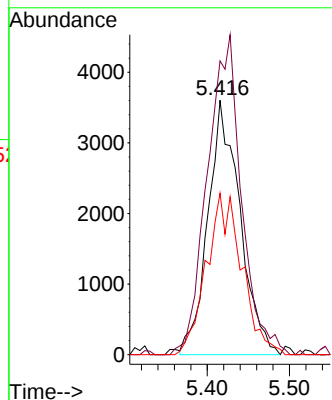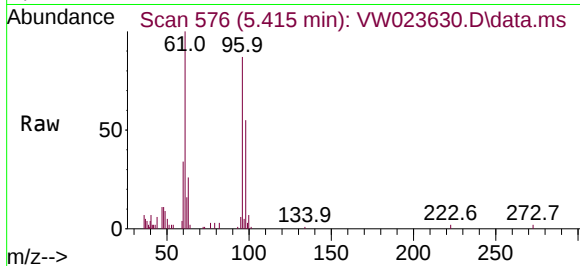

#39
cis-1,3-Dichloropropene
Concen: 0.540 ug/L
RT: 10.037 min Scan# 1334
Delta R.T. -0.036 min
Lab File: VW023630.D
Acq: 13 Jul 2022 02:19

Tgt Ion: 75 Resp: 4105
Ion Ratio Lower Upper
75 100
77 51.8 23.0 42.6#

