




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023599.D
Acq On : 12 Jul 2022 09:38
Operator : SY/VA
Sample : VW0712SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK541

Manual IntegrationsAPPROVED

Quant Time: Jul 13 01:32:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 01:31:49 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

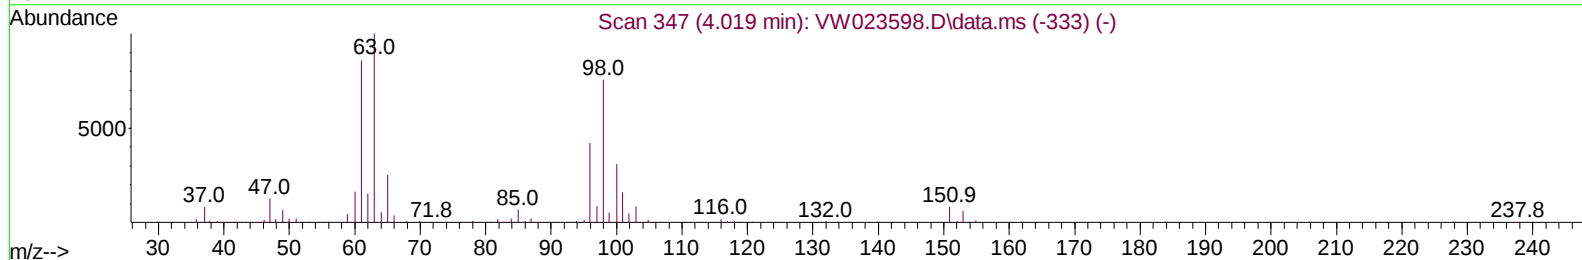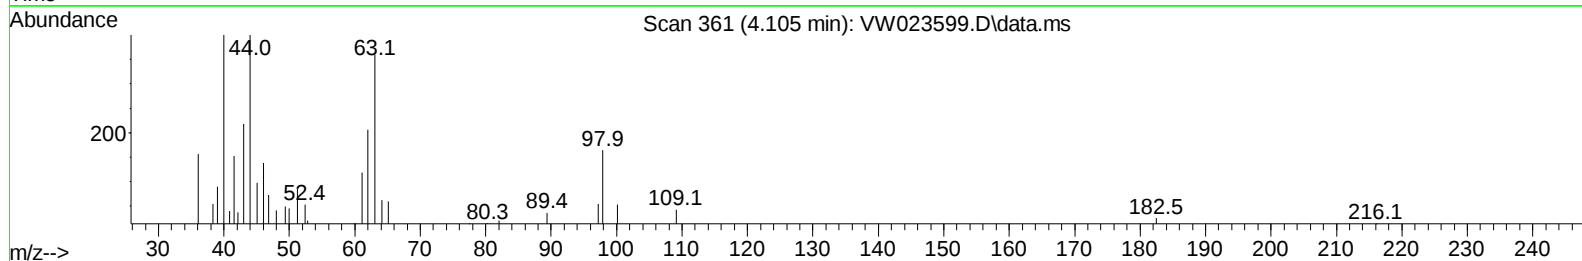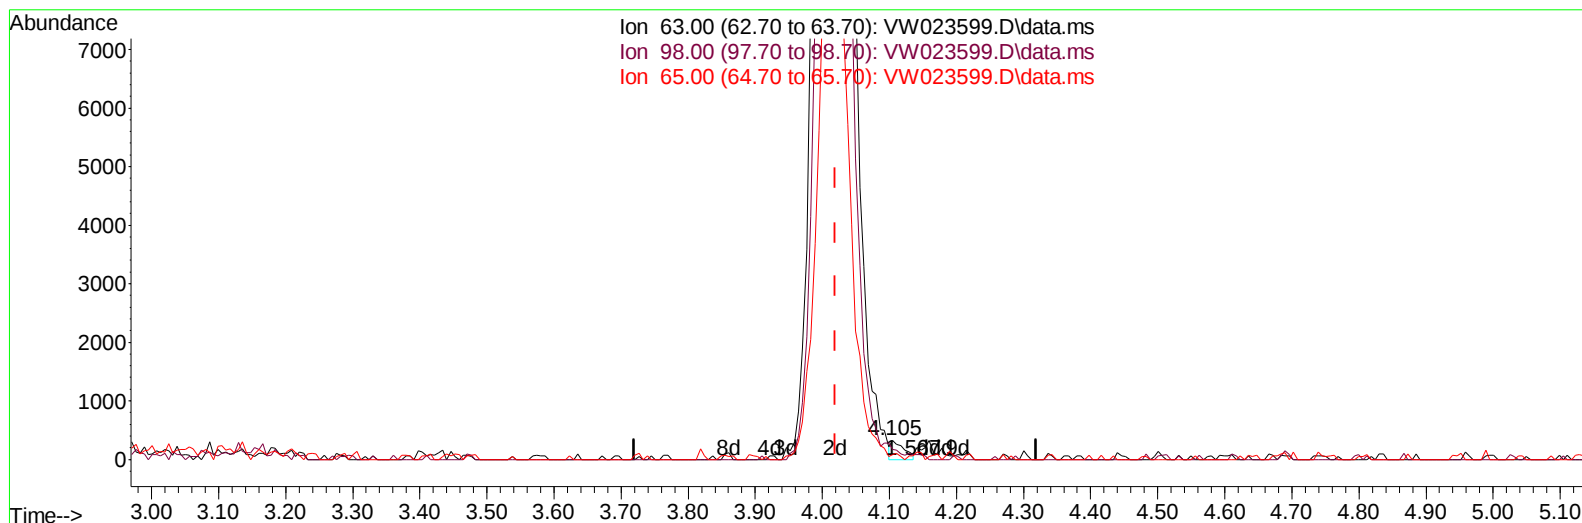

TIC: VW023599.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.105min (+ 0.085) 0.07 ug/L

response 436

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.10	55.05
65.00	22.40	20.87
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023599.D
 Acq On : 12 Jul 2022 09:38
 Operator : SY/VA
 Sample : VW0712SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK541

Manual IntegrationsAPPROVED

Quant Time: Jul 13 01:32:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 01:31:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

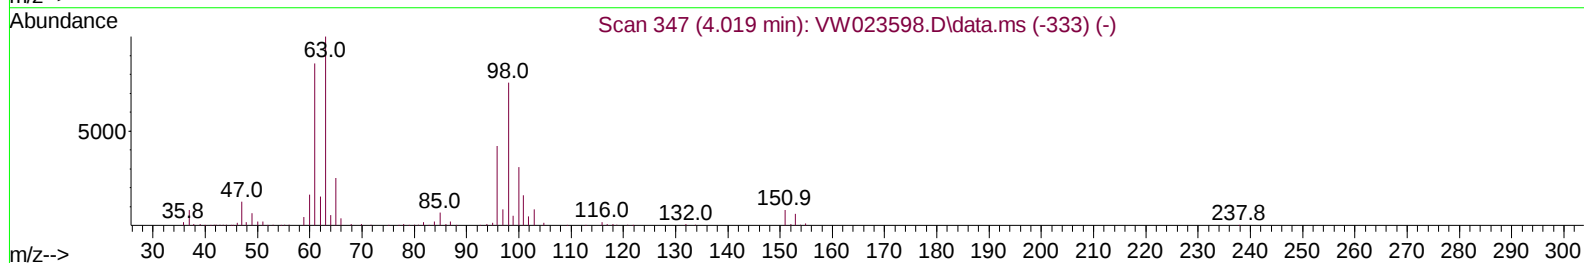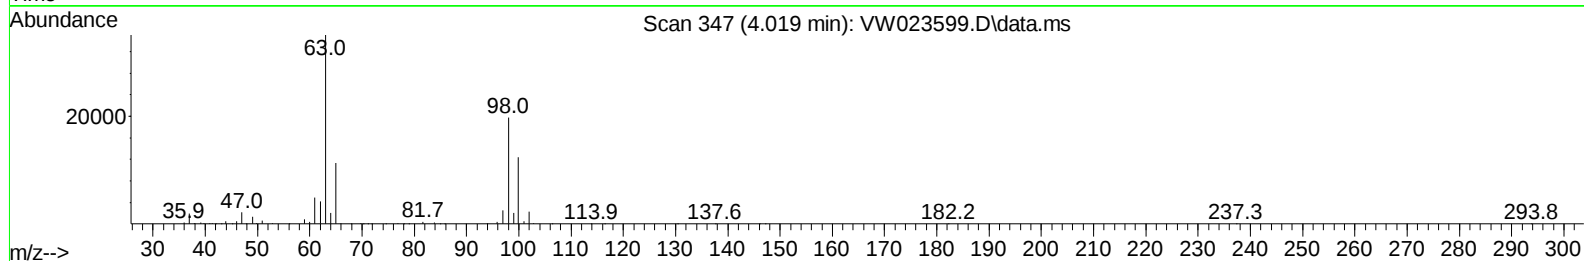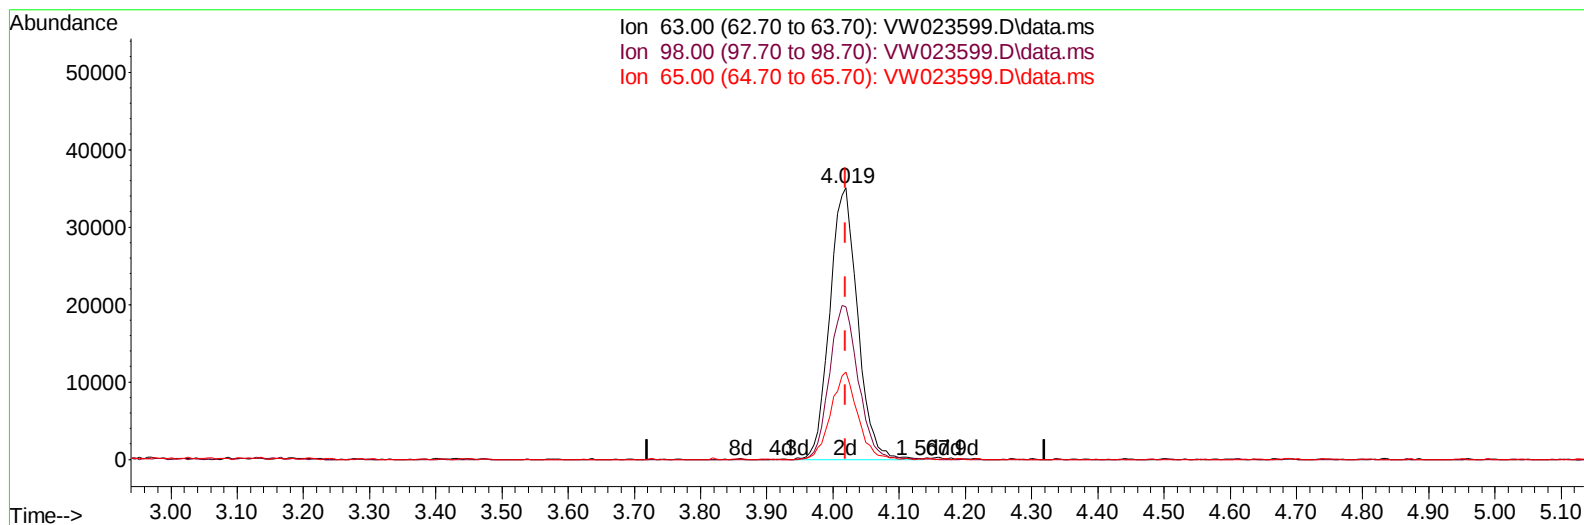

TIC: VW023599.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (+ 0.000) 16.03 ug/L m

response 102453

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.10	0.23#
65.00	22.40	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023599.D
 Acq On : 12 Jul 2022 09:38
 Operator : SY/VA
 Sample : VW0712SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK541

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 01:32:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 01:31:49 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		313119	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		297264	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		138413	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		121432	21.424	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	85.680%	
7) Chloroethane-d5	2.879	69		66414	20.488	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	81.960%	
11) 1,1-Dichloroethene-d2	4.019	63		102453m	16.032	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	64.120%	
21) 2-Butanone-d5	7.080	46		51706	43.929	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	87.860%	
24) Chloroform-d	7.647	84		200000	22.425	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.680%	
26) 1,2-Dichloroethane-d4	8.305	65		114941	22.801	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	91.200%	
32) Benzene-d6	8.275	84		376685	22.902	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	9.275	67		112661	23.396	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	93.600%	
41) Toluene-d8	10.323	98		344656	21.619	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	86.480%	
43) trans-1,3-Dichloroprop...	10.579	79		46086	21.440	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	85.760%	
47) 2-Hexanone-d5	10.921	63		41926	44.517	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	89.040%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		103886	21.746	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	87.000%	
66) 1,2-Dichlorobenzene-d4	13.853	152		124460	24.923	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	99.680%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023599.D
Acq On : 12 Jul 2022 09:38
Operator : SY/VA
Sample : VW0712SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK541

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 01:32:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 01:31:49 2022
Response via : Initial Calibration

