




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023610.D
 Acq On : 12 Jul 2022 17:01
 Operator : SY/VA
 Sample : N3676-10
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B09

Manual IntegrationsAPPROVED

Quant Time: Jul 13 01:35:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 01:31:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

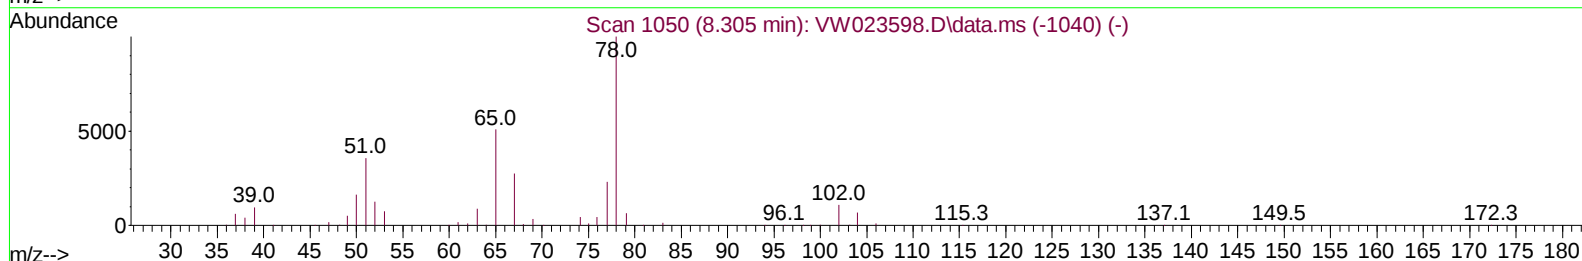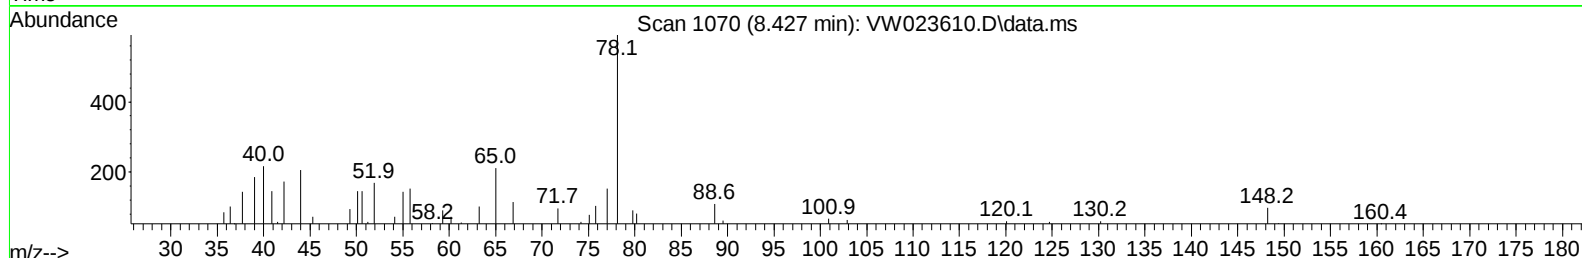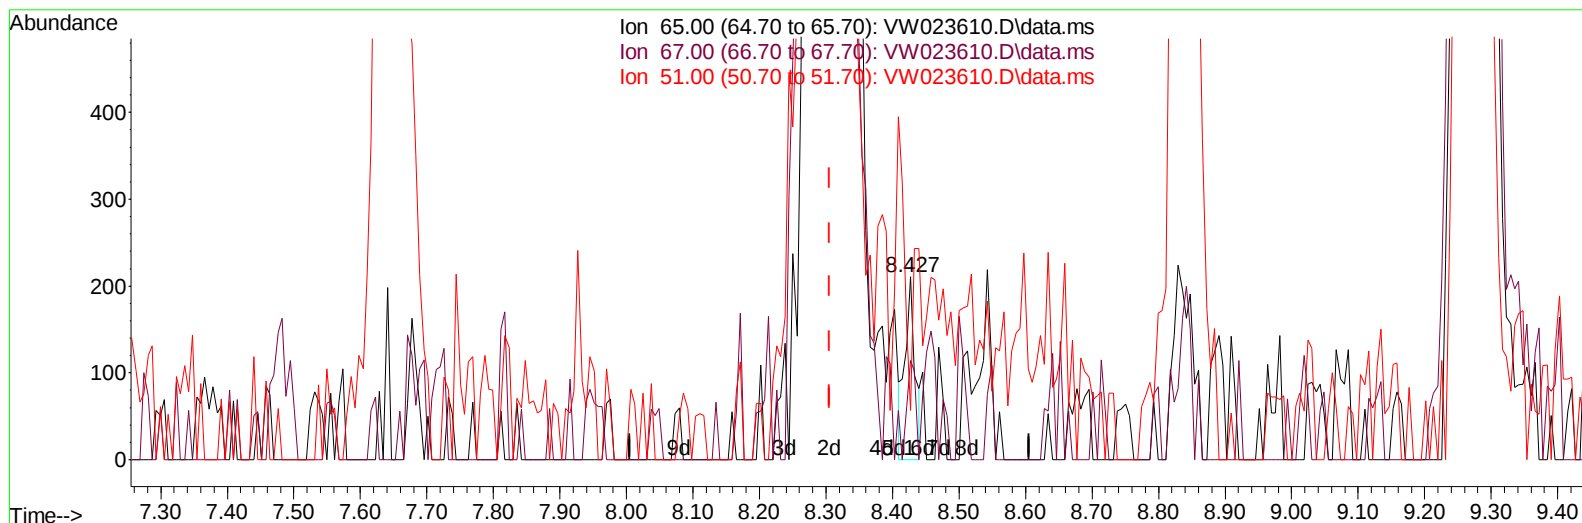

TIC: VW023610.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.427min (+ 0.122) 0.07 ug/L

response 224

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	45.09
51.00	94.50	80.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023610.D
 Acq On : 12 Jul 2022 17:01
 Operator : SY/VA
 Sample : N3676-10
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B09

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 01:35:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 01:31:49 2022
 Response via : Initial Calibration

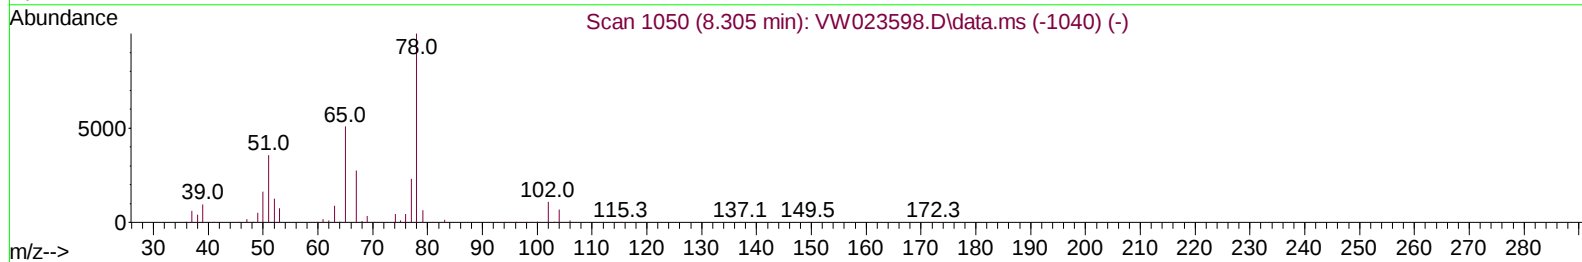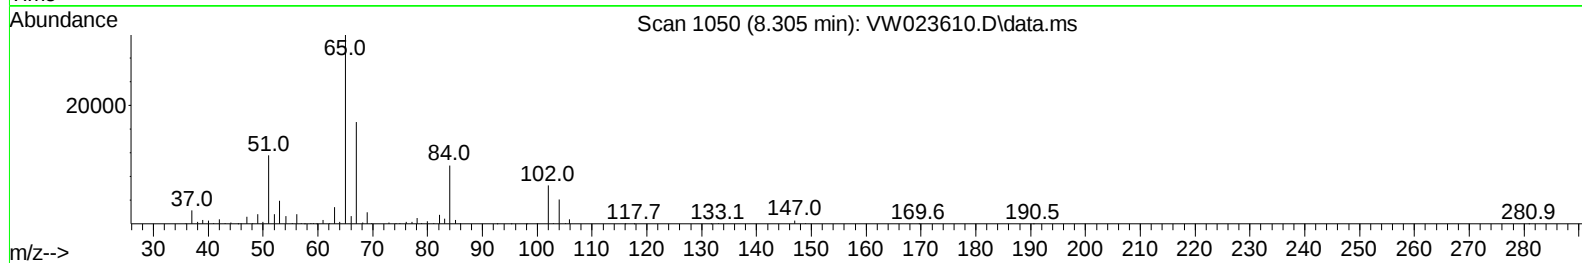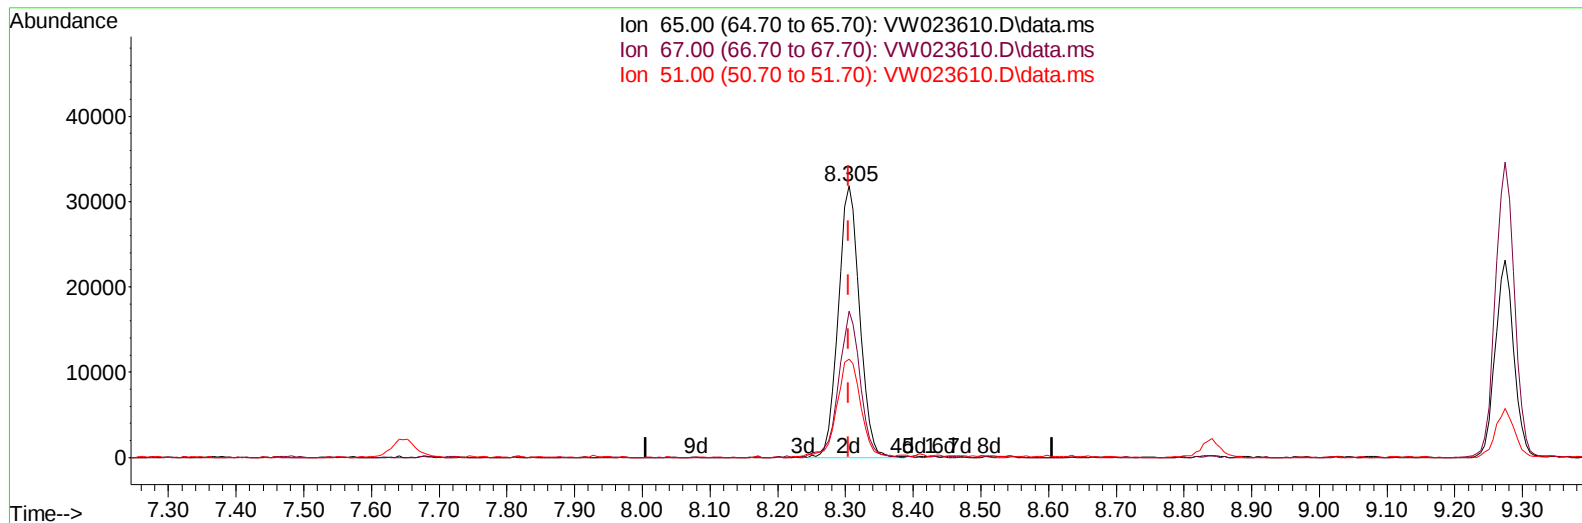

TIC: VW023610.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 22.60 ug/L m

response 69481

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.15#
51.00	94.50	0.26#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023610.D
 Acq On : 12 Jul 2022 17:01
 Operator : SY/VA
 Sample : N3676-10
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B09

Manual IntegrationsAPPROVED

Quant Time: Jul 13 01:35:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 01:31:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	190955	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	167407	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	62181	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	77372	22.384	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	89.520%	
7) Chloroethane-d5	2.873	69	43817	22.164	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	88.640%	
11) 1,1-Dichloroethene-d2	4.007	63	68060	17.464	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	69.840%	
21) 2-Butanone-d5	7.080	46	40881	56.952	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	113.900%	
24) Chloroform-d	7.647	84	123177	22.647	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.600%	
26) 1,2-Dichloroethane-d4	8.305	65	69481m	22.601	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.400%	
32) Benzene-d6	8.275	84	225156	24.308	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	97.240%	
36) 1,2-Dichloropropane-d6	9.274	67	68064	25.099	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	100.400%	
41) Toluene-d8	10.323	98	186105	20.728	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	82.920%	
43) trans-1,3-Dichloroprop...	10.579	79	22911	18.927	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	75.720%	
47) 2-Hexanone-d5	10.921	63	26723	50.384	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.760%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	64884	24.117	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	96.480%	
66) 1,2-Dichlorobenzene-d4	13.853	152	52541	23.420	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.680%	
Target Compounds						Qvalue
5) vinyl chloride	2.349	62	6022	1.400	ug/L	# 1
13) Acetone	4.123	43	24205	45.754	ug/L	96
17) trans-1,2-Dichloroethene	5.415	96	7345	2.687	ug/L	94
42) Toluene	10.390	91	15763	1.374	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023610.D
Acq On : 12 Jul 2022 17:01
Operator : SY/VA
Sample : N3676-10
Misc : 5.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B09

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 01:35:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 01:31:49 2022
Response via : Initial Calibration

