




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023623.D
Acq On : 12 Jul 2022 23:26
Operator : SY/VA
Sample : N3678-01
Misc : 6.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B20

Manual IntegrationsAPPROVED

Quant Time: Jul 13 06:13:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 02:42:59 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

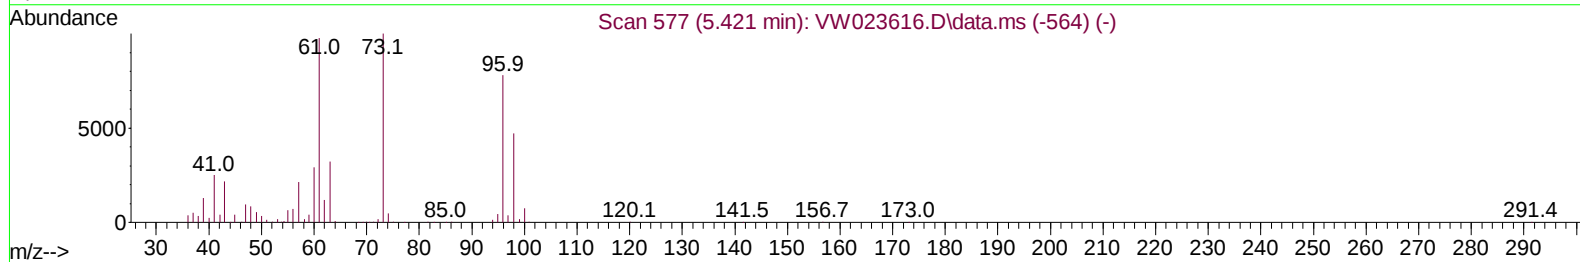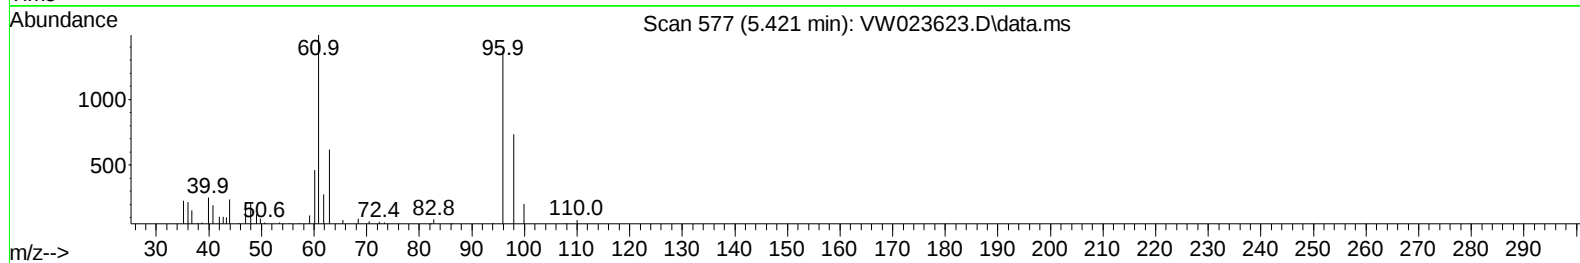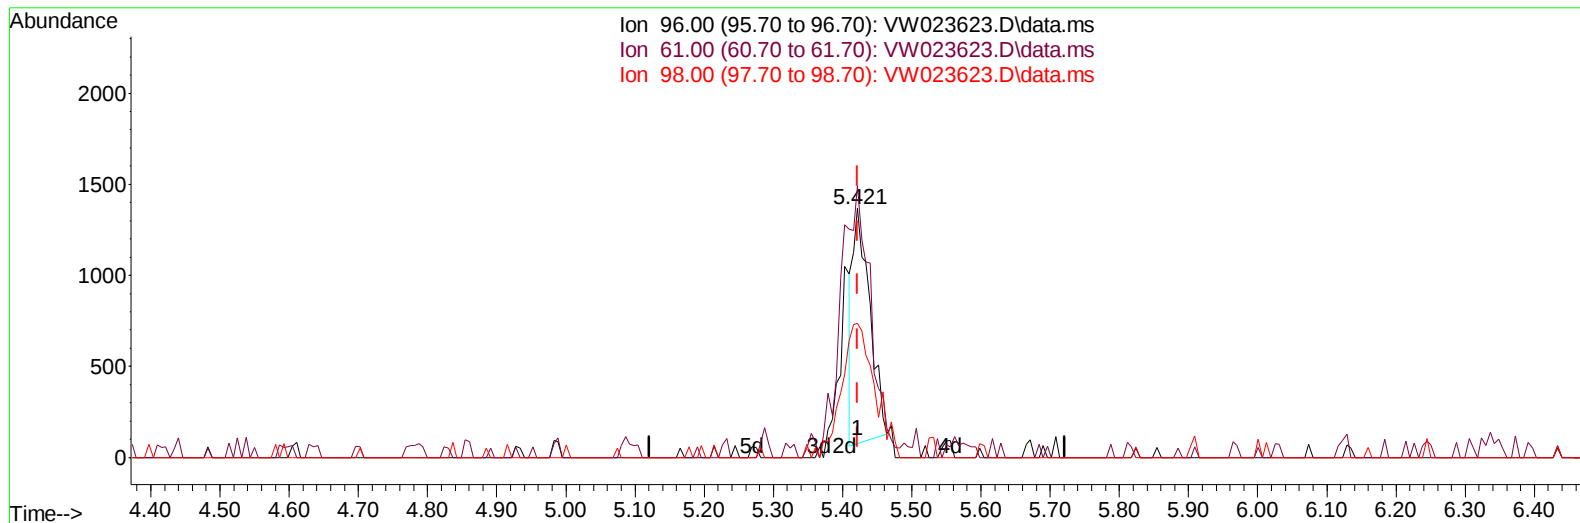

TIC: VW023623.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.421min (+ 0.000) 1.45 ug/L

response 2192

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	131.90	108.99
98.00	65.00	53.80
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023623.D
Acq On : 12 Jul 2022 23:26
Operator : SY/VA
Sample : N3678-01
Misc : 6.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B20

Manual IntegrationsAPPROVED

Quant Time: Jul 13 06:13:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 02:42:59 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

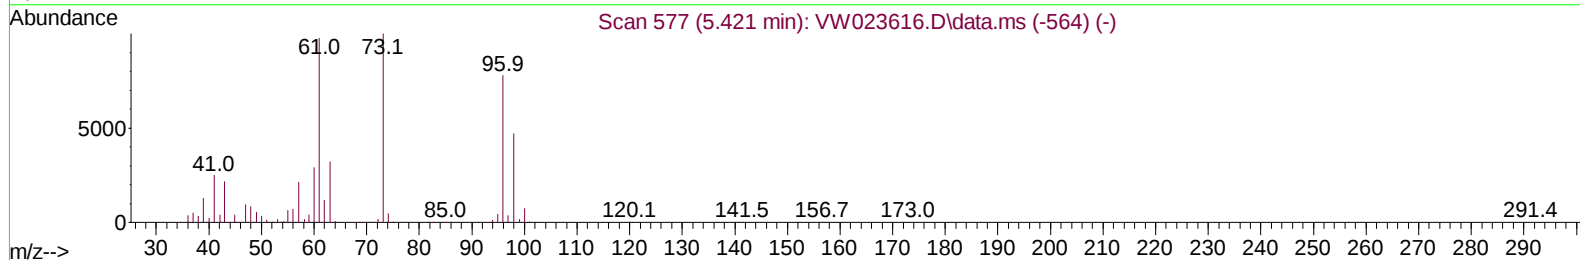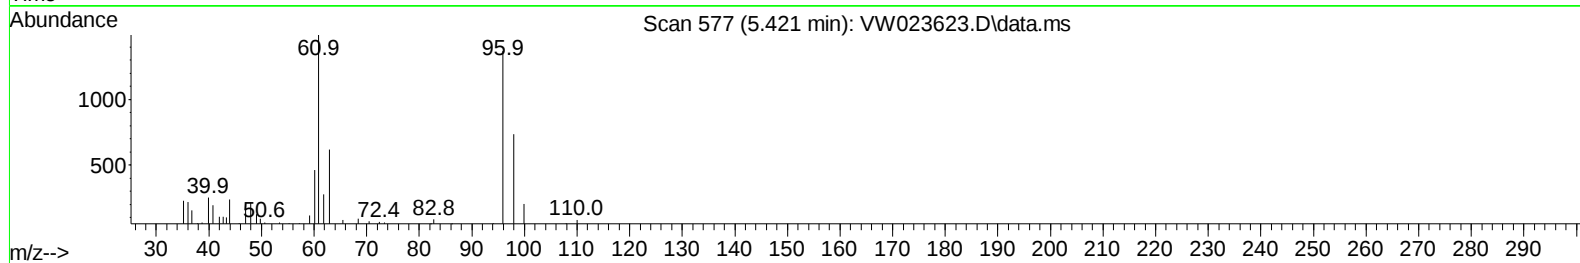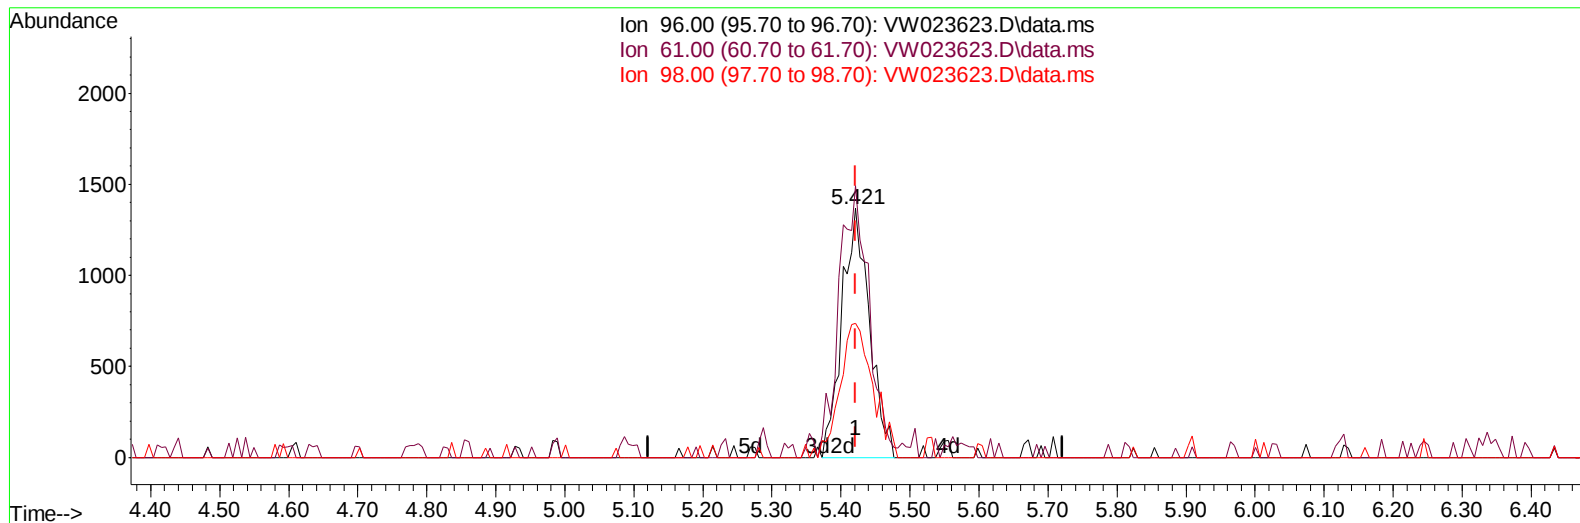

TIC: VW023623.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.421min (+ 0.000) 2.49 ug/L m

response 3769

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	131.90	108.99
98.00	65.00	53.80
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023623.D
 Acq On : 12 Jul 2022 23:26
 Operator : SY/VA
 Sample : N3678-01
 Misc : 6.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B20

Manual IntegrationsAPPROVED

Quant Time: Jul 13 06:13:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 02:42:59 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	105851	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	105129	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	39533	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	38125	19.897	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	79.600%	
7) Chloroethane-d5	2.873	69	26769	24.427	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	97.720%	
11) 1,1-Dichloroethene-d2	4.001	63	33136	15.339	ug/L	-0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	61.360%	
21) 2-Butanone-d5	7.080	46	33477	84.134	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	168.260%#	
24) Chloroform-d	7.647	84	85776	28.450	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	113.800%	
26) 1,2-Dichloroethane-d4	8.305	65	55888	32.796	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	131.200%#	
32) Benzene-d6	8.275	84	140320	24.123	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	96.480%	
36) 1,2-Dichloropropane-d6	9.274	67	49321	28.961	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	115.840%	
41) Toluene-d8	10.323	98	115913	20.559	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	82.240%	
43) trans-1,3-Dichloroprop...	10.579	79	15953	20.986	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.960%	
47) 2-Hexanone-d5	10.927	63	19725	59.221	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	118.440%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	52060	30.814	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	123.240%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	37656	26.401	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	105.600%	
Target Compounds						
13) Acetone	4.123	43	8655	29.514	ug/L	95
17) trans-1,2-Dichloroethene	5.421	96	3769m	2.488	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023623.D
Acq On : 12 Jul 2022 23:26
Operator : SY/VA
Sample : N3678-01
Misc : 6.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B20

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 06:13:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 02:42:59 2022
Response via : Initial Calibration

