

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023613.D
 Acq On : 12 Jul 2022 18:16
 Operator : SY/VA
 Sample : N3676-13
 Misc : 4.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B12

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/13/2022
 Supervised By : Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 01:35:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 01:31:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	81466	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	76230	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	28682	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	37783	25.621	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 102.480%			
7) Chloroethane-d5	2.879	69	26051	30.888	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 123.560%			
11) 1,1-Dichloroethene-d2	4.001	63	36256	21.807	ug/L	-0.02
Spiked Amount 25.000	Range 45 - 110		Recovery = 87.240%			
21) 2-Butanone-d5	7.080	46	21541	70.341	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 140.680%#			
24) Chloroform-d	7.647	84	60287	25.981	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 103.920%			
26) 1,2-Dichloroethane-d4	8.305	65	35876m	27.354	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 109.400%			
32) Benzene-d6	8.275	84	105369	24.982	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 99.920%			
36) 1,2-Dichloropropane-d6	9.274	67	34023	27.552	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 110.200%			
41) Toluene-d8	10.323	98	86823	21.237	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 84.960%			
43) trans-1,3-Dichloroprop...	10.579	79	12091	21.935	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 87.760%			
47) 2-Hexanone-d5	10.927	63	12508	51.790	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 103.580%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	37354	30.491	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 121.960%#			
66) 1,2-Dichlorobenzene-d4	13.853	152	27491	26.566	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 106.280%			
Target Compounds					Qvalue	
13) Acetone	4.135	43	12455	55.185	ug/L	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023613.D
Acq On : 12 Jul 2022 18:16
Operator : SY/VA
Sample : N3676-13
Misc : 4.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5B12

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 07/13/2022
Supervised By : Mahesh Dadoda 07/13/2022


Quant Time: Jul 13 01:35:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 01:31:49 2022
Response via : Initial Calibration

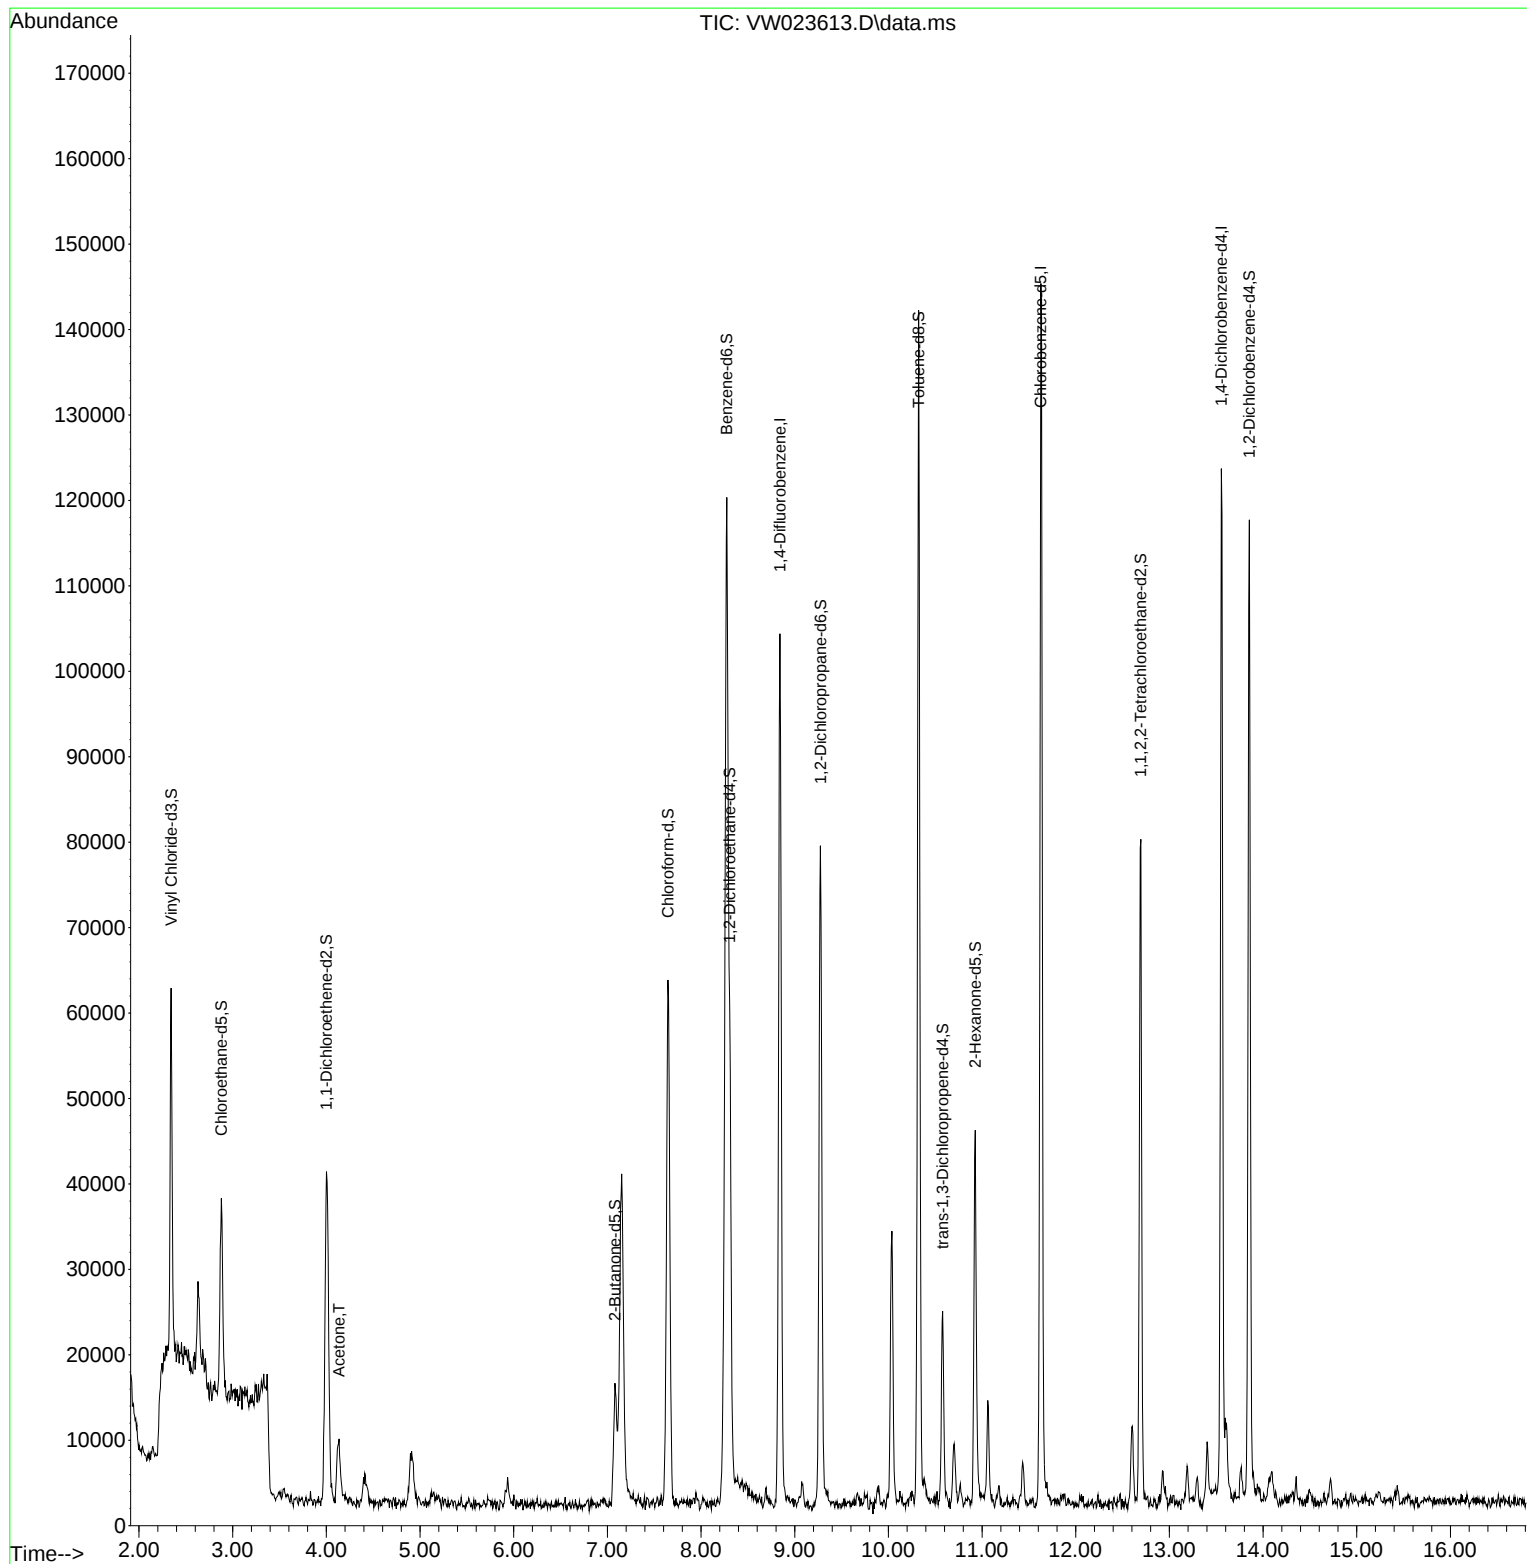

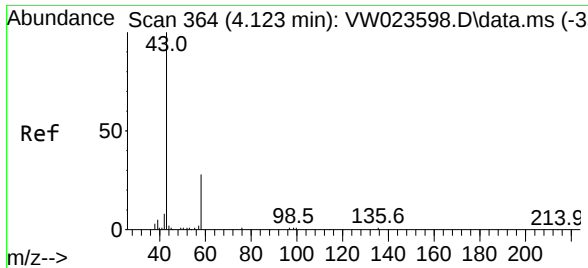

#13
 Acetone
 Concen: 55.185 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023613.D
 Acq: 12 Jul 2022 18:16

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B12

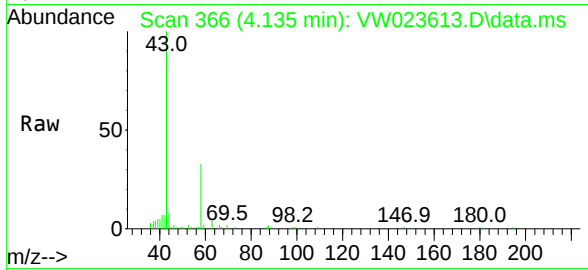

Tgt Ion: 43 Resp: 1245
 Ion Ratio Lower Upper
 43 100
 58 20.0 0.0 61.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

