

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
 Data File : VW023625.D
 Acq On : 13 Jul 2022 00:15
 Operator : SY/VA
 Sample : N3678-03
 Misc : 6.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B22

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 06:13:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 13 02:42:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	174963	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	156329	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	55647	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	74006	23.367	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.480%		
7) Chloroethane-d5	2.873	69	39212	21.648	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.600%		
11) 1,1-Dichloroethene-d2	4.007	63	63644	17.824	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.280%		
21) 2-Butanone-d5	7.080	46	37603	57.174	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	114.340%		
24) Chloroform-d	7.647	84	121156	24.311	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	97.240%		
26) 1,2-Dichloroethane-d4	8.305	65	70899m	25.170	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.680%		
32) Benzene-d6	8.275	84	218649	25.278	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	101.120%		
36) 1,2-Dichloropropane-d6	9.275	67	67861	26.797	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	107.200%		
41) Toluene-d8	10.323	98	182495	21.767	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	87.080%		
43) trans-1,3-Dichloroprop...	10.579	79	22689	20.072	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.280%		
47) 2-Hexanone-d5	10.921	63	25797	52.085	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.180%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	65186	25.946	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152	46270	23.047	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.200%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	8376	17.280	ug/L	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071222\
Data File : VW023625.D
Acq On : 13 Jul 2022 00:15
Operator : SY/VA
Sample : N3678-03
Misc : 6.14g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5B22

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022


Quant Time: Jul 13 06:13:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 13 02:42:59 2022
Response via : Initial Calibration

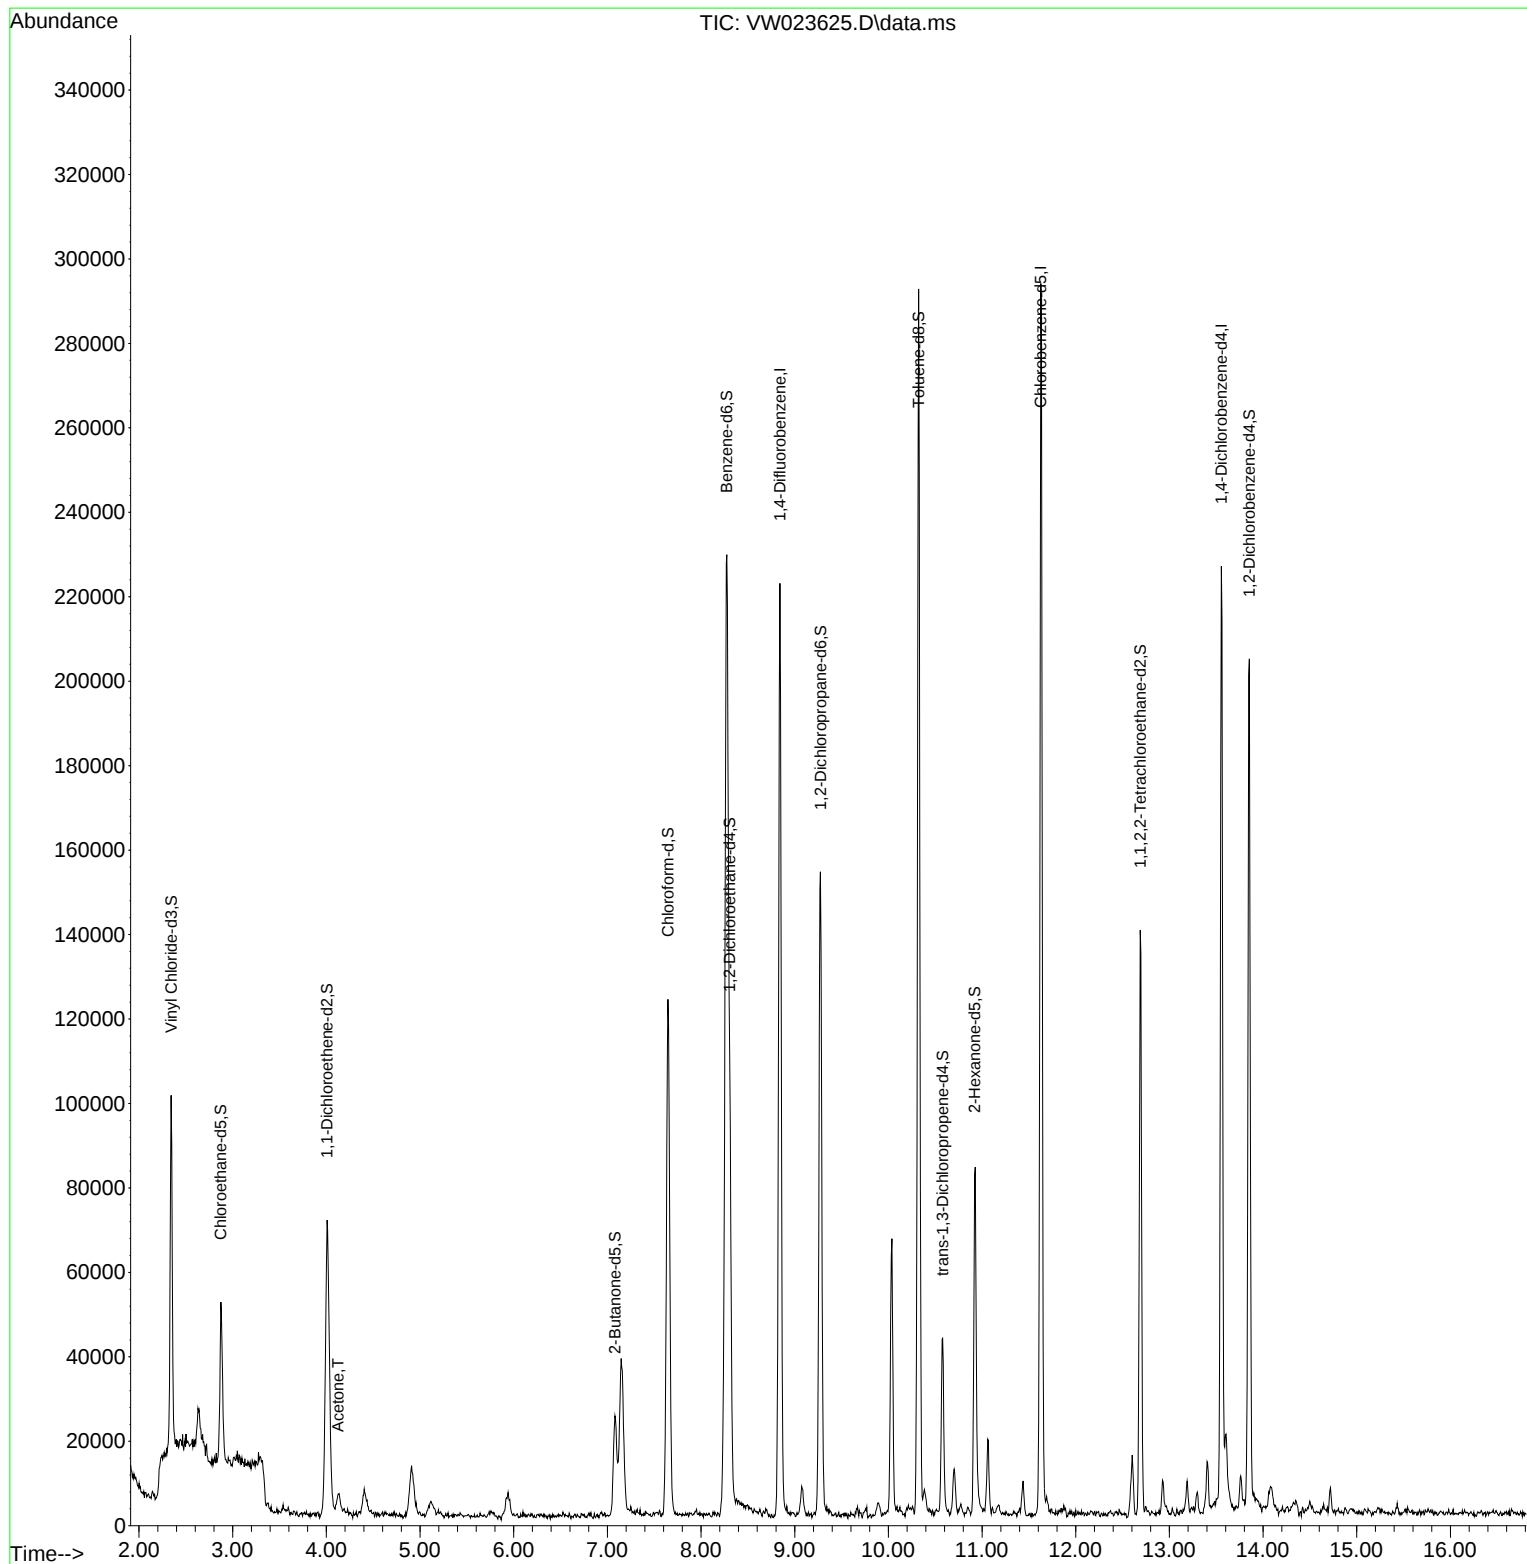

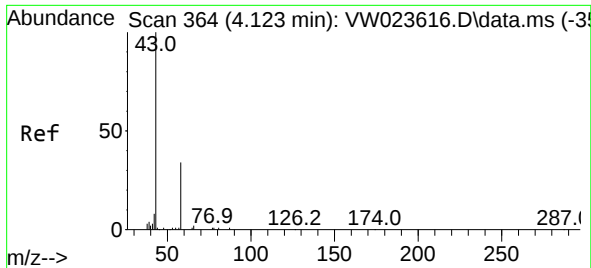

#13
 Acetone
 Concen: 17.280 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW023625.D
 Acq: 13 Jul 2022 00:15

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B22

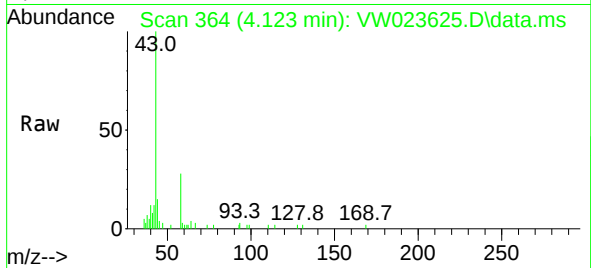

Tgt Ion: 43 Resp: 8370
 Ion Ratio Lower Upper
 43 100
 58 13.1 0.0 61.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

