




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023654.D
Acq On : 13 Jul 2022 18:04
Operator : SY/VA
Sample : N3678-19
Misc : 6.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B40

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:14:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

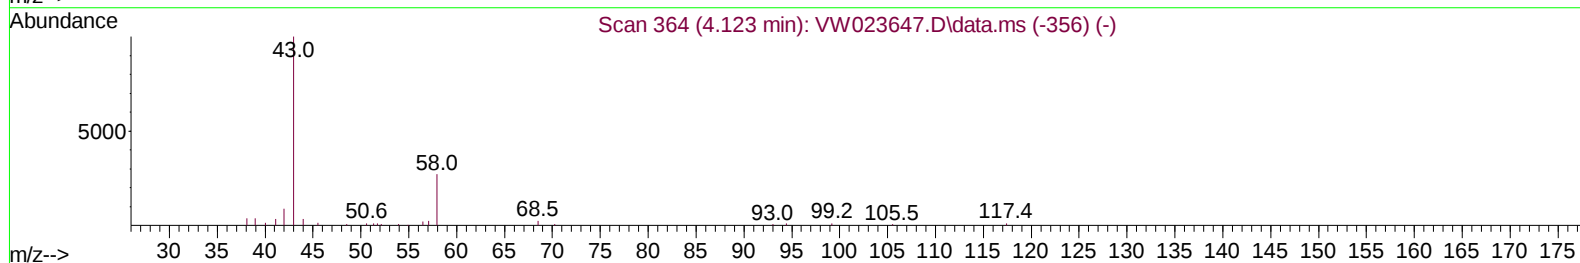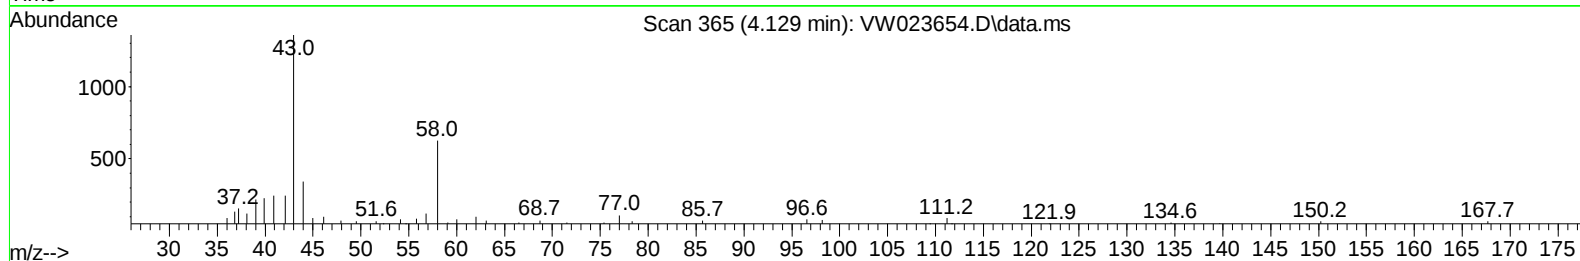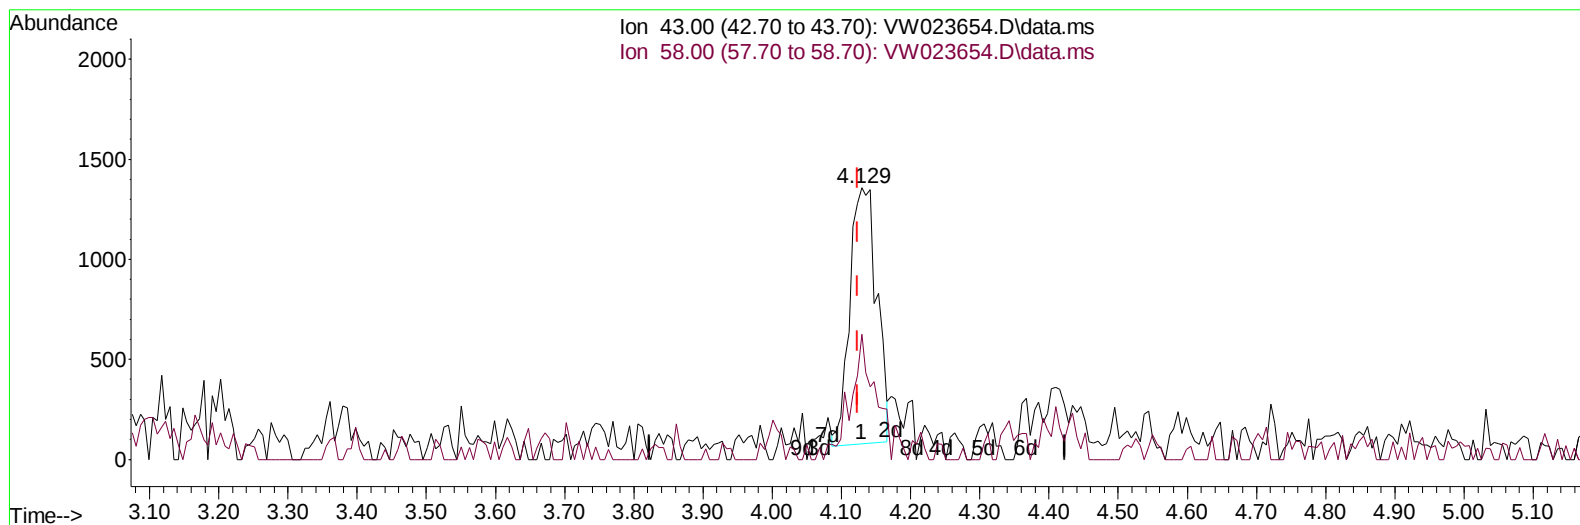

TIC: VW023654.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 42.82 ug/L

response 3459

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	32.41
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023654.D
 Acq On : 13 Jul 2022 18:04
 Operator : SY/VA
 Sample : N3678-19
 Misc : 6.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B40

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:14:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

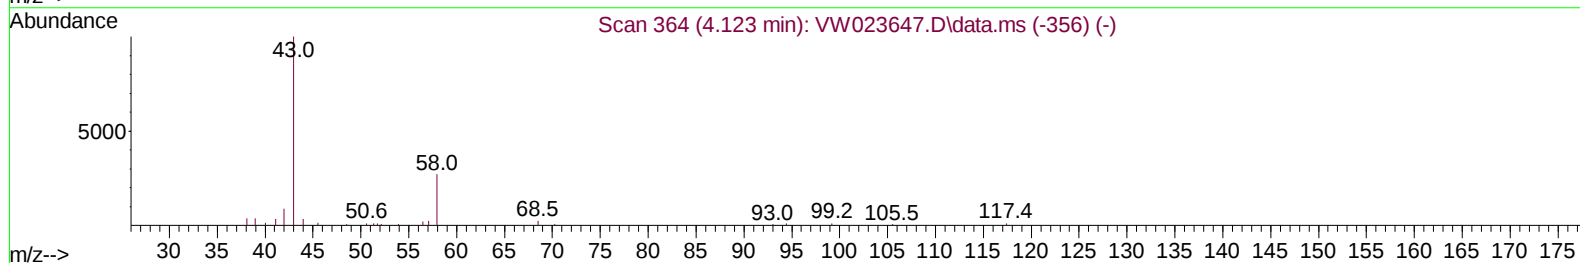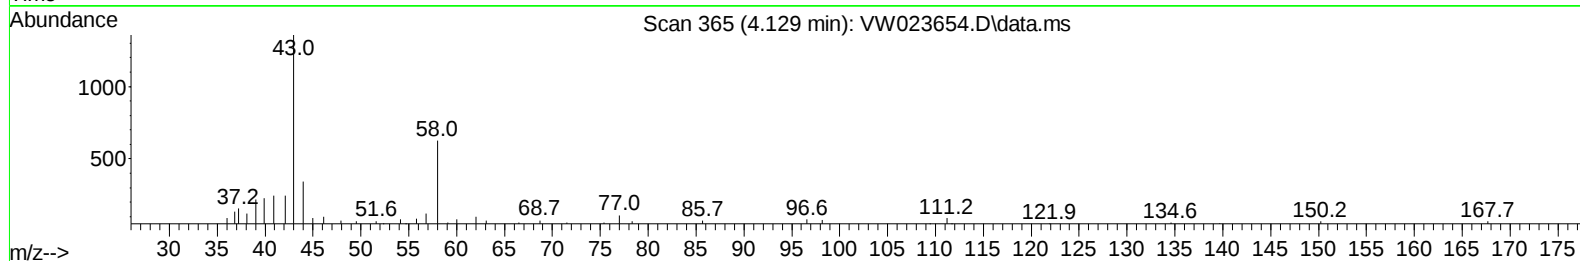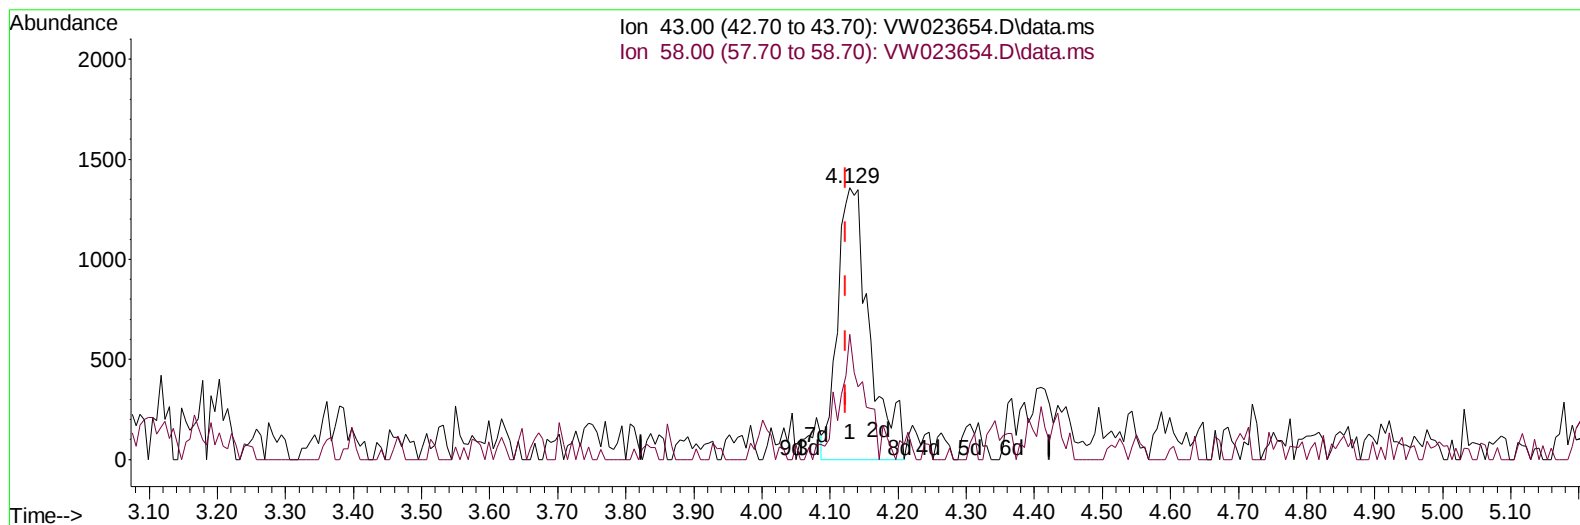

TIC: VW023654.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 54.34 ug/L m

response 4390

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	25.54
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023654.D
Acq On : 13 Jul 2022 18:04
Operator : SY/VA
Sample : N3678-19
Misc : 6.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B40

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:14:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

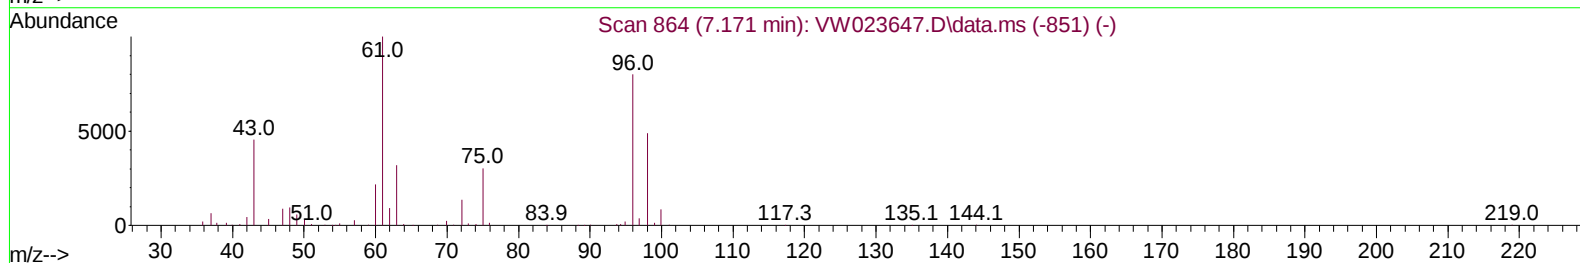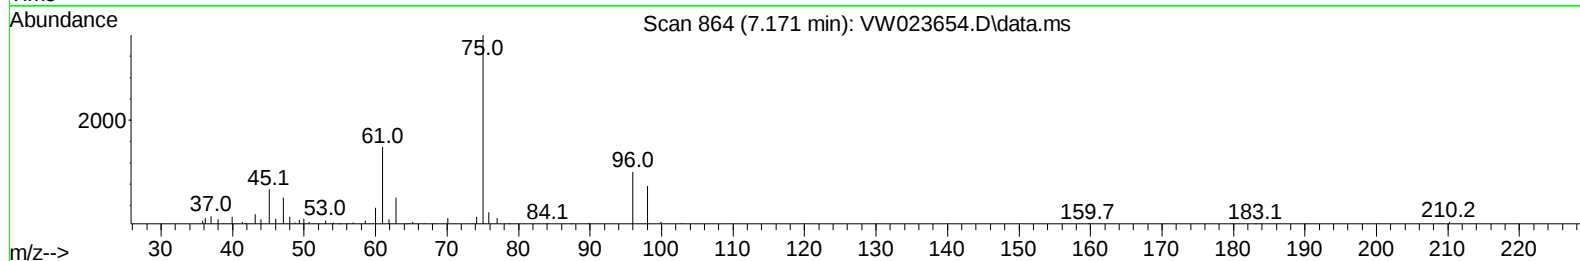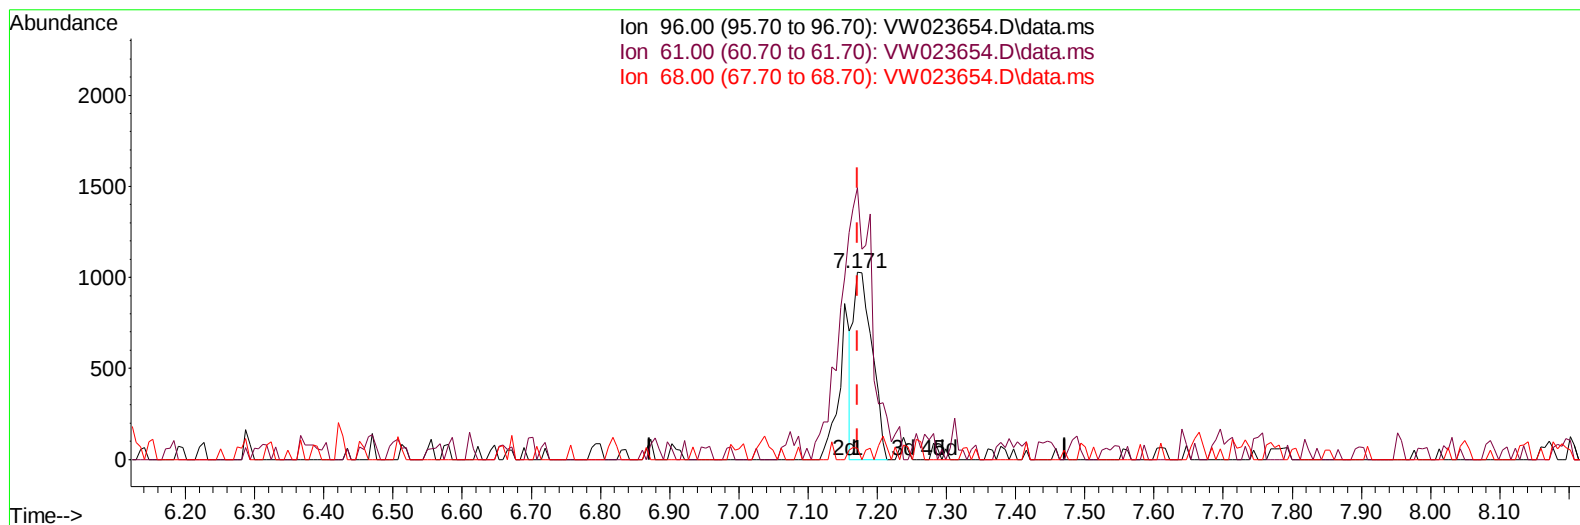

TIC: VW023654.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.171min (0.000) 4.75 ug/L

response 1952

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.40	145.04
68.00	0.30	5.93#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023654.D
 Acq On : 13 Jul 2022 18:04
 Operator : SY/VA
 Sample : N3678-19
 Misc : 6.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B40

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:14:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

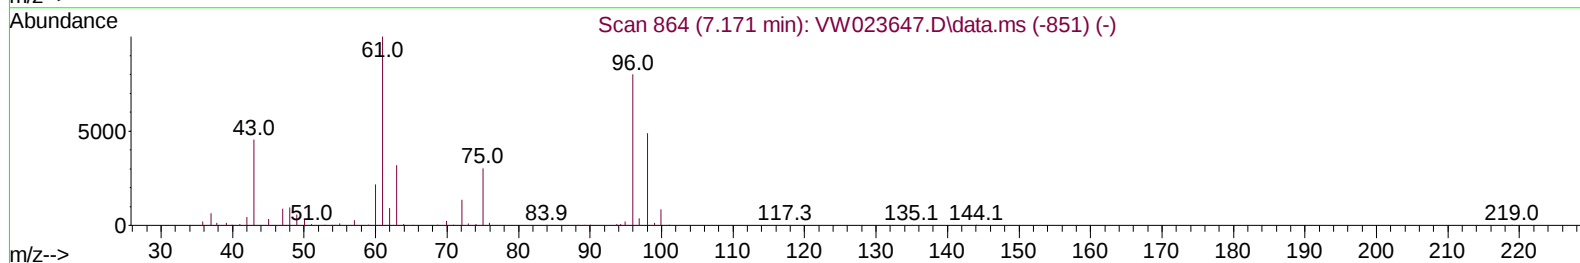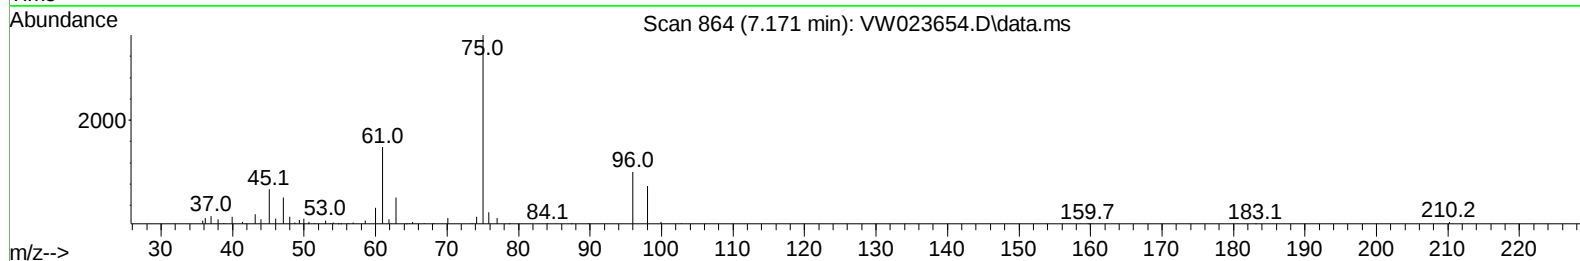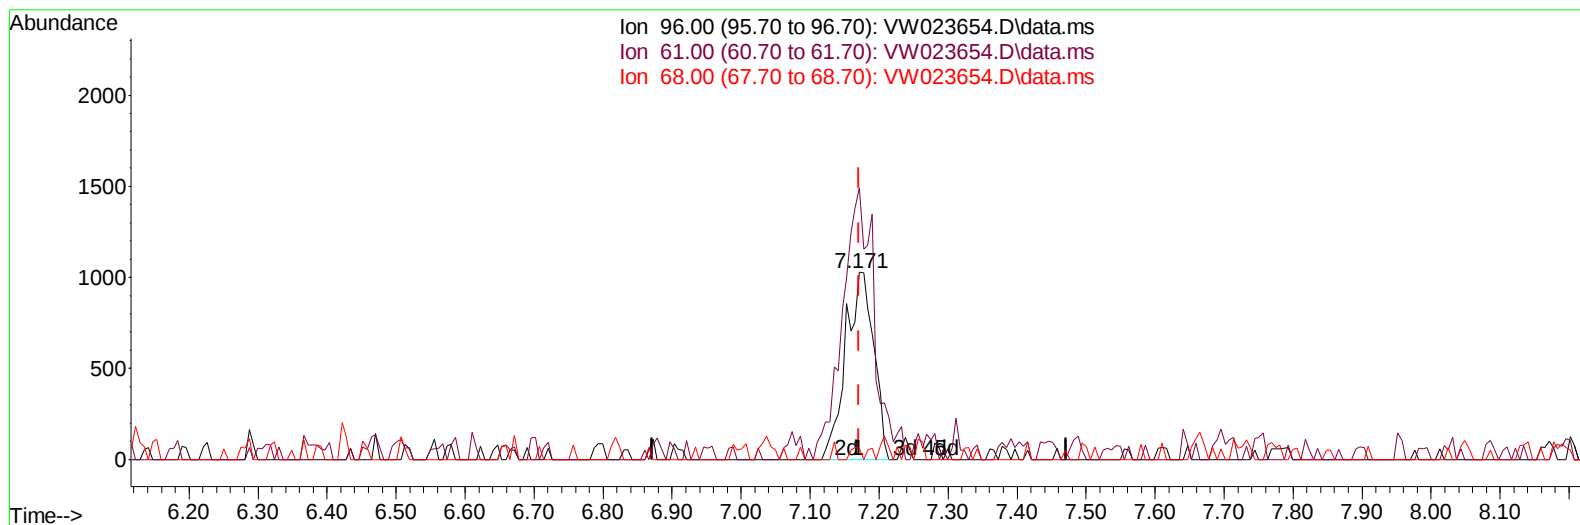

TIC: VW023654.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.171min (0.000) 7.04 ug/L m

response 2894

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.40	145.04
68.00	0.30	5.93#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023654.D
 Acq On : 13 Jul 2022 18:04
 Operator : SY/VA
 Sample : N3678-19
 Misc : 6.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B40

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:14:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	28842	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	25847	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	9714	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	19112	25.945	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	103.760%	
7) Chloroethane-d5	2.879	69	14263	29.023	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	116.080%	
11) 1,1-Dichloroethene-d2	4.013	63	12602	21.009	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	84.040%	
21) 2-Butanone-d5	7.080	46	10082	88.236	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	176.480%#	
24) Chloroform-d	7.647	84	20135	23.978	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.920%	
26) 1,2-Dichloroethane-d4	8.305	65	13700	26.675	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	106.720%	
32) Benzene-d6	8.281	84	34452	25.641	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	102.560%	
36) 1,2-Dichloropropane-d6	9.275	67	12455	30.774	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	123.080%#	
41) Toluene-d8	10.323	98	28542	20.943	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	83.760%	
43) trans-1,3-Dichloroprop...	10.579	79	4276	22.540	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.160%	
47) 2-Hexanone-d5	10.927	63	5081	59.703	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	119.400%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	14728	32.929	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	131.720%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	9004	25.965	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.880%	
Target Compounds						
5) vinyl chloride	2.349	62	24466	29.684	ug/L	Qvalue 93
13) Acetone	4.129	43	4390m	54.342	ug/L	
20) cis-1,2-Dichloroethene	7.171	96	2894m	7.042	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023654.D
Acq On : 13 Jul 2022 18:04
Operator : SY/VA
Sample : N3678-19
Misc : 6.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B40

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 02:14:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

