

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023657.D
 Acq On : 13 Jul 2022 19:18
 Operator : SY/VA
 Sample : N3676-10RE
 Misc : 6.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B09RE




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

07/14/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Jul 14 02:15:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Ion 96.00 (95.70 to 96.70): VW023657.D\data.ms
 Ion 61.00 (60.70 to 61.70): VW023657.D\data.ms
 Ion 98.00 (97.70 to 98.70): VW023657.D\data.ms

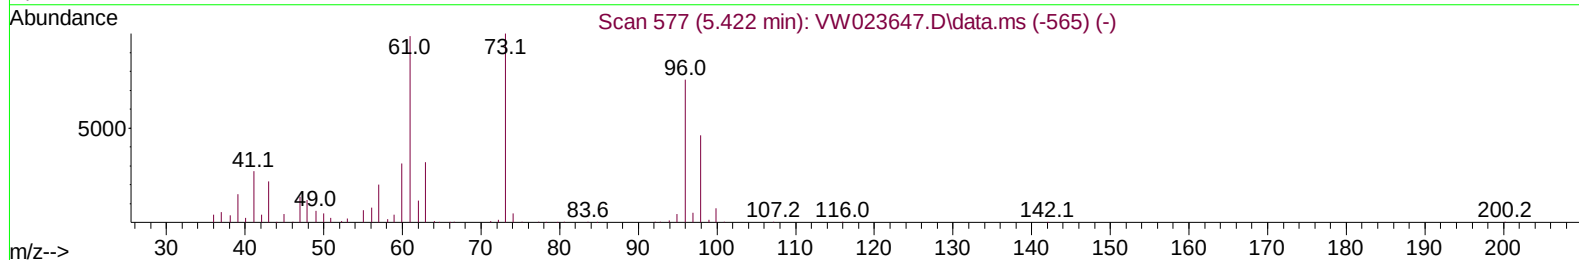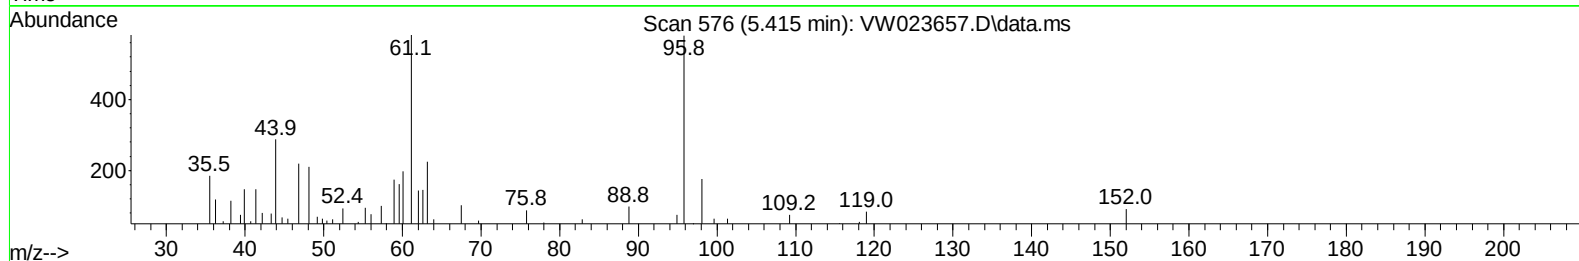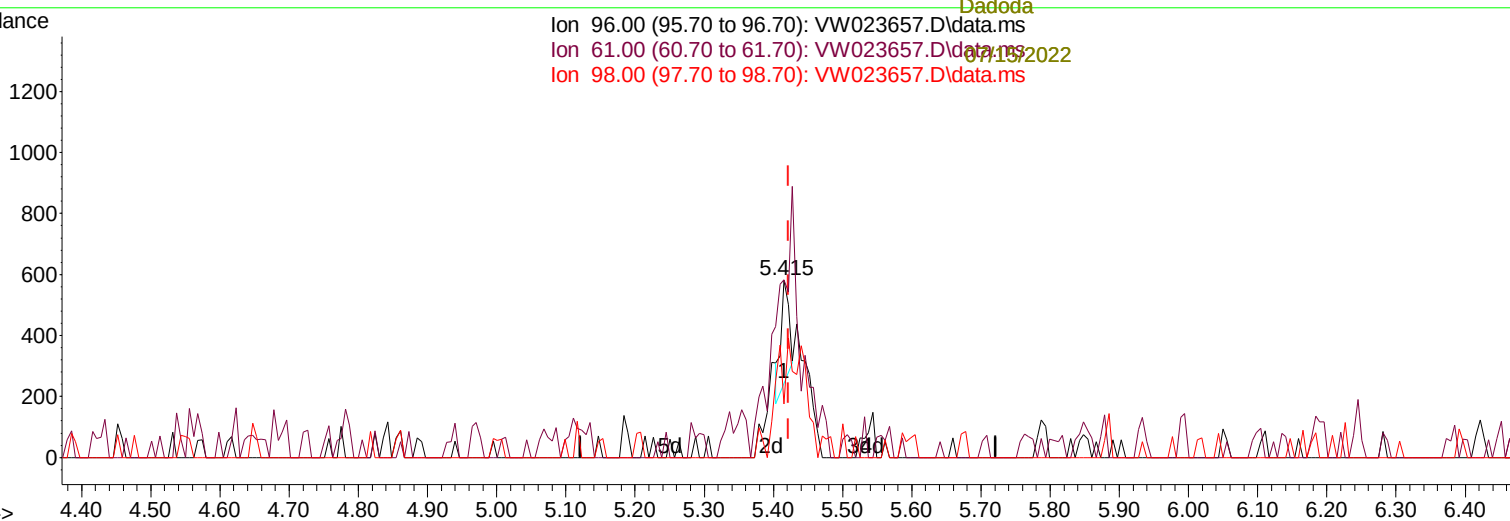

TIC: VW023657.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.415min (-0.006) 0.20 ug/L

response 278

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.70	100.17
98.00	61.20	30.29#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023657.D
 Acq On : 13 Jul 2022 19:18
 Operator : SY/VA
 Sample : N3676-10RE
 Misc : 6.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B09RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

07/14/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Jul 14 02:15:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

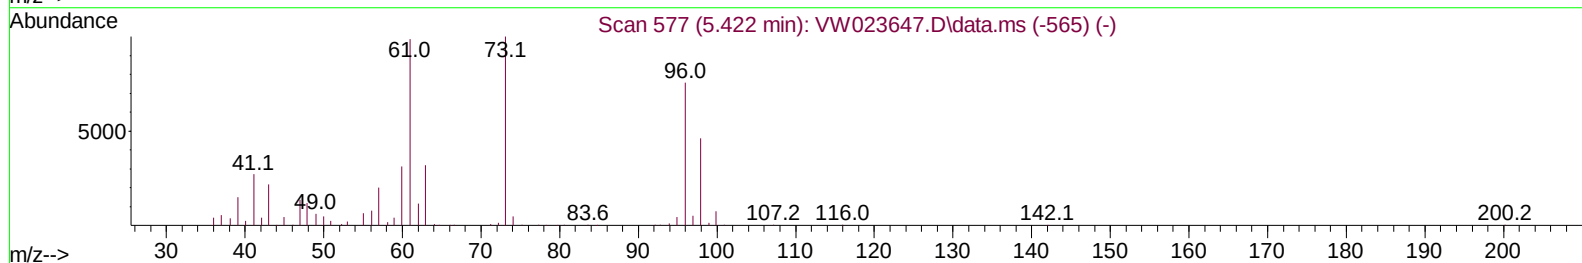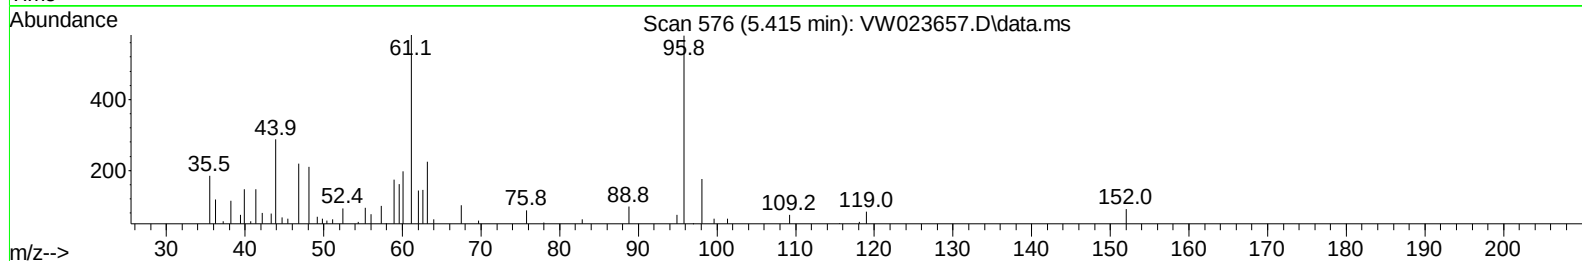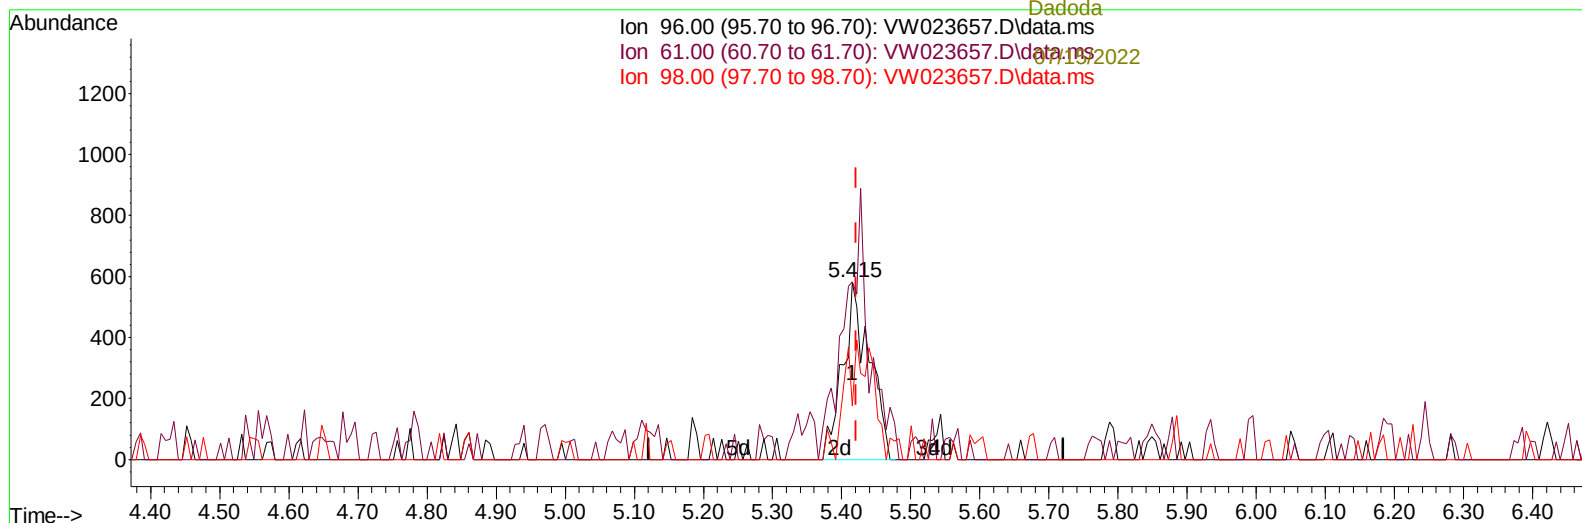

TIC: VW023657.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.415min (-0.006) 1.13 ug/L m

response 1564

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.70	100.17
98.00	61.20	30.29#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023657.D
 Acq On : 13 Jul 2022 19:18
 Operator : SY/VA
 Sample : N3676-10RE
 Misc : 6.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B09RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 02:15:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

07/14/2022
 Supervised By :Mahesh
 Dadoda

07/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----07/15/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	107936	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	99773	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	35263	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	66425	24.095	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.400%	
7) Chloroethane-d5	2.873	69	39956	21.726	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.920%	
11) 1,1-Dichloroethene-d2	4.001	63	40396	17.995	ug/L	-0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.000%	
21) 2-Butanone-d5	7.080	46	22972	53.723	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.440%	
24) Chloroform-d	7.653	84	78263	24.905	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.600%	
26) 1,2-Dichloroethane-d4	8.305	65	46700	24.298	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.200%	
32) Benzene-d6	8.275	84	136730	26.363	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	105.440%	
36) 1,2-Dichloropropane-d6	9.268	67	43019	27.536	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	110.160%	
41) Toluene-d8	10.323	98	115636	21.981	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.920%	
43) trans-1,3-Dichloroprop...	10.579	79	14417	19.687	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	78.760%	
47) 2-Hexanone-d5	10.921	63	15536	47.292	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.580%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	39996	23.166	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	92.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	34078	27.072	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	108.280%	
Target Compounds						
13) Acetone	4.123	43	13009	43.030	ug/L	88
17) trans-1,2-Dichloroethene	5.415	96	1564m	1.127	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023657.D
Acq On : 13 Jul 2022 19:18
Operator : SY/VA
Sample : N3676-10RE
Misc : 6.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B09RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

07/14/2022
Supervised By :Mahesh
Dadoda

07/15/2022

