




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023659.D
 Acq On : 13 Jul 2022 20:07
 Operator : SY/VA
 Sample : N3678-01RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B20RE

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:15:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

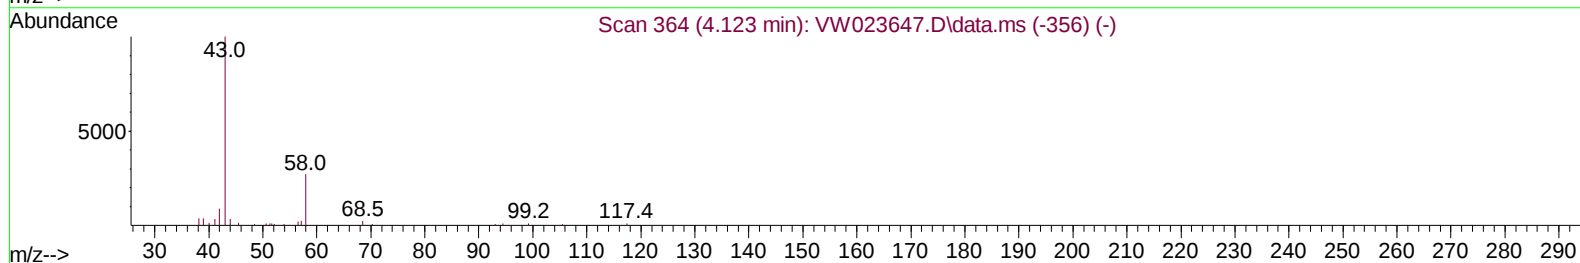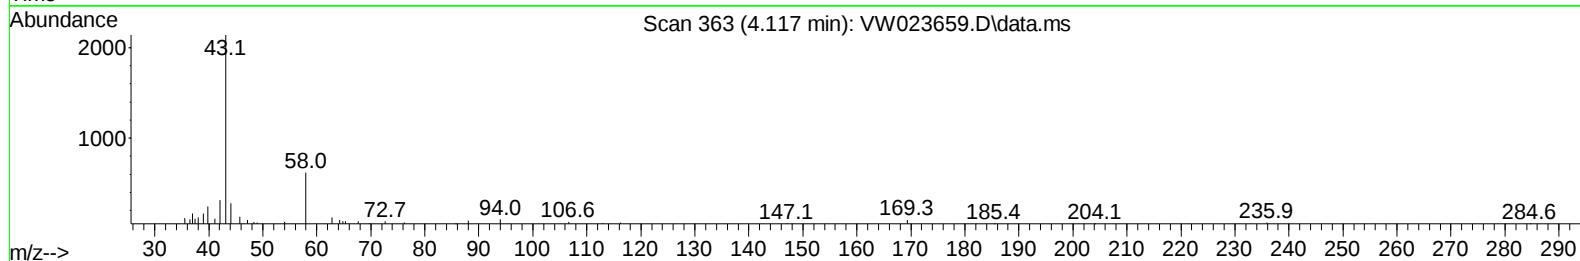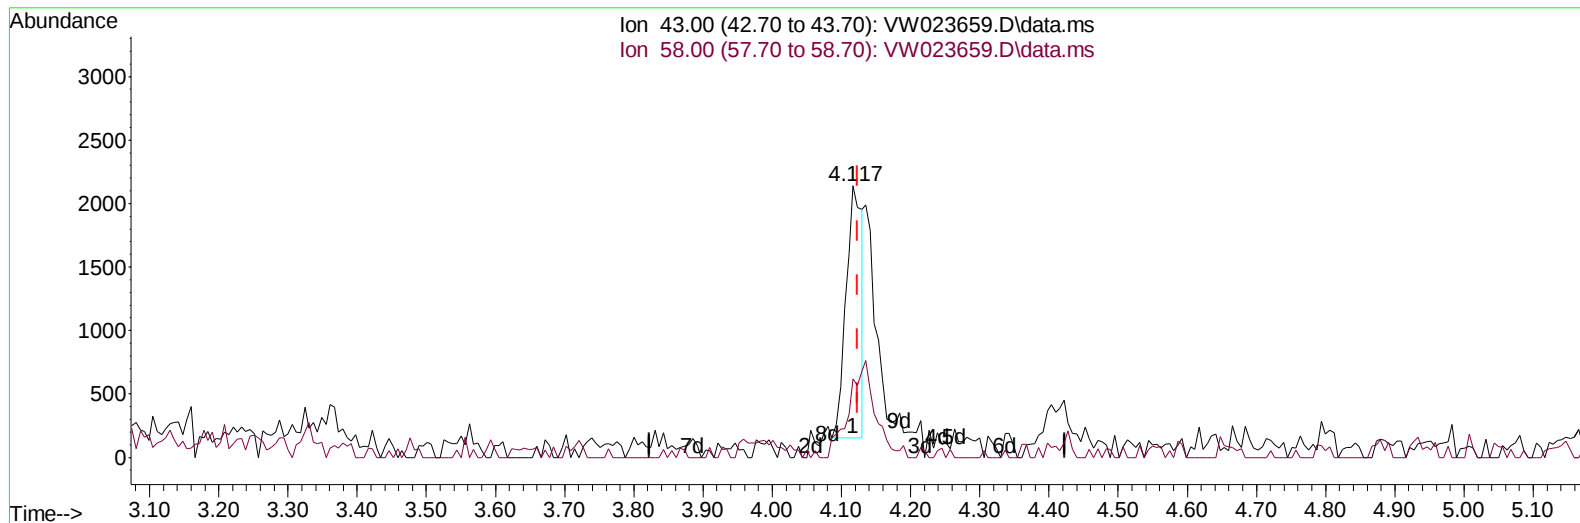

TIC: VW023659.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 16.71 ug/L

response 3133

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	63.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023659.D
 Acq On : 13 Jul 2022 20:07
 Operator : SY/VA
 Sample : N3678-01RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B20RE

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:15:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

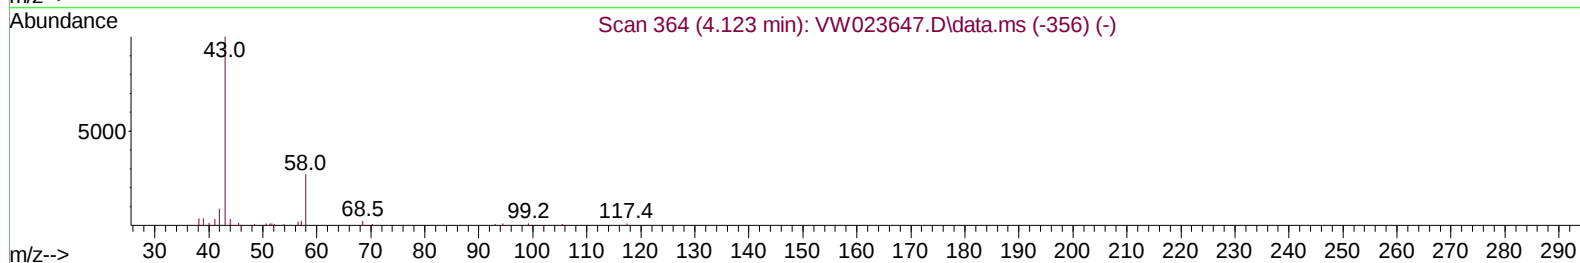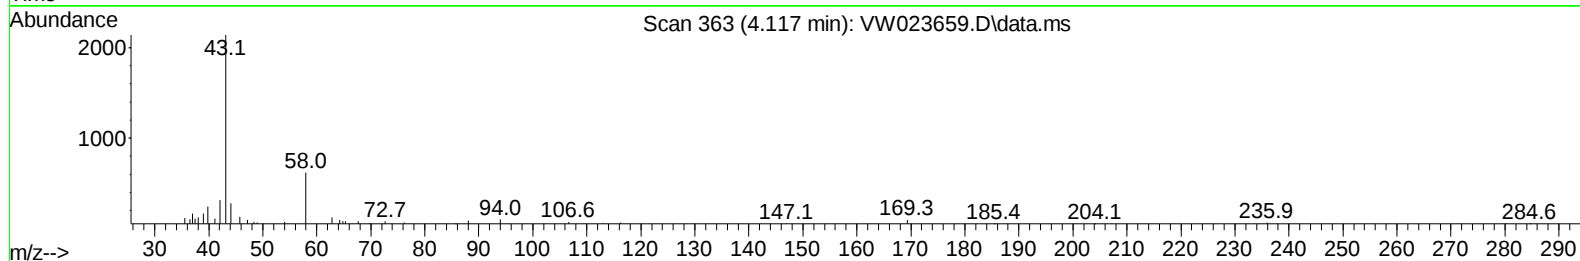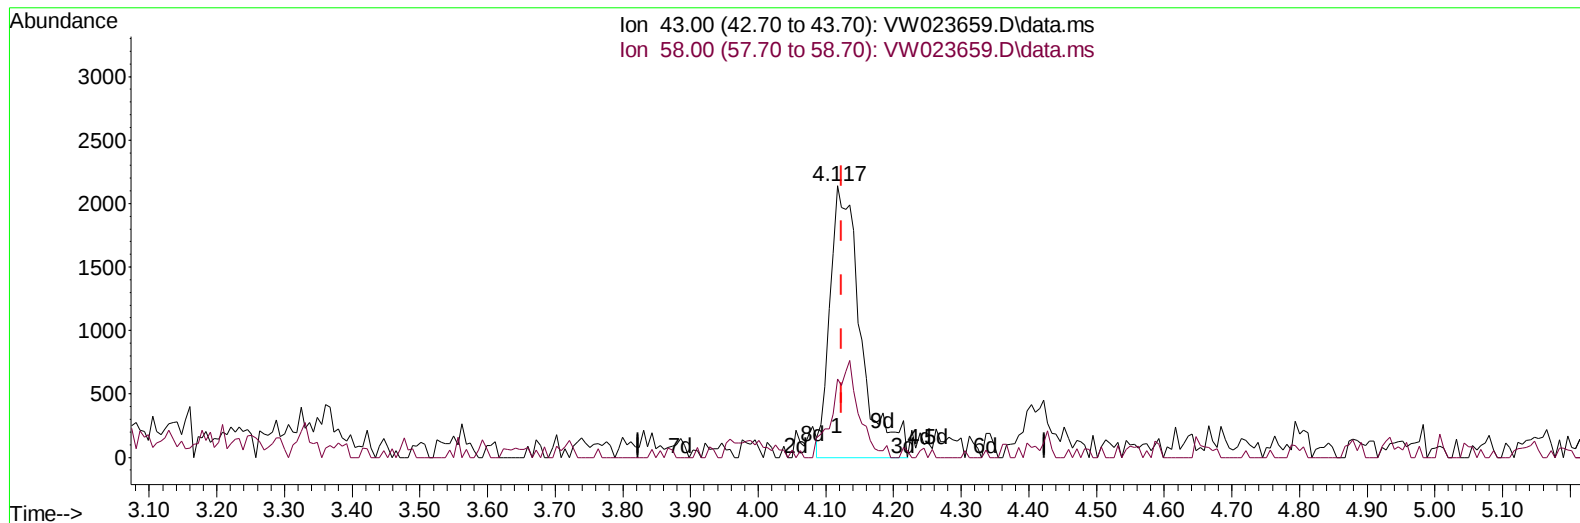

TIC: VW023659.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 35.73 ug/L m

response 6699

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	29.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023659.D
Acq On : 13 Jul 2022 20:07
Operator : SY/VA
Sample : N3678-01RE
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B20RE

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:15:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

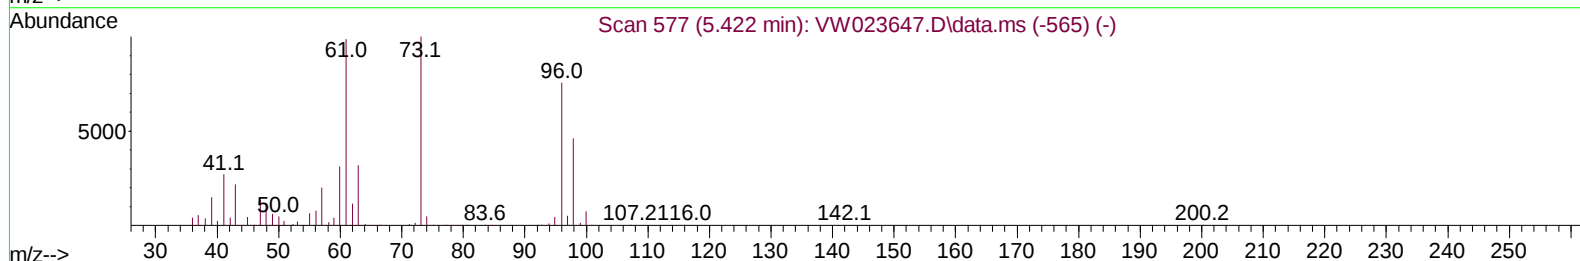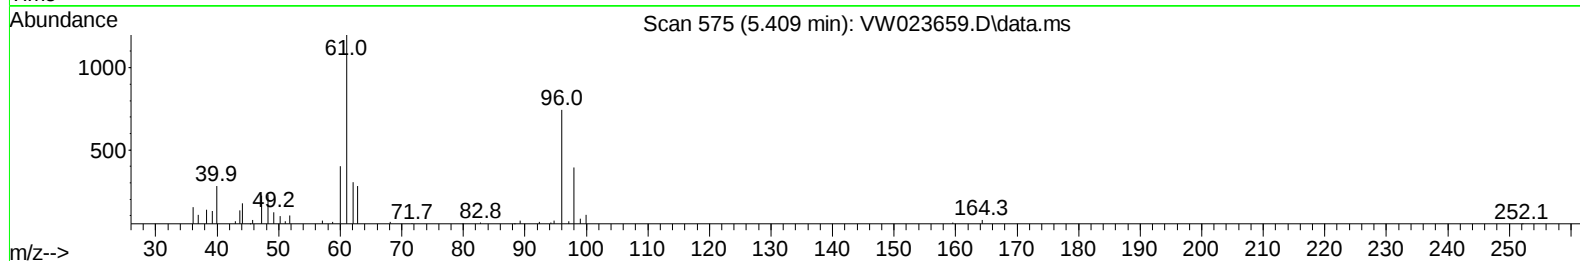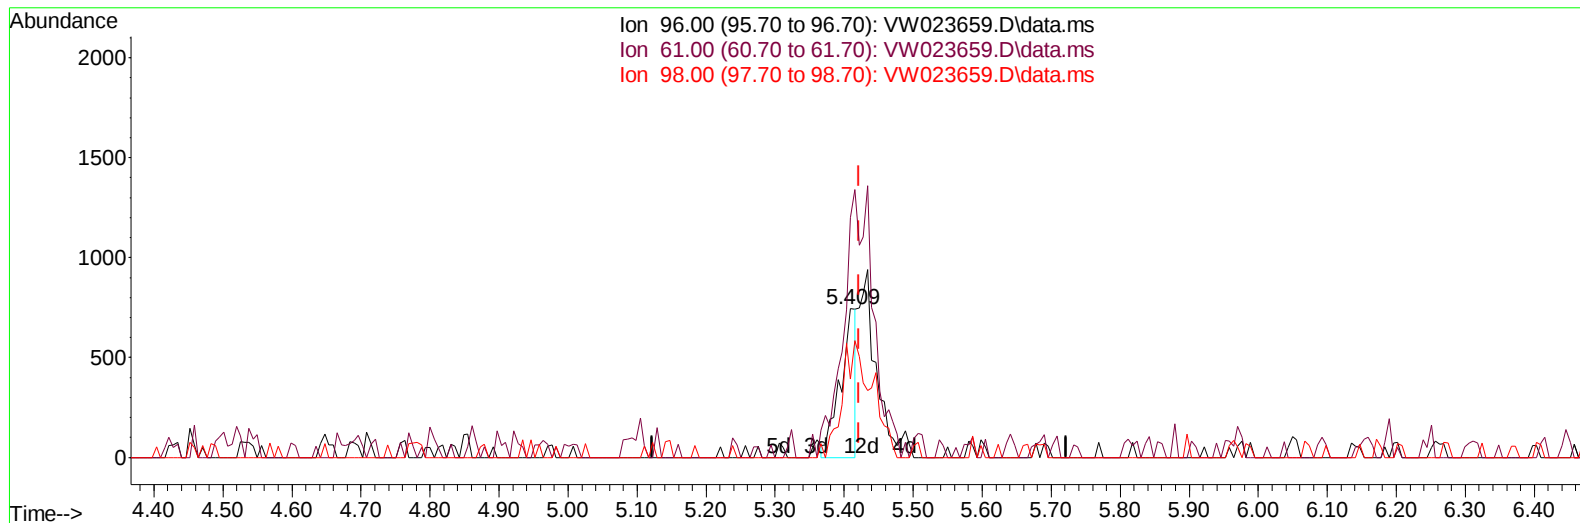

TIC: VW023659.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.409min (-0.012) 1.37 ug/L

response 1176

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.70	161.16
98.00	61.20	52.69
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023659.D
Acq On : 13 Jul 2022 20:07
Operator : SY/VA
Sample : N3678-01RE
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B20RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 02:15:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

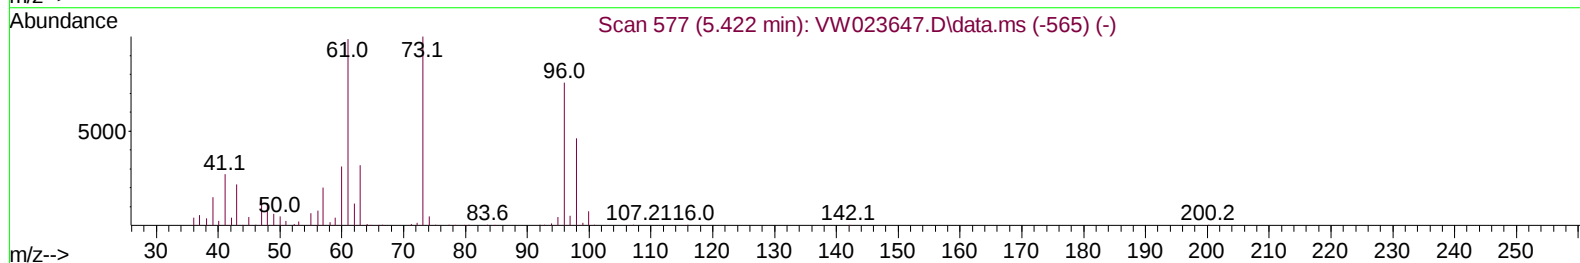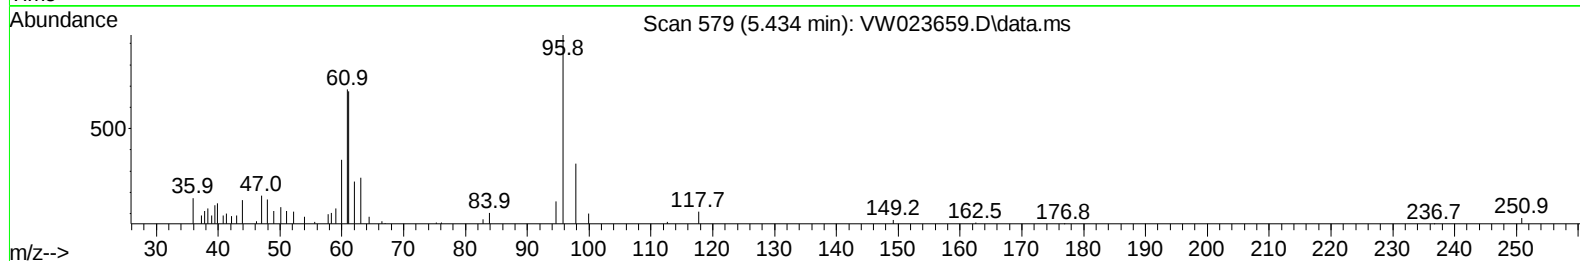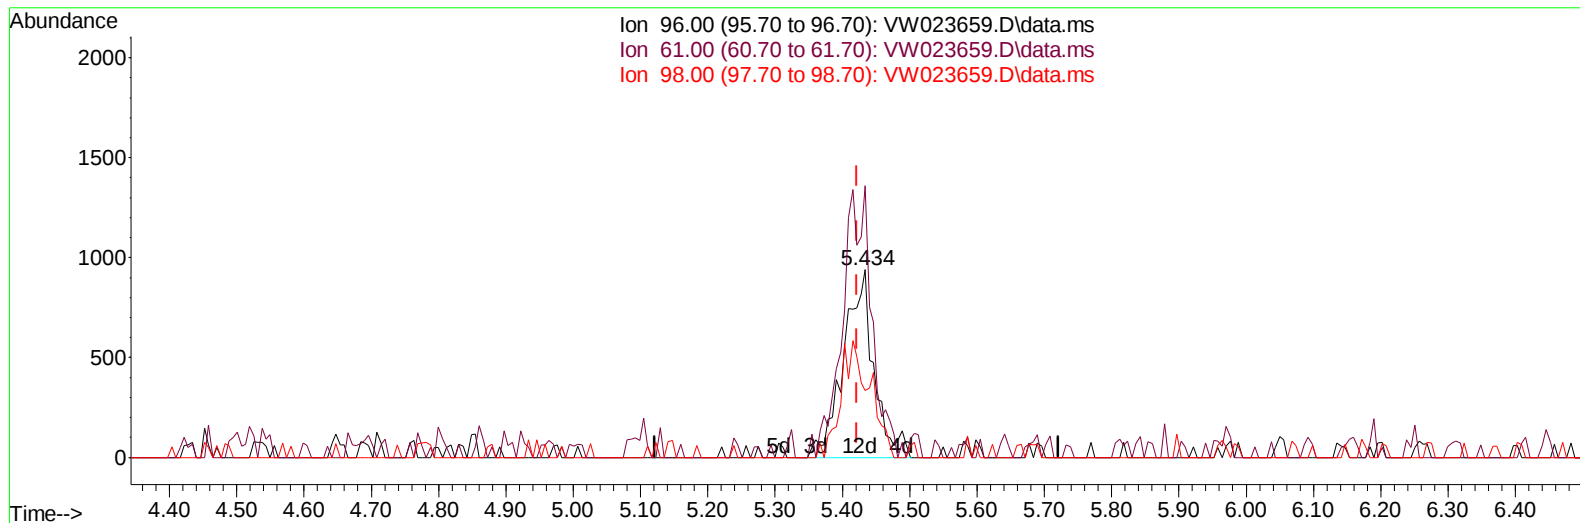

TIC: VW023659.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.434min (+ 0.012) 3.40 ug/L m

response 2927

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.70	72.77#
98.00	61.20	35.74#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023659.D
 Acq On : 13 Jul 2022 20:07
 Operator : SY/VA
 Sample : N3678-01RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B20RE

Manual IntegrationsAPPROVED

Quant Time: Jul 14 02:15:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	66931	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	63925	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	22788	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	45036	26.345	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.360%	
7) Chloroethane-d5	2.873	69	28123	24.660	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	98.640%	
11) 1,1-Dichloroethene-d2	4.001	63	28553	20.512	ug/L	-0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	82.040%	
21) 2-Butanone-d5	7.086	46	16803	63.370	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	126.740%	
24) Chloroform-d	7.647	84	51363	26.358	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	105.440%	
26) 1,2-Dichloroethane-d4	8.305	65	30571	25.651	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	102.600%	
32) Benzene-d6	8.269	84	87198	26.241	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	104.960%	
36) 1,2-Dichloropropane-d6	9.275	67	28363	28.336	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	113.360%	
41) Toluene-d8	10.323	98	72628	21.547	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	86.200%	
43) trans-1,3-Dichloroprop...	10.579	79	8852	18.867	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	75.480%	
47) 2-Hexanone-d5	10.927	63	10151	48.228	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.460%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	26723	24.158	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	96.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152	22119	27.190	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	108.760%	
Target Compounds						
13) Acetone	4.117	43	6699m	35.734	ug/L	Qvalue
17) trans-1,2-Dichloroethene	5.434	96	2927m	3.400	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023659.D
Acq On : 13 Jul 2022 20:07
Operator : SY/VA
Sample : N3678-01RE
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B20RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 02:15:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

