




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023672.D
 Acq On : 14 Jul 2022 02:41
 Operator : SY/VA
 Sample : N3679-06
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B46

Manual IntegrationsAPPROVED

Quant Time: Jul 14 06:05:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

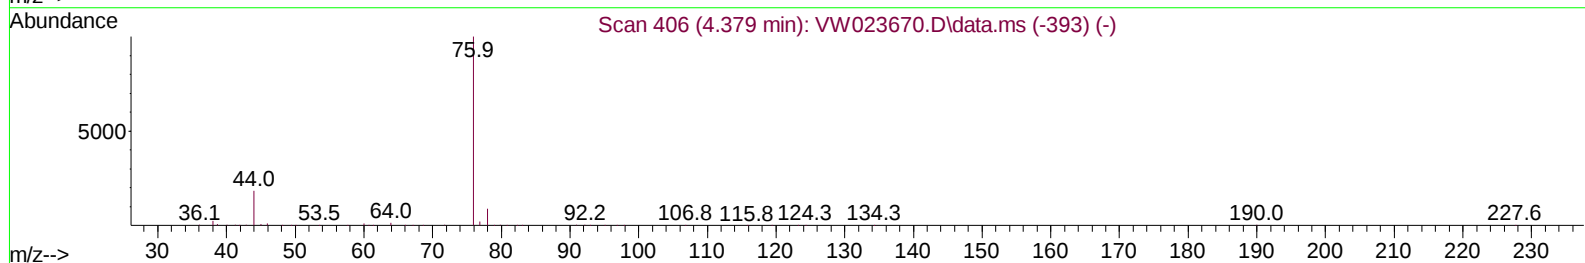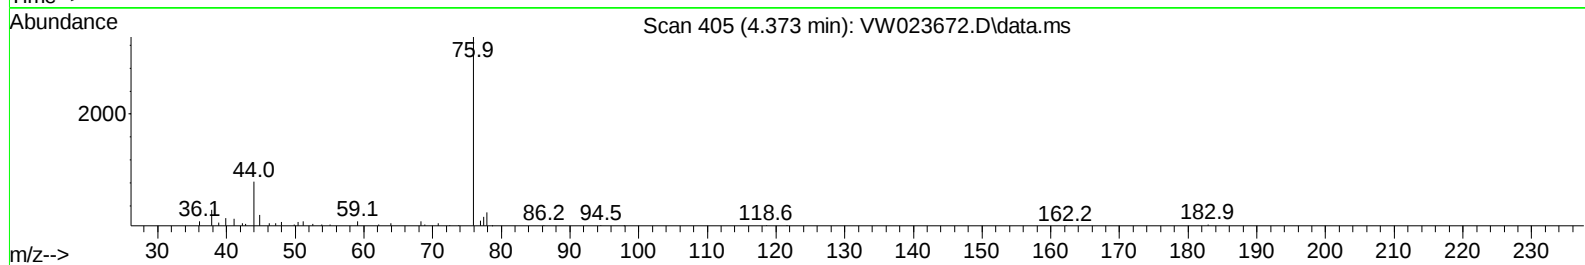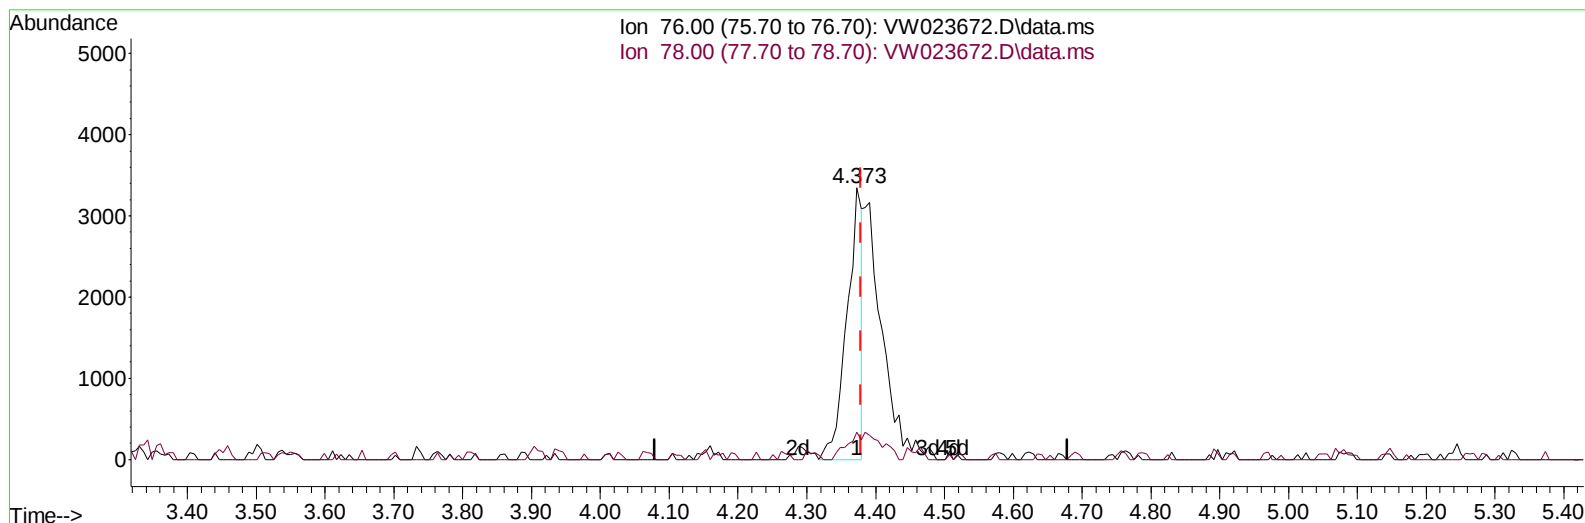

TIC: VW023672.D\data.ms

(14) Carbon disulfide (T)

4.373min (-0.006) 0.82 ug/L

response 5157

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	9.99
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023672.D
 Acq On : 14 Jul 2022 02:41
 Operator : SY/VA
 Sample : N3679-06
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B46

Manual IntegrationsAPPROVED

Quant Time: Jul 14 06:05:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

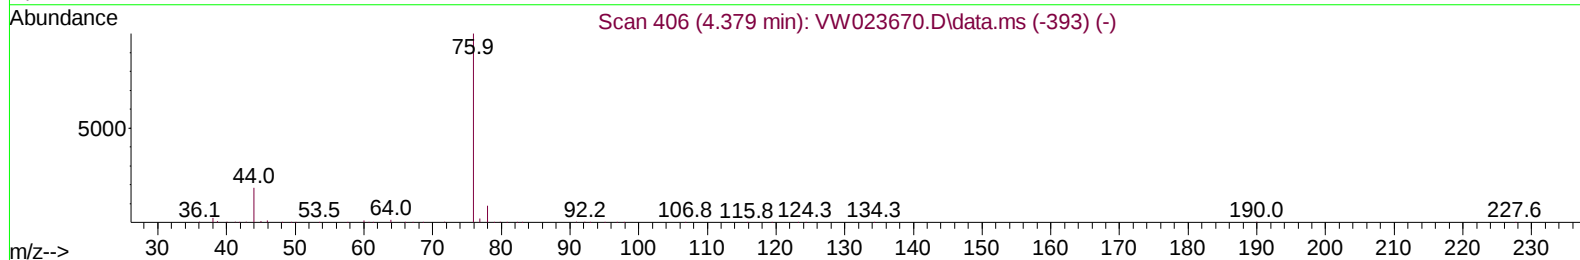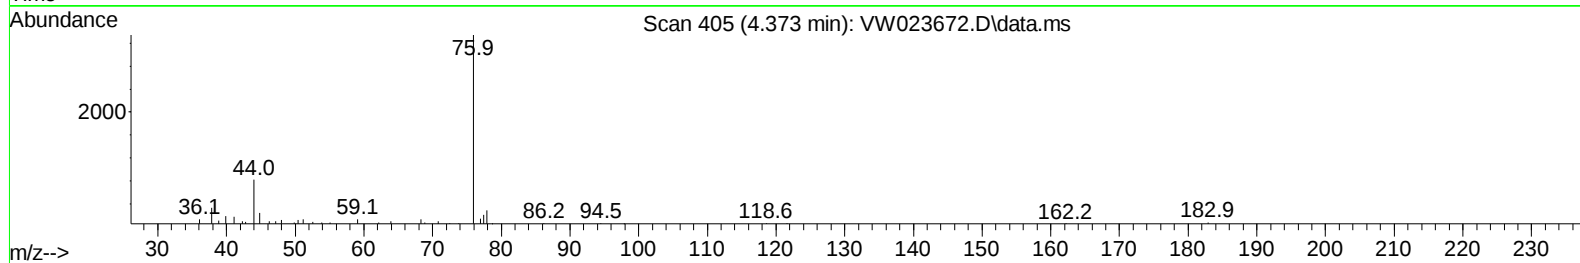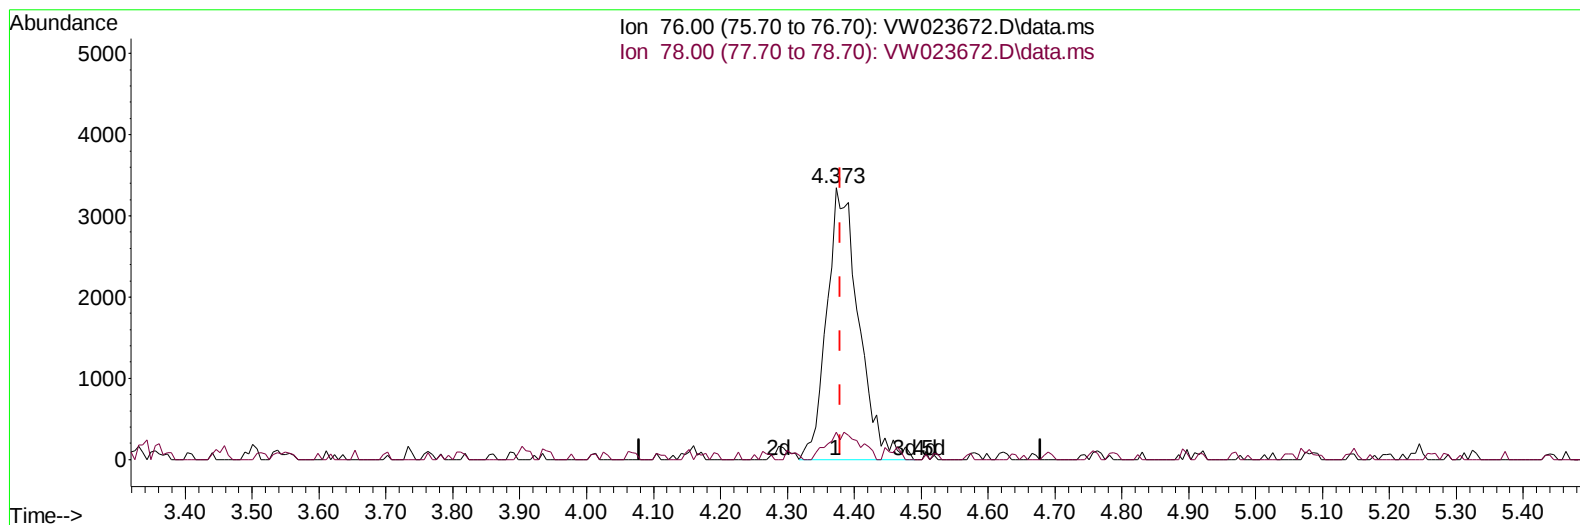

TIC: VW023672.D\data.ms

(14) Carbon disulfide (T)

4.373min (-0.006) 1.77 ug/L m

response 11111

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	8.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023672.D
 Acq On : 14 Jul 2022 02:41
 Operator : SY/VA
 Sample : N3679-06
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B46

Manual IntegrationsAPPROVED

Quant Time: Jul 14 06:05:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	200992	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	186806	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	74599	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	91343	17.794	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.160%	
7) Chloroethane-d5	2.879	69	70731	20.653	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.600%	
11) 1,1-Dichloroethene-d2	4.013	63	54237	12.975	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.880%	
21) 2-Butanone-d5	7.080	46	38624	48.507	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	97.020%	
24) Chloroform-d	7.647	84	129642	22.154	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.600%	
26) 1,2-Dichloroethane-d4	8.305	65	80015	22.357	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	89.440%	
32) Benzene-d6	8.275	84	232038	23.895	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	95.560%	
36) 1,2-Dichloropropane-d6	9.274	67	75108	25.677	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.720%	
41) Toluene-d8	10.323	98	216145	21.944	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.760%	
43) trans-1,3-Dichloroprop...	10.579	79	22968	16.752	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	67.000%	
47) 2-Hexanone-d5	10.920	63	28967	47.095	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.180%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	69118	21.382	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.520%	
66) 1,2-Dichlorobenzene-d4	13.853	152	65105	24.448	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.800%	
Target Compounds						
					Qvalue	
5) vinyl chloride	2.355	62	26955	4.693	ug/L #	77
13) Acetone	4.129	43	7257	12.891	ug/L	86
14) Carbon disulfide	4.373	76	11111m	1.773	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023672.D
Acq On : 14 Jul 2022 02:41
Operator : SY/VA
Sample : N3679-06
Misc : 6.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B46

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 06:05:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 04:56:40 2022
Response via : Initial Calibration

