




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023680.D
Acq On : 14 Jul 2022 05:57
Operator : SY/VA
Sample : N3679-14
Misc : 6.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B54

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 06:42:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 04:56:40 2022
Response via : Initial Calibration

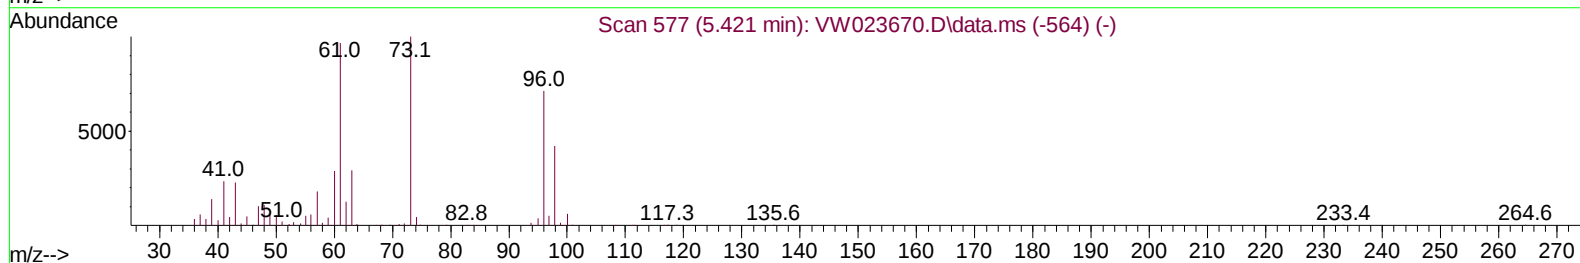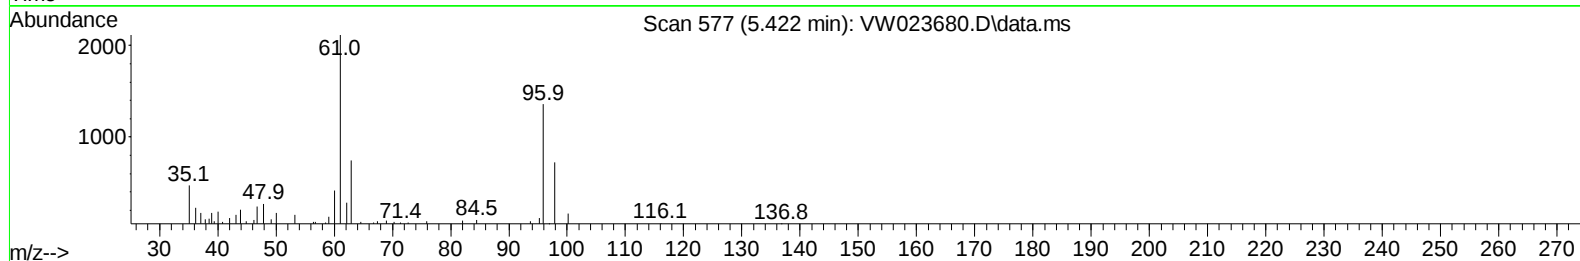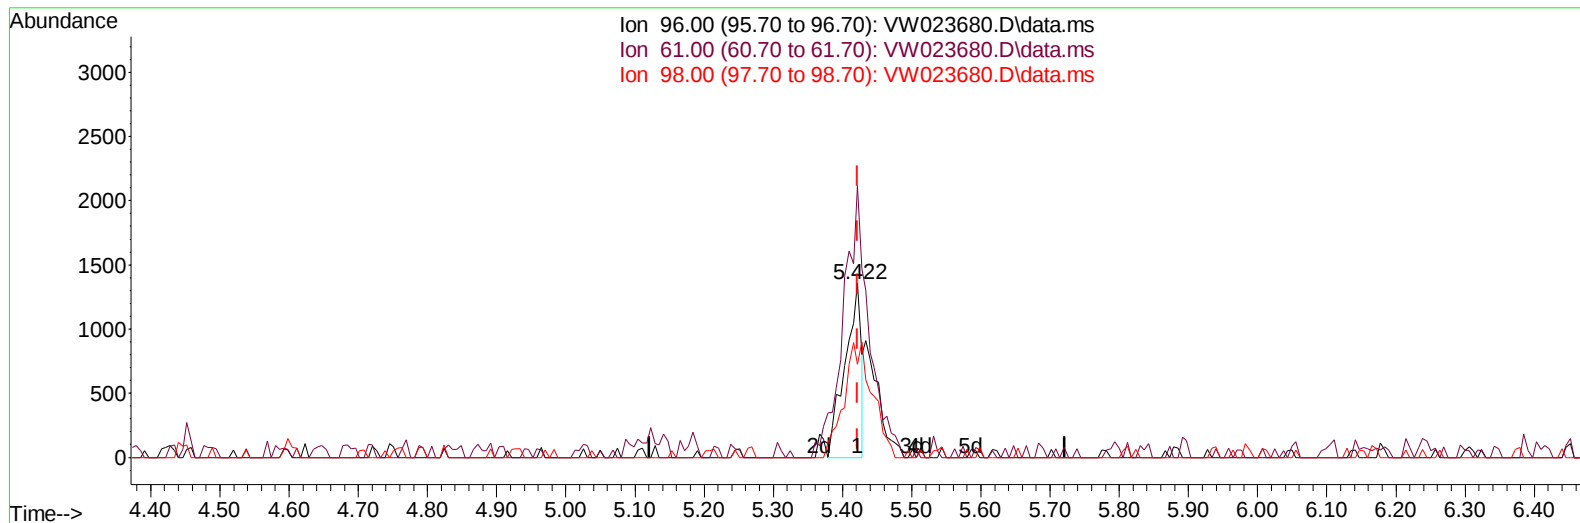

TIC: VW023680.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.422min (+ 0.000) 0.91 ug/L

response 2211

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.70	155.86
98.00	61.20	53.43
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023680.D
 Acq On : 14 Jul 2022 05:57
 Operator : SY/VA
 Sample : N3679-14
 Misc : 6.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B54

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 06:42:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

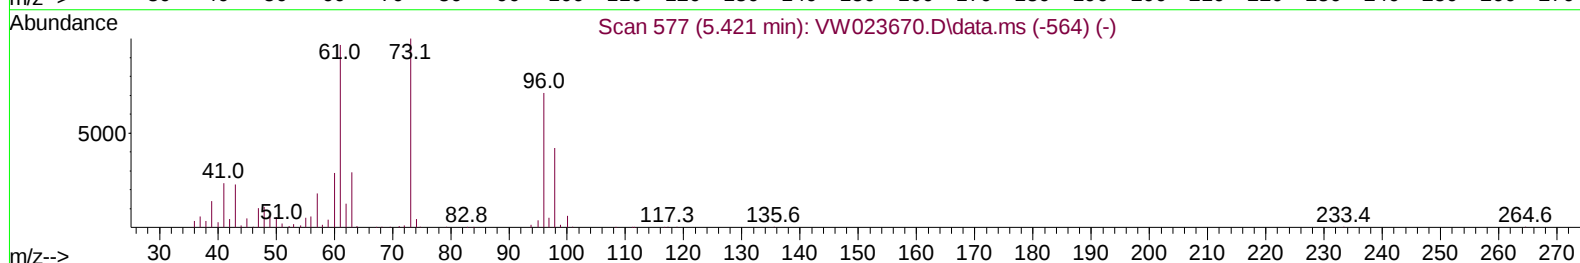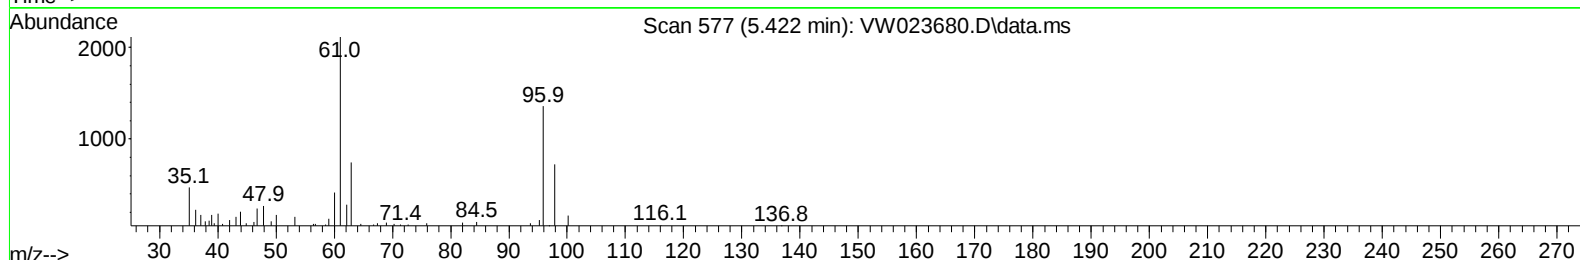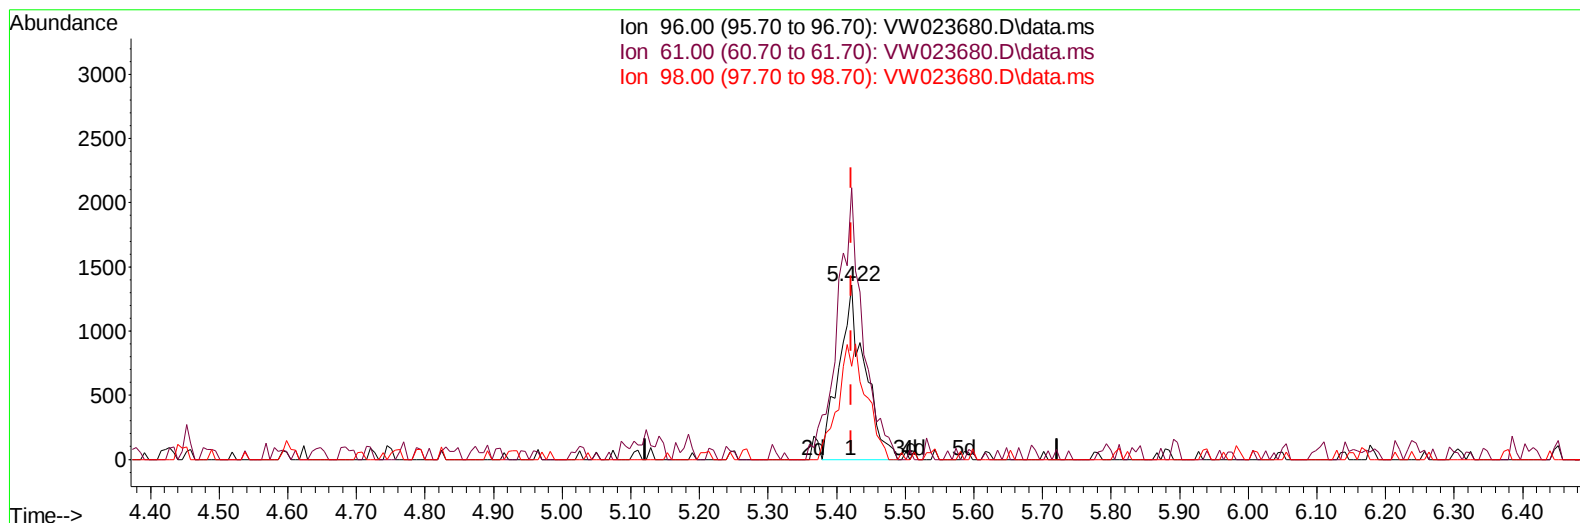

TIC: VW023680.D\data.ms

(17) trans-1,2-Dichloroethene (T)

5.422min (+ 0.000) 1.45 ug/L m

response 3533

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	129.70	155.86
98.00	61.20	53.43
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023680.D
 Acq On : 14 Jul 2022 05:57
 Operator : SY/VA
 Sample : N3679-14
 Misc : 6.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B54

Manual IntegrationsAPPROVED

Quant Time: Jul 14 06:42:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	189608	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	174161	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	58630	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	90528	18.694	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.760%	
7) Chloroethane-d5	2.879	69	70059	21.685	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.760%	
11) 1,1-Dichloroethene-d2	4.013	63	52303	13.263	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.040%	
21) 2-Butanone-d5	7.074	46	40299	53.649	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.300%	
24) Chloroform-d	7.647	84	130682	23.673	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	94.680%	
26) 1,2-Dichloroethane-d4	8.305	65	80253	23.769	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	95.080%	
32) Benzene-d6	8.269	84	229608	25.361	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	101.440%	
36) 1,2-Dichloropropane-d6	9.275	67	74827	27.439	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	109.760%	
41) Toluene-d8	10.323	98	201895	21.985	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.960%	
43) trans-1,3-Dichloroprop...	10.579	79	19333	15.124	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	60.480%	
47) 2-Hexanone-d5	10.927	63	28806	50.233	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.460%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	66578	22.091	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	88.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	52329	25.002	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.000%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	2.355	62	19525	3.603	ug/L #	71
13) Acetone	4.129	43	17602	33.144	ug/L	96
14) Carbon disulfide	4.379	76	6991	1.182	ug/L #	94
17) trans-1,2-Dichloroethene	5.422	96	3533m	1.449	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023680.D
Acq On : 14 Jul 2022 05:57
Operator : SY/VA
Sample : N3679-14
Misc : 6.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B54

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 06:42:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 04:56:40 2022
Response via : Initial Calibration

