




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023685.D
 Acq On : 14 Jul 2022 07:59
 Operator : SY/VA
 Sample : N3698-05
 Misc : 5.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B70

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:31:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

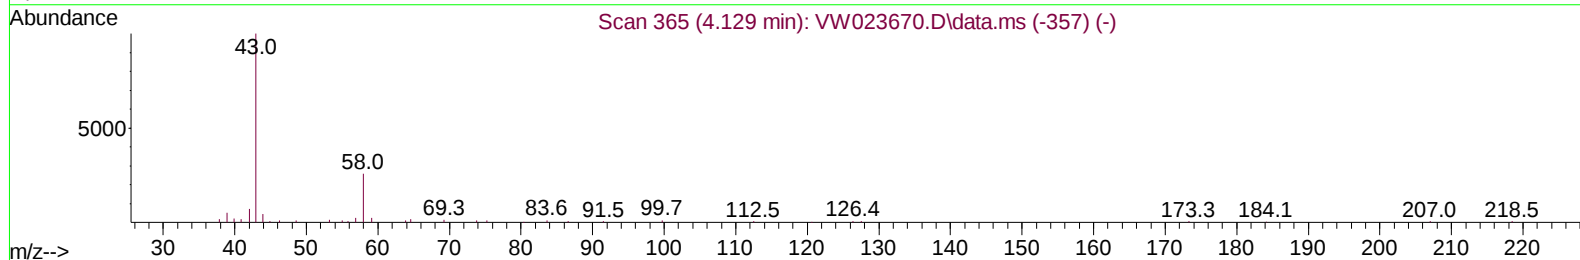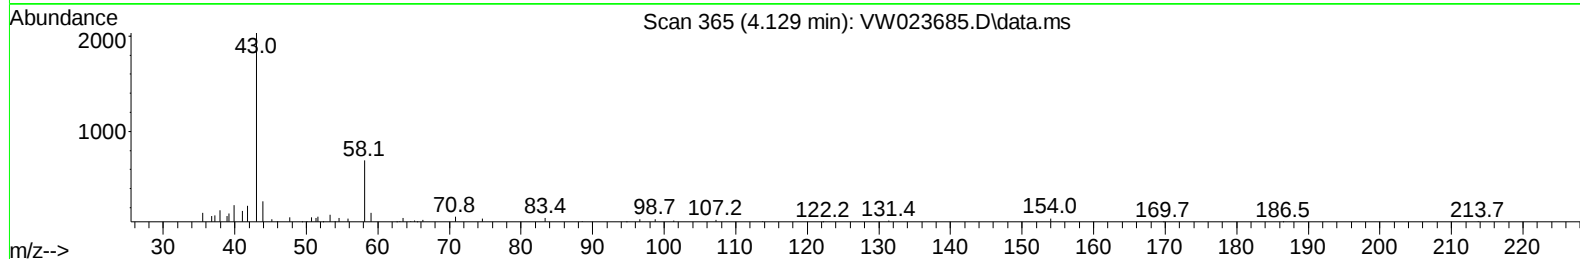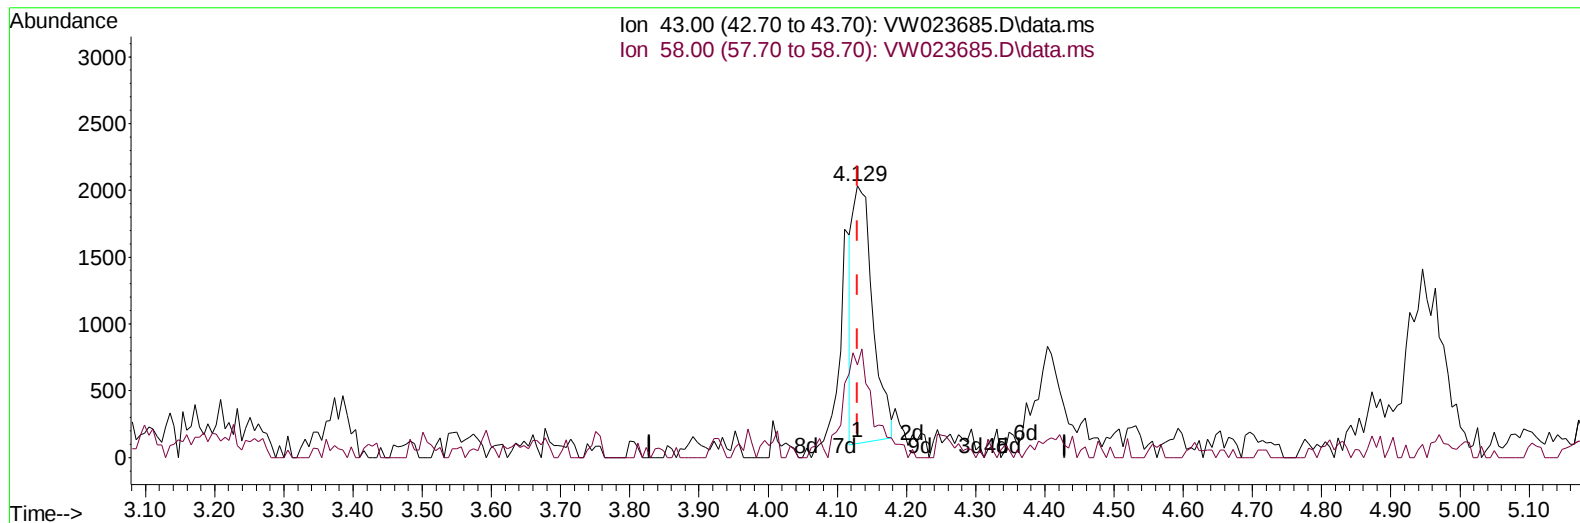

TIC: VW023685.D\data.ms

(13) Acetone (T)

4.129min (+ 0.000) 10.81 ug/L

response 3921

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	49.96
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023685.D
 Acq On : 14 Jul 2022 07:59
 Operator : SY/VA
 Sample : N3698-05
 Misc : 5.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B70

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:31:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

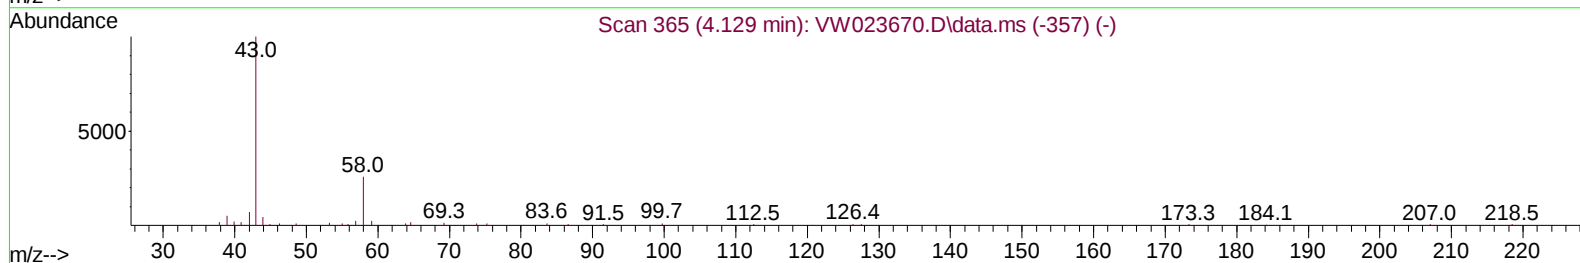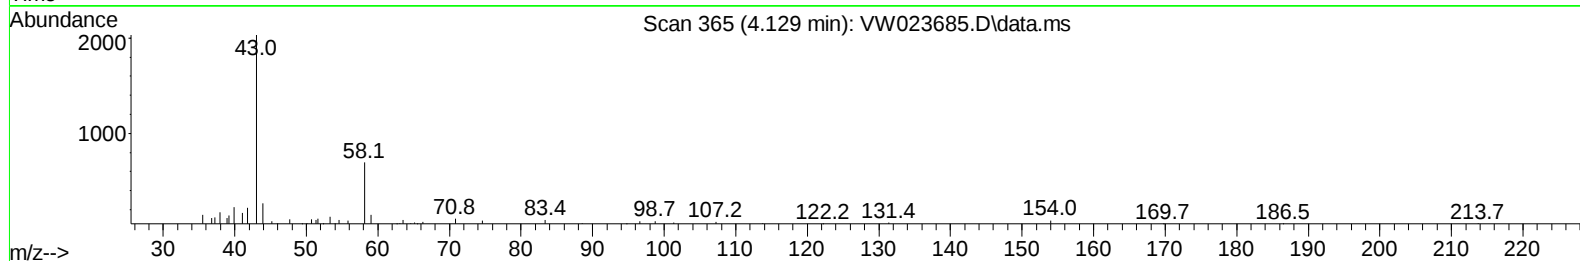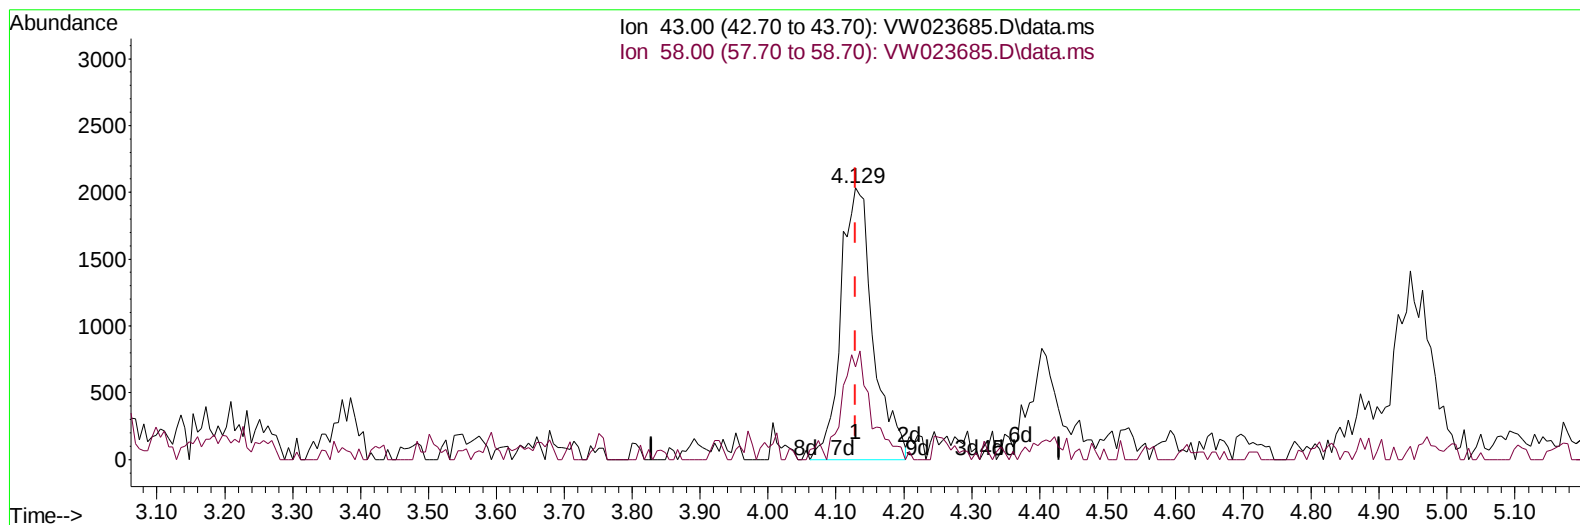

TIC: VW023685.D\data.ms

(13) Acetone (T)

4.129min (+ 0.000) 18.47 ug/L m

response 6699

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	29.24
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023685.D
 Acq On : 14 Jul 2022 07:59
 Operator : SY/VA
 Sample : N3698-05
 Misc : 5.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B70

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:31:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	129512	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	120776	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	51235	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	61958	18.731	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.920%	
7) Chloroethane-d5	2.879	69	45003	20.394	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	81.560%	
11) 1,1-Dichloroethene-d2	4.007	63	42589	15.811	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	63.240%	
21) 2-Butanone-d5	7.074	46	23266	45.346	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	90.700%	
24) Chloroform-d	7.653	84	84834	22.498	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.000%	
26) 1,2-Dichloroethane-d4	8.299	65	50652	21.964	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	87.840%	
32) Benzene-d6	8.275	84	158490	25.244	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	100.960%	
36) 1,2-Dichloropropane-d6	9.274	67	48293	25.536	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.160%	
41) Toluene-d8	10.323	98	141145	22.164	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	88.640%	
43) trans-1,3-Dichloroprop...	10.579	79	15123	17.060	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	68.240%	
47) 2-Hexanone-d5	10.920	63	15593	39.211	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	78.420%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	42485	20.328	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	81.320%	
66) 1,2-Dichlorobenzene-d4	13.853	152	45297	24.766	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.080%	
Target Compounds						
5) vinyl chloride	2.355	62	32058	8.662	ug/L	91
13) Acetone	4.129	43	6699m	18.467	ug/L	
20) cis-1,2-Dichloroethene	7.165	96	30756	16.667	ug/L #	97
34) Trichloroethene	9.098	95	2267	1.251	ug/L	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023685.D
Acq On : 14 Jul 2022 07:59
Operator : SY/VA
Sample : N3698-05
Misc : 5.81g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B70

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:31:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 04:56:40 2022
Response via : Initial Calibration

