

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023686.D
 Acq On : 14 Jul 2022 08:23
 Operator : SY/VA
 Sample : N3698-06
 Misc : 5.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B71

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:32:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

07/15/2022
 Supervised By :Mahesh
 Dadoda

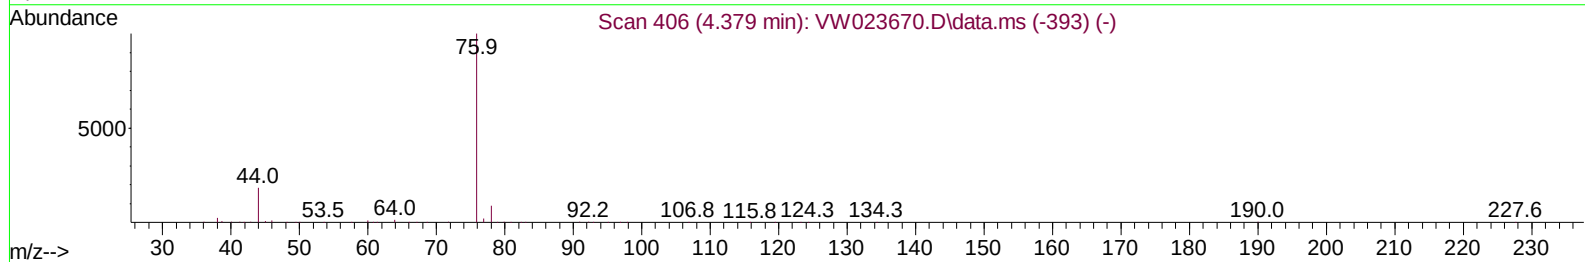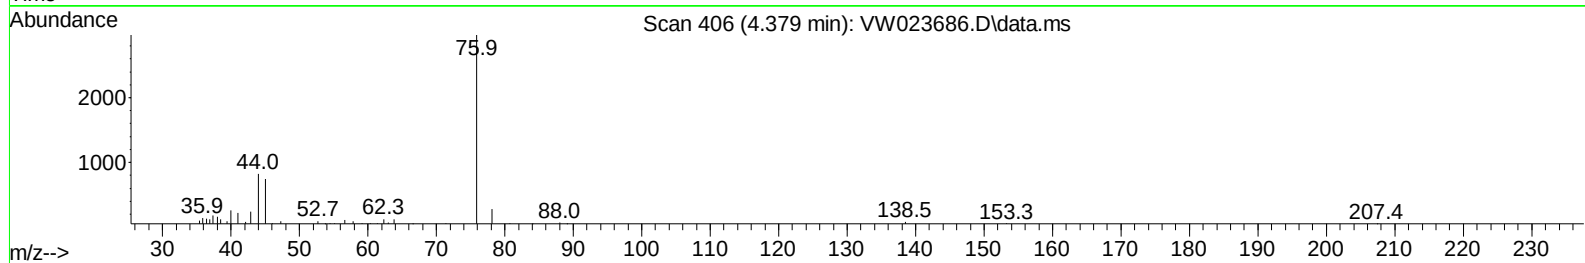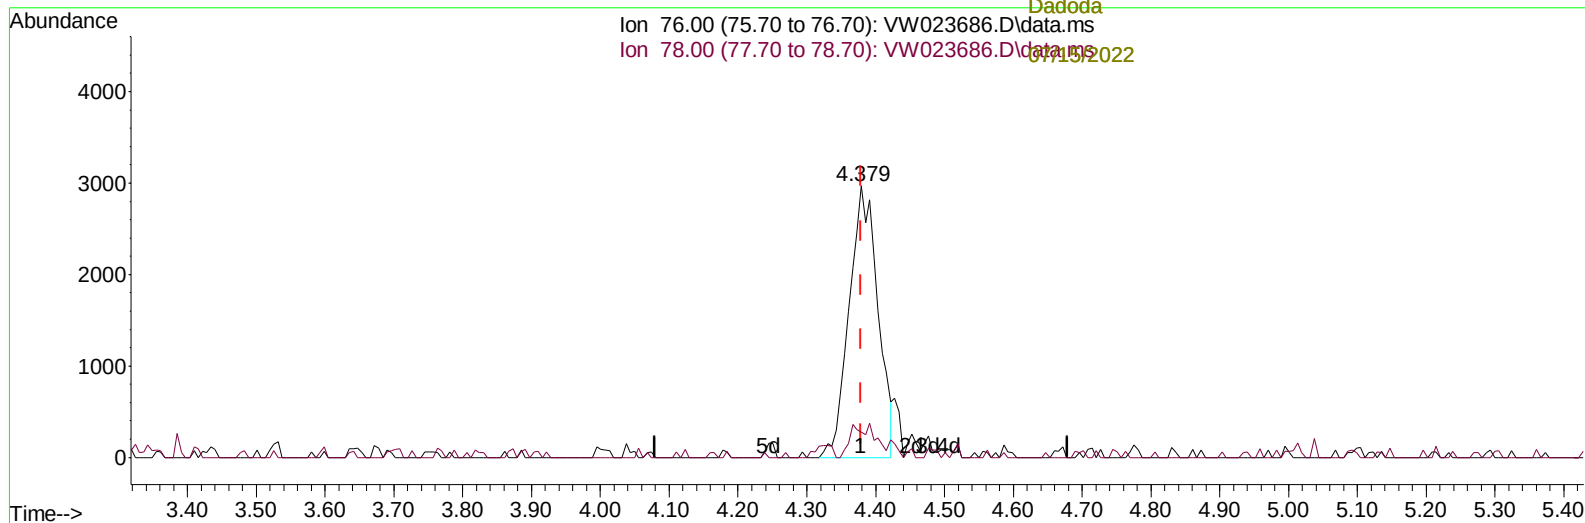

TIC: VW023686.D\data.ms

(14) Carbon disulfide (T)

4.379min (+ 0.000) 1.44 ug/L

response 8561

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	9.23
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023686.D
 Acq On : 14 Jul 2022 08:23
 Operator : SY/VA
 Sample : N3698-06
 Misc : 5.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B71

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:32:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

07/15/2022
 Supervised By :Mahesh
 Dadoda

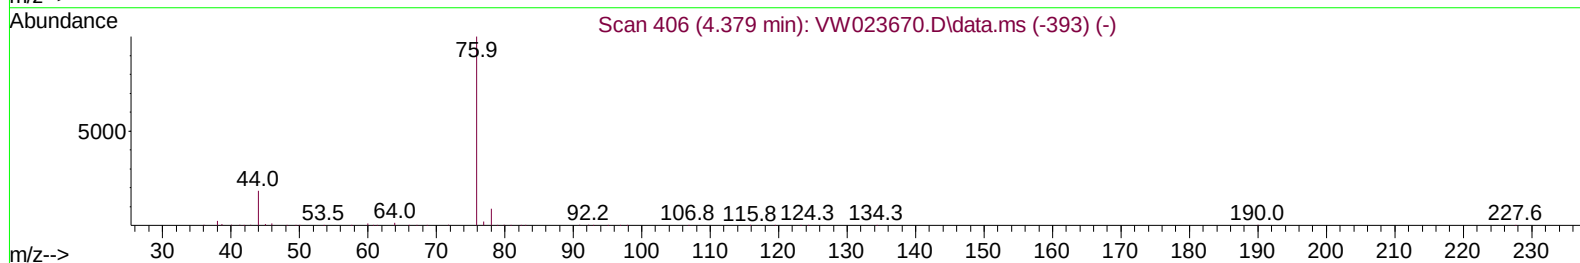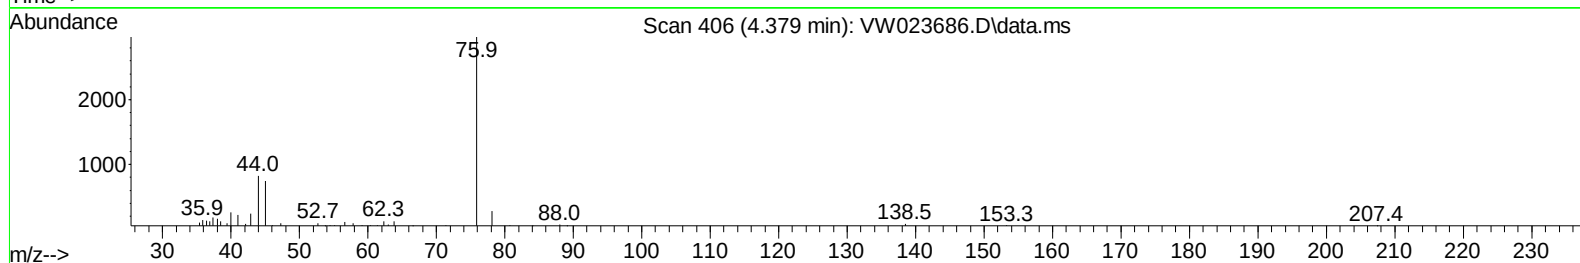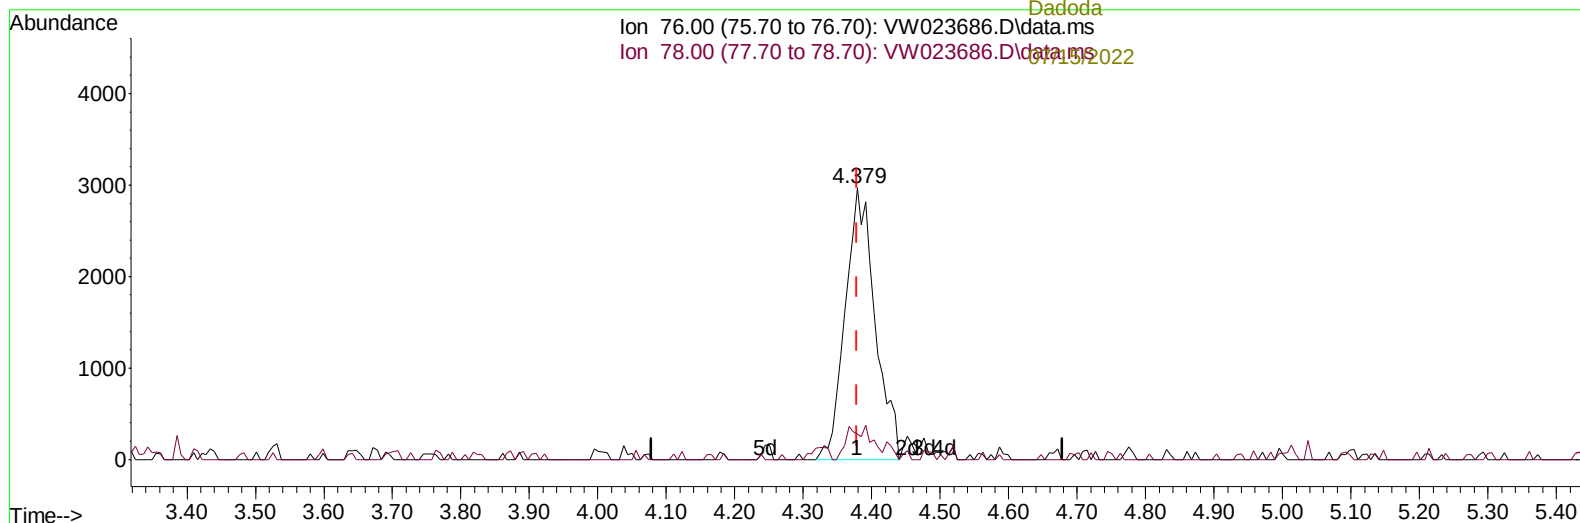

TIC: VW023686.D\data.ms

(14) Carbon disulfide (T)

4.379min (+ 0.000) 1.52 ug/L m

response 8983

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	9.23
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023686.D
 Acq On : 14 Jul 2022 08:23
 Operator : SY/VA
 Sample : N3698-06
 Misc : 5.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B71

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:32:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

07/15/2022
 Supervised By :Mahesh
 Dadoda

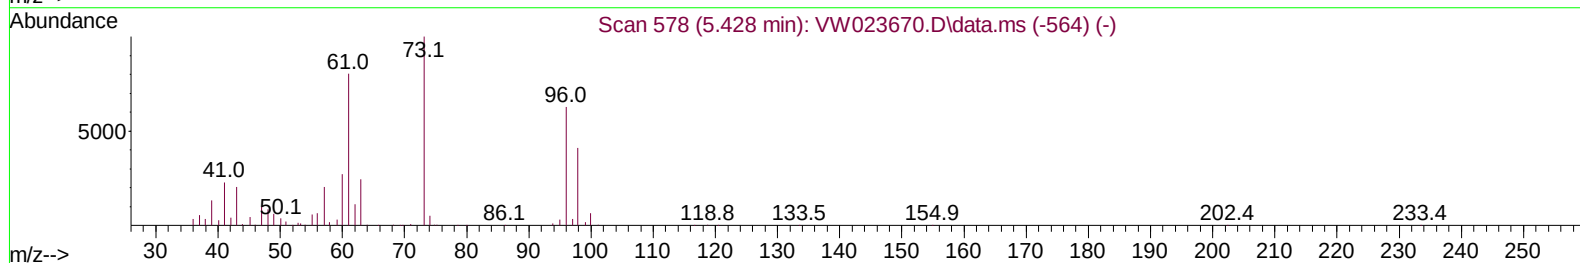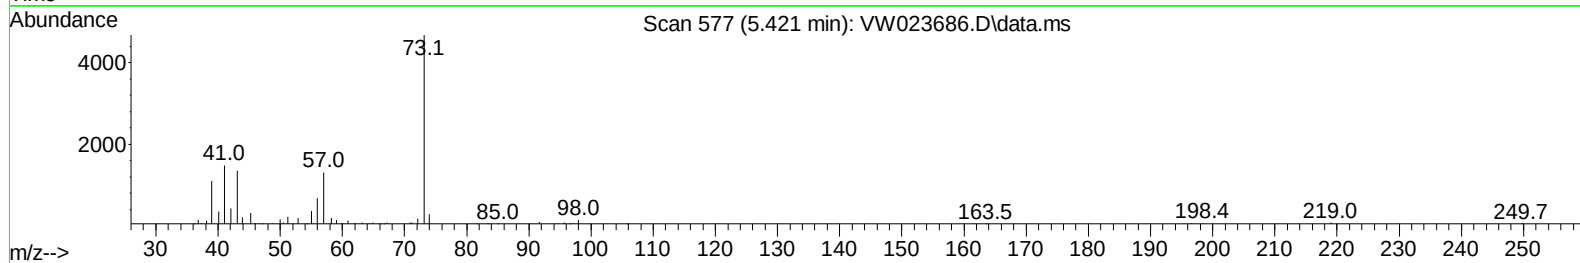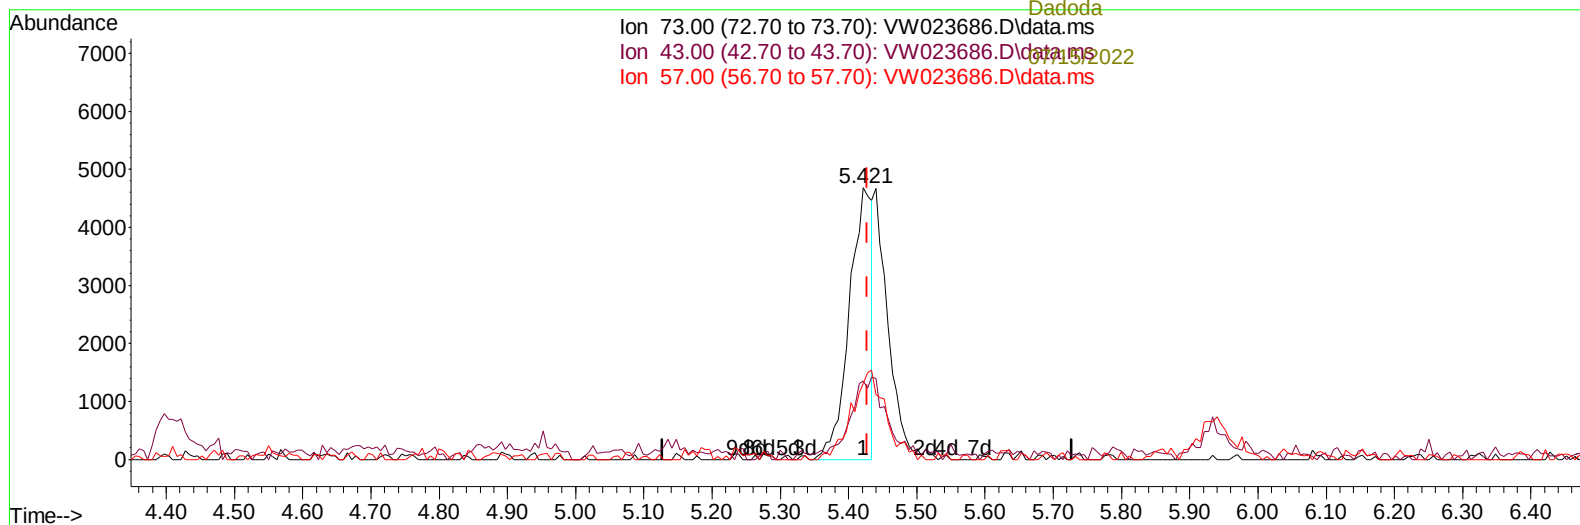

TIC: VW023686.D\data.ms

(18) Methyl tert-butyl Ether (T)

5.421min (-0.006) 2.87 ug/L

response 10834

Ion	Exp%	Act%
73.00	100.00	100.00
43.00	22.00	20.80
57.00	21.00	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023686.D
 Acq On : 14 Jul 2022 08:23
 Operator : SY/VA
 Sample : N3698-06
 Misc : 5.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B71




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

07/15/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Jul 15 01:32:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Ion 73.00 (72.70 to 73.70): VW023686.D\data.ms
 Ion 43.00 (42.70 to 43.70): VW023686.D\data.ms
 Ion 57.00 (56.70 to 57.70): VW023686.D\data.ms

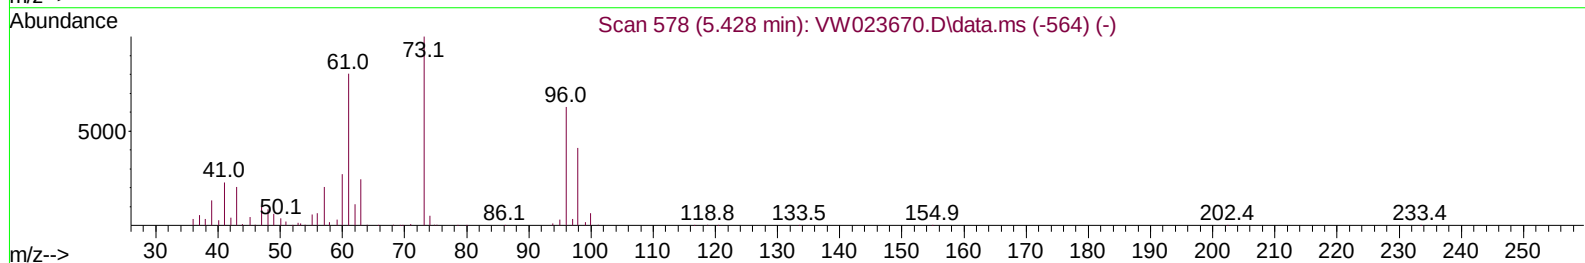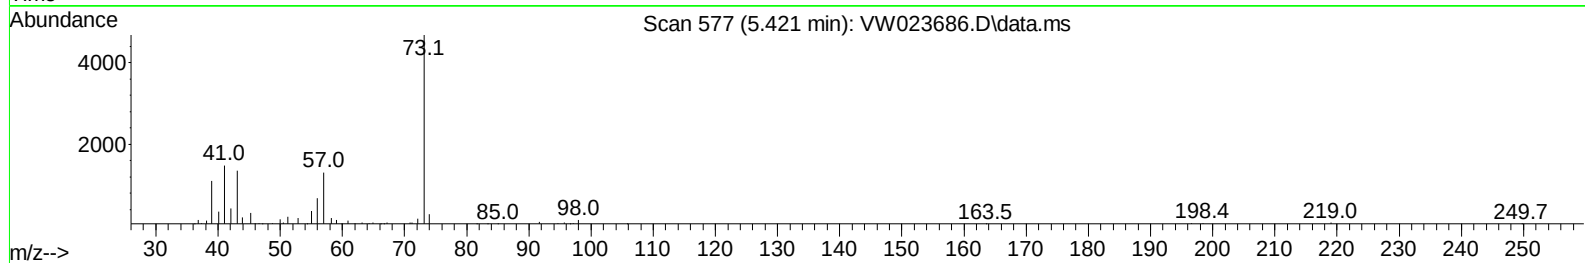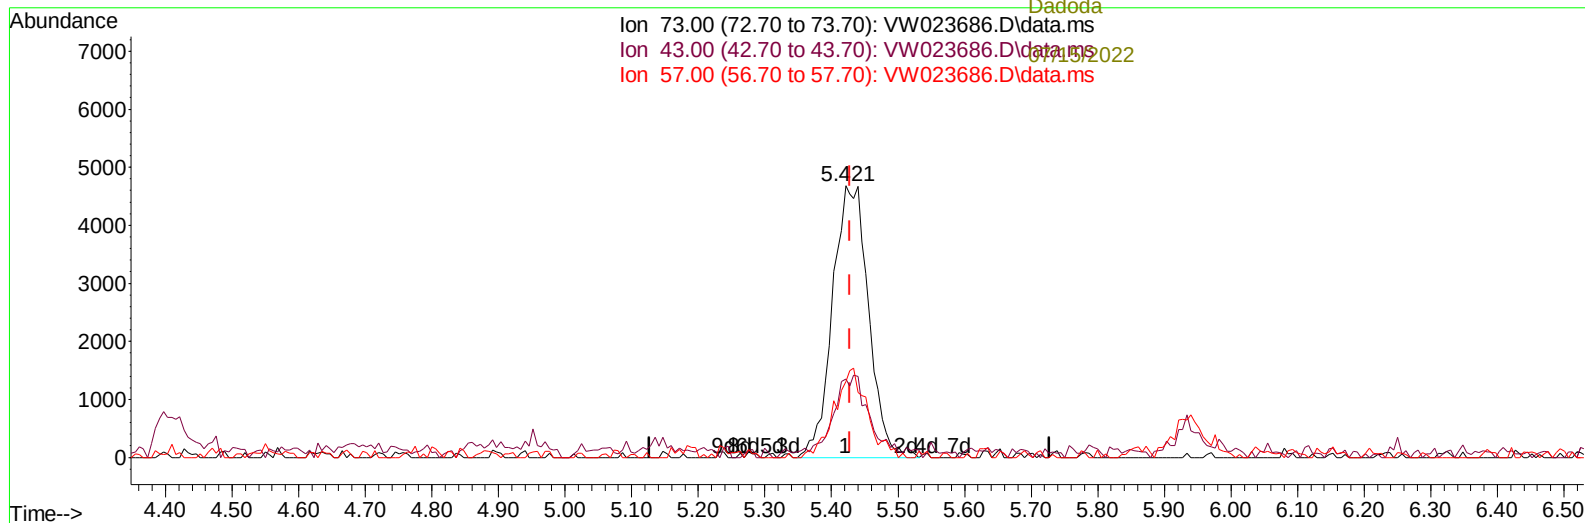

TIC: VW023686.D\data.ms

(18) Methyl tert-butyl Ether (T)

5.421min (-0.006) 4.66 ug/L m

response 17622

Ion	Exp%	Act%
73.00	100.00	100.00
43.00	22.00	12.79#
57.00	21.00	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023686.D
 Acq On : 14 Jul 2022 08:23
 Operator : SY/VA
 Sample : N3698-06
 Misc : 5.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B71

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:32:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

07/15/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----07/15/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	190005	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	176372	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	64615	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	95143	19.605	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.440%	
7) Chloroethane-d5	2.879	69	80428	24.843	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	99.360%	
11) 1,1-Dichloroethene-d2	4.013	63	56814	14.377	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.520%	
21) 2-Butanone-d5	7.080	46	36223	48.122	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.240%	
24) Chloroform-d	7.647	84	129747	23.454	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	8.305	65	80249	23.719	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.880%	
32) Benzene-d6	8.275	84	244827	26.703	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	106.800%	
36) 1,2-Dichloropropane-d6	9.274	67	75610	27.378	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	109.520%	
41) Toluene-d8	10.323	98	213064	22.911	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	91.640%	
43) trans-1,3-Dichloroprop...	10.579	79	20798	16.066	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	64.280%	
47) 2-Hexanone-d5	10.920	63	26557	45.731	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.460%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	64597	21.165	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	84.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	59980	26.003	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	104.000%	
Target Compounds						
13) Acetone	4.123	43	7945	14.929	ug/L	96
14) Carbon disulfide	4.379	76	8983m	1.516	ug/L	
18) Methyl tert-butyl Ether	5.421	73	17622m	4.661	ug/L	
33) Benzene	8.323	78	14884	1.485	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023686.D
Acq On : 14 Jul 2022 08:23
Operator : SY/VA
Sample : N3698-06
Misc : 5.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B71

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:32:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 04:56:40 2022
Response via : Initial Calibration

