

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023651.D
 Acq On : 13 Jul 2022 16:50
 Operator : SY/VA
 Sample : N3678-16
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B37

Quant Time: Jul 14 02:14:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	231680	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	213917	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	93394	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	117188	19.804	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.200%
7) Chloroethane-d5	2.885	69	92901	23.534	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.120%
11) 1,1-Dichloroethene-d2	4.013	63	71004	14.736	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.960%
21) 2-Butanone-d5	7.079	46	39965	43.543	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.080%
24) Chloroform-d	7.646	84	149016	22.092	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.360%
26) 1,2-Dichloroethane-d4	8.305	65	84904	20.580	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.320%
32) Benzene-d6	8.274	84	264624	23.797	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.200%
36) 1,2-Dichloropropane-d6	9.274	67	81604	24.362	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.440%
41) Toluene-d8	10.323	98	251286	22.278	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.120%
43) trans-1,3-Dichloroprop...	10.579	79	32146	20.474	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.880%
47) 2-Hexanone-d5	10.926	63	31180	44.268	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.540%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	77108	20.830	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	82957	24.882	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.520%
Target Compounds					Qvalue	
13) Acetone	4.135	43	7423	11.439	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023651.D
Acq On : 13 Jul 2022 16:50
Operator : SY/VA
Sample : N3678-16
Misc : 6.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B37

Quant Time: Jul 14 02:14:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

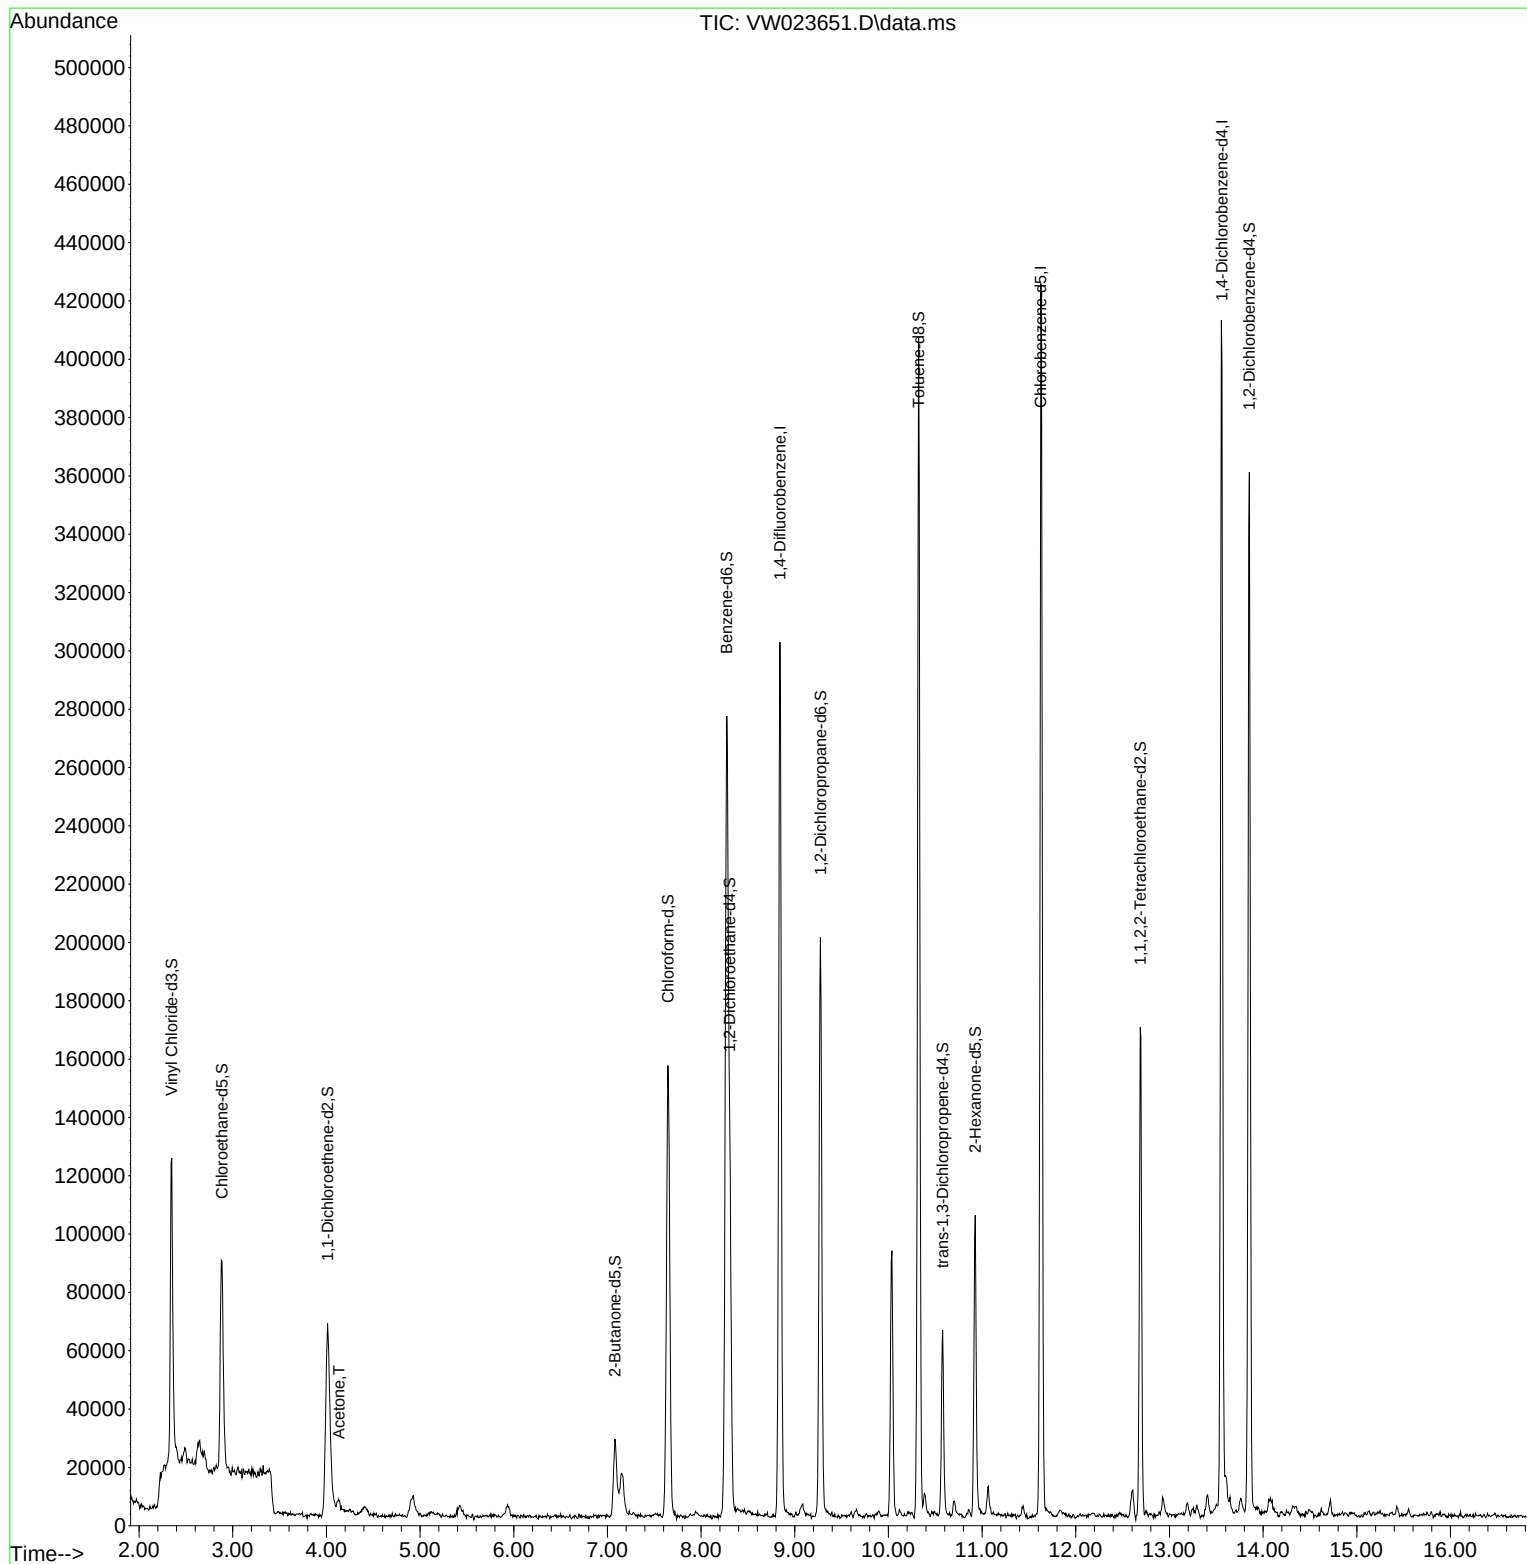

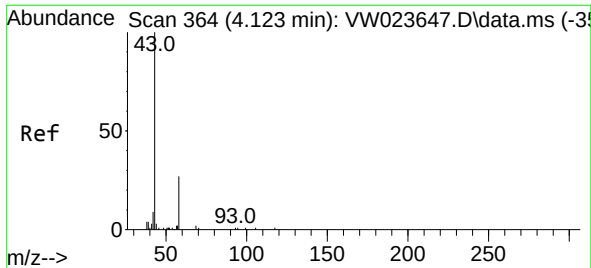

#13
 Acetone
 Concen: 11.439 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023651.D
 Acq: 13 Jul 2022 16:50

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B37

Tgt Ion: 43 Resp: 7423
 Ion Ratio Lower Upper
 43 100
 58 25.7 0.0 64.2

