

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023656.D
 Acq On : 13 Jul 2022 18:53
 Operator : SY/VA
 Sample : N3676-08RE
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B07RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 02:14:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	76026	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	66035	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	22234	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	47441	24.432	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.720%		
7) Chloroethane-d5	2.873	69	25586	19.752	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.000%		
11) 1,1-Dichloroethene-d2	4.007	63	29749	18.814	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	75.240%		
21) 2-Butanone-d5	7.086	46	23645m	78.506	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	157.020%#		
24) Chloroform-d	7.647	84	54822	24.767	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.080%		
26) 1,2-Dichloroethane-d4	8.305	65	34645m	25.591	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	102.360%		
32) Benzene-d6	8.275	84	94285	27.467	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	109.880%		
36) 1,2-Dichloropropane-d6	9.275	67	30597	29.591	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	118.360%		
41) Toluene-d8	10.323	98	75795	21.768	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	87.080%		
43) trans-1,3-Dichloroprop...	10.579	79	8377	17.284	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	69.120%		
47) 2-Hexanone-d5	10.927	63	14433	66.381	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	132.760%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	33830	29.606	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	118.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	21616	27.234	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	108.920%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	27309	128.245	ug/L	98
14) Carbon disulfide	4.373	76	9893	4.173	ug/L	98
20) cis-1,2-Dichloroethene	7.165	96	4815	4.445	ug/L #	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023656.D
Acq On : 13 Jul 2022 18:53
Operator : SY/VA
Sample : N3676-08RE
Misc : 6.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5B07RE

Quant Time: Jul 14 02:14:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 07/14/2022
Supervised By : Mahesh Dadoda 07/15/2022

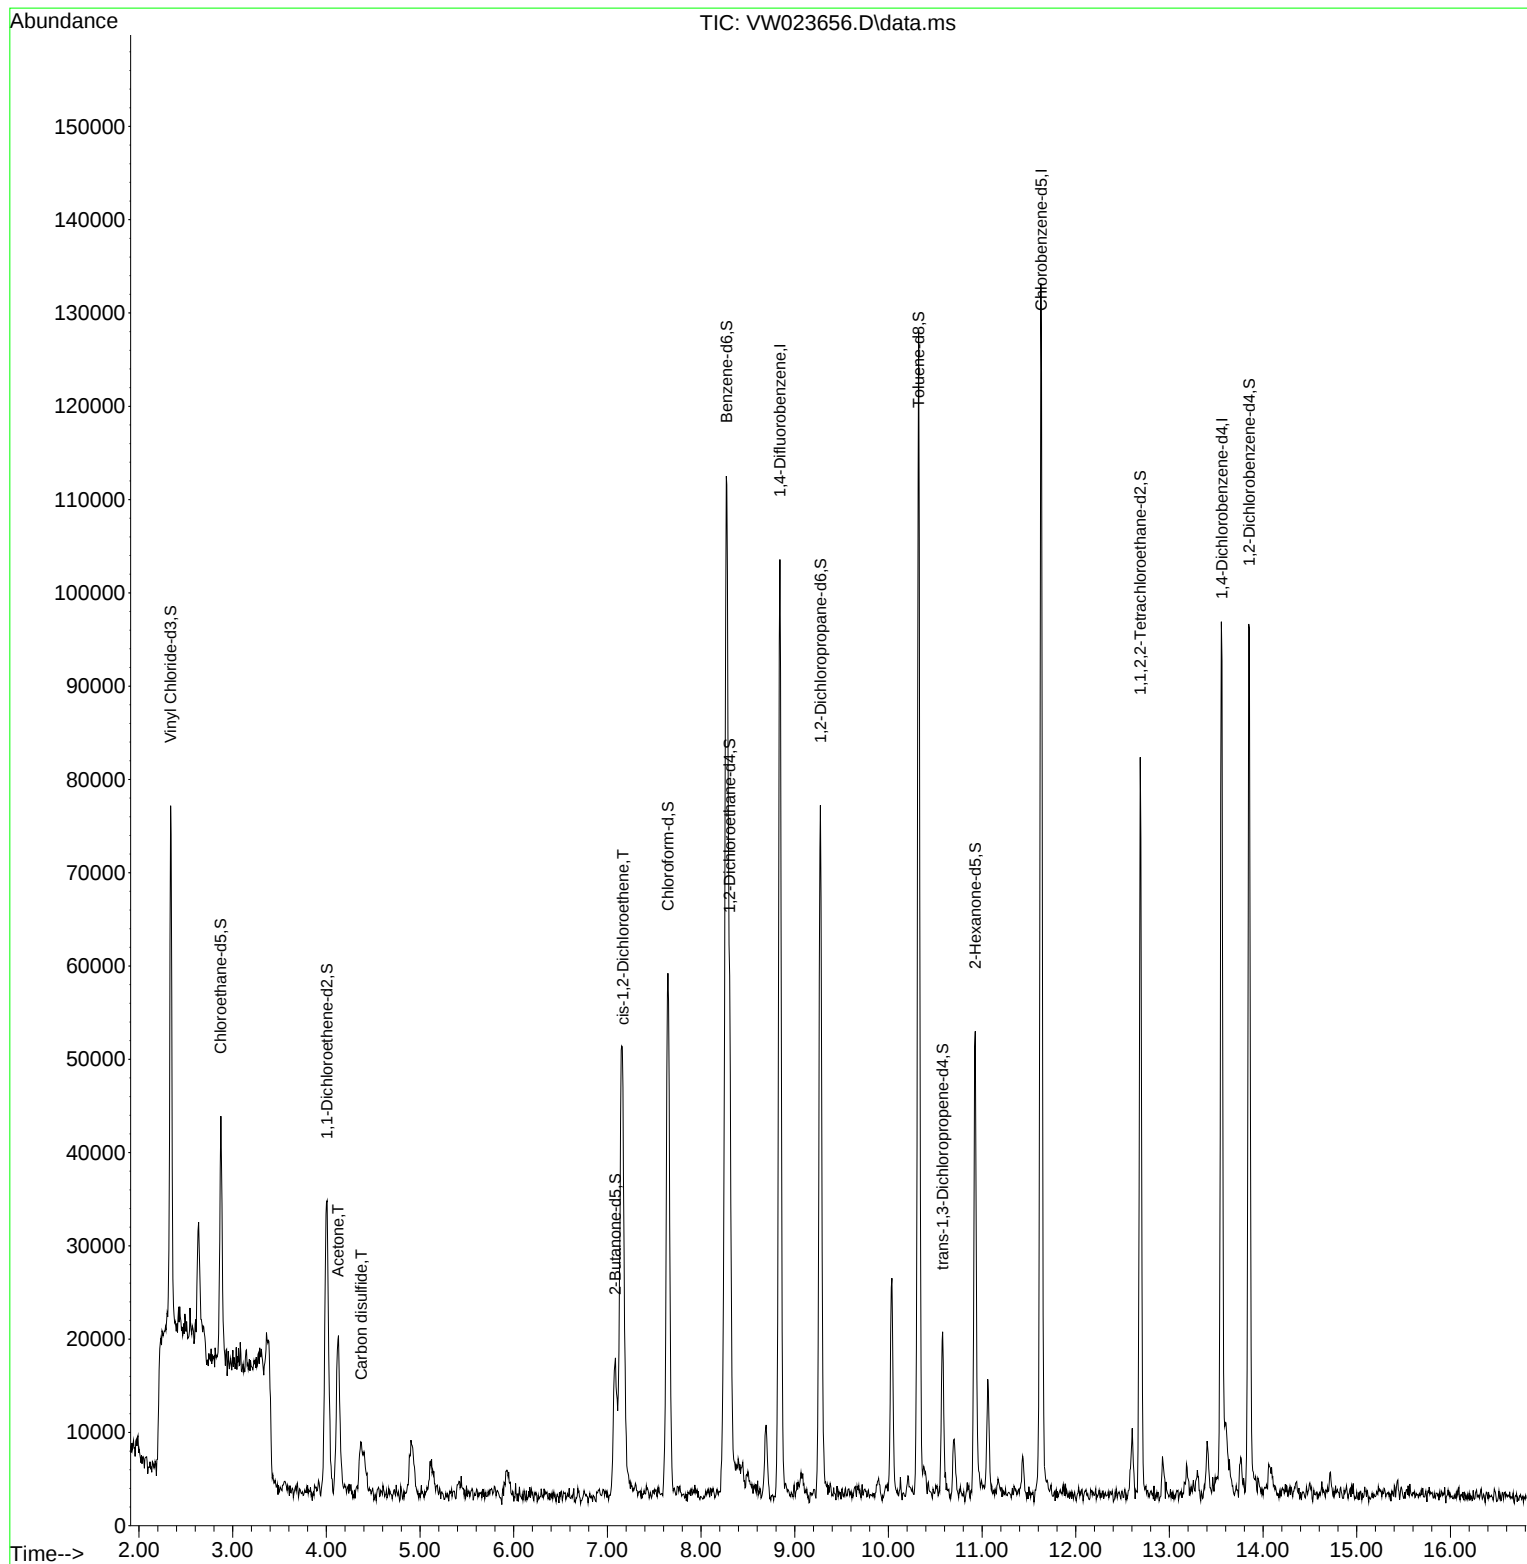

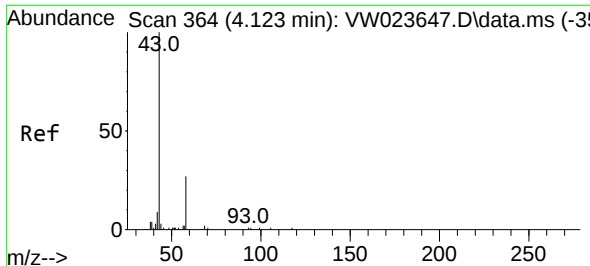

#13
Acetone
Concen: 128.245 ug/L
RT: 4.123 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW023656.D
Acq: 13 Jul 2022 18:53




Instrument :
MSVOA_W
ClientSampleId :
F5B07RE

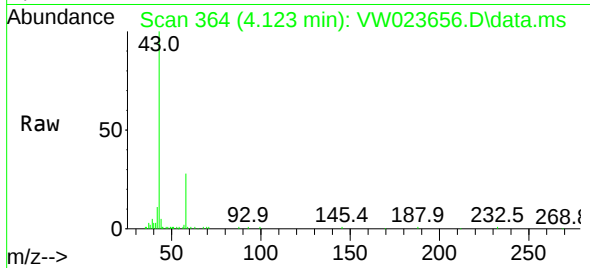


Tgt Ion: 43 Resp: 27309
Ion Ratio Lower Upper
43 100
58 31.1 0.0 64.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

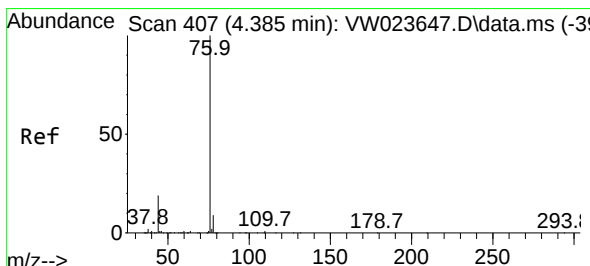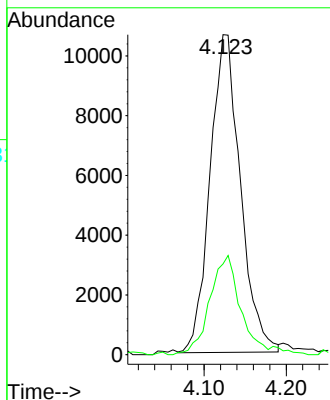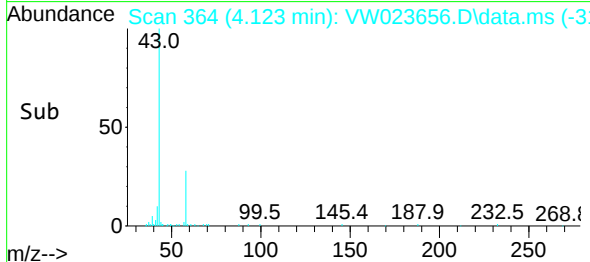


#14
Carbon disulfide
Concen: 4.173 ug/L
RT: 4.373 min Scan# 405
Delta R.T. -0.012 min
Lab File: VW023656.D
Acq: 13 Jul 2022 18:53

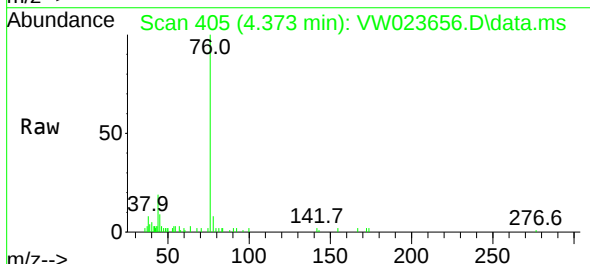


Tgt Ion: 76 Resp: 9893
Ion Ratio Lower Upper
76 100
78 8.3 7.2 10.8

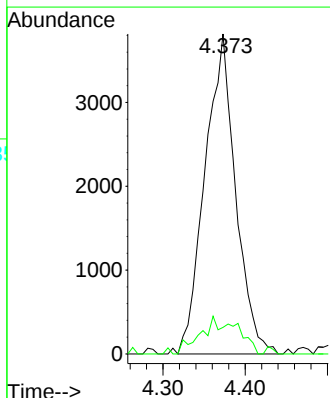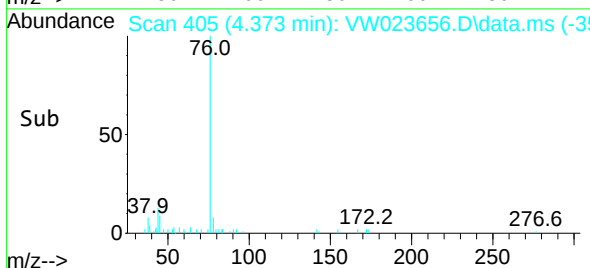

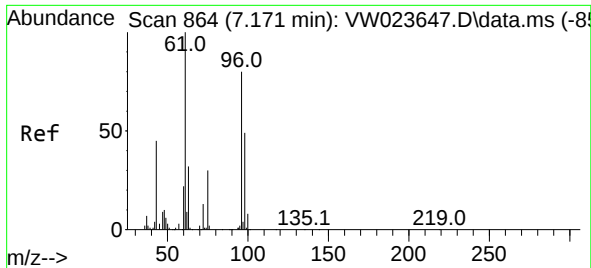

#20
 cis-1,2-Dichloroethene
 Concen: 4.445 ug/L
 RT: 7.165 min Scan# 80
 Delta R.T. -0.006 min
 Lab File: VW023656.D
 Acq: 13 Jul 2022 18:53

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B07RE

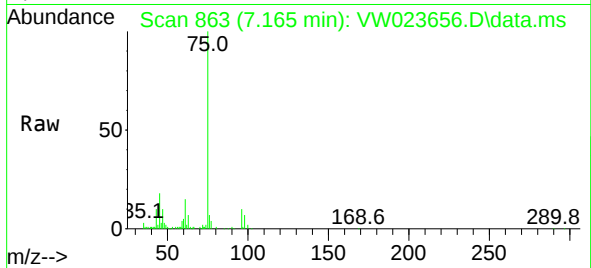

Tgt Ion: 96 Resp: 481
 Ion Ratio Lower Upper
 96 100
 61 149.5 90.6 168.2
 68 0.0 0.2 0.4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

