

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023664.D
 Acq On : 13 Jul 2022 22:11
 Operator : SY/VA
 Sample : N3678-15RE
 Misc : 5.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B36RE

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/14/2022
 Supervised By : Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 02:16:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 02:04:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	94052	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	88030	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	32583	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	49431	20.578	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.320%		
7) Chloroethane-d5	2.879	69	25723	16.051	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.200%		
11) 1,1-Dichloroethene-d2	4.007	63	27416	14.016	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.080%		
21) 2-Butanone-d5	7.080	46	19352	51.938	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	103.880%		
24) Chloroform-d	7.647	84	58465	21.351	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.400%		
26) 1,2-Dichloroethane-d4	8.305	65	35460m	21.173	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.680%		
32) Benzene-d6	8.274	84	97908	21.396	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.600%		
36) 1,2-Dichloropropane-d6	9.274	67	32720	23.738	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.960%		
41) Toluene-d8	10.323	98	85889	18.504	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	74.000%		
43) trans-1,3-Dichloroprop...	10.579	79	11181	17.305	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	69.240%		
47) 2-Hexanone-d5	10.920	63	12417	42.839	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	85.680%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	32699	21.466	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.880%		
66) 1,2-Dichlorobenzene-d4	13.853	152	26377	22.677	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.720%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	7983m	30.304	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023664.D
Acq On : 13 Jul 2022 22:11
Operator : SY/VA
Sample : N3678-15RE
Misc : 5.95g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5B36RE

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 07/14/2022
Supervised By : Mahesh Dadoda 07/15/2022


Quant Time: Jul 14 02:16:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 02:04:07 2022
Response via : Initial Calibration

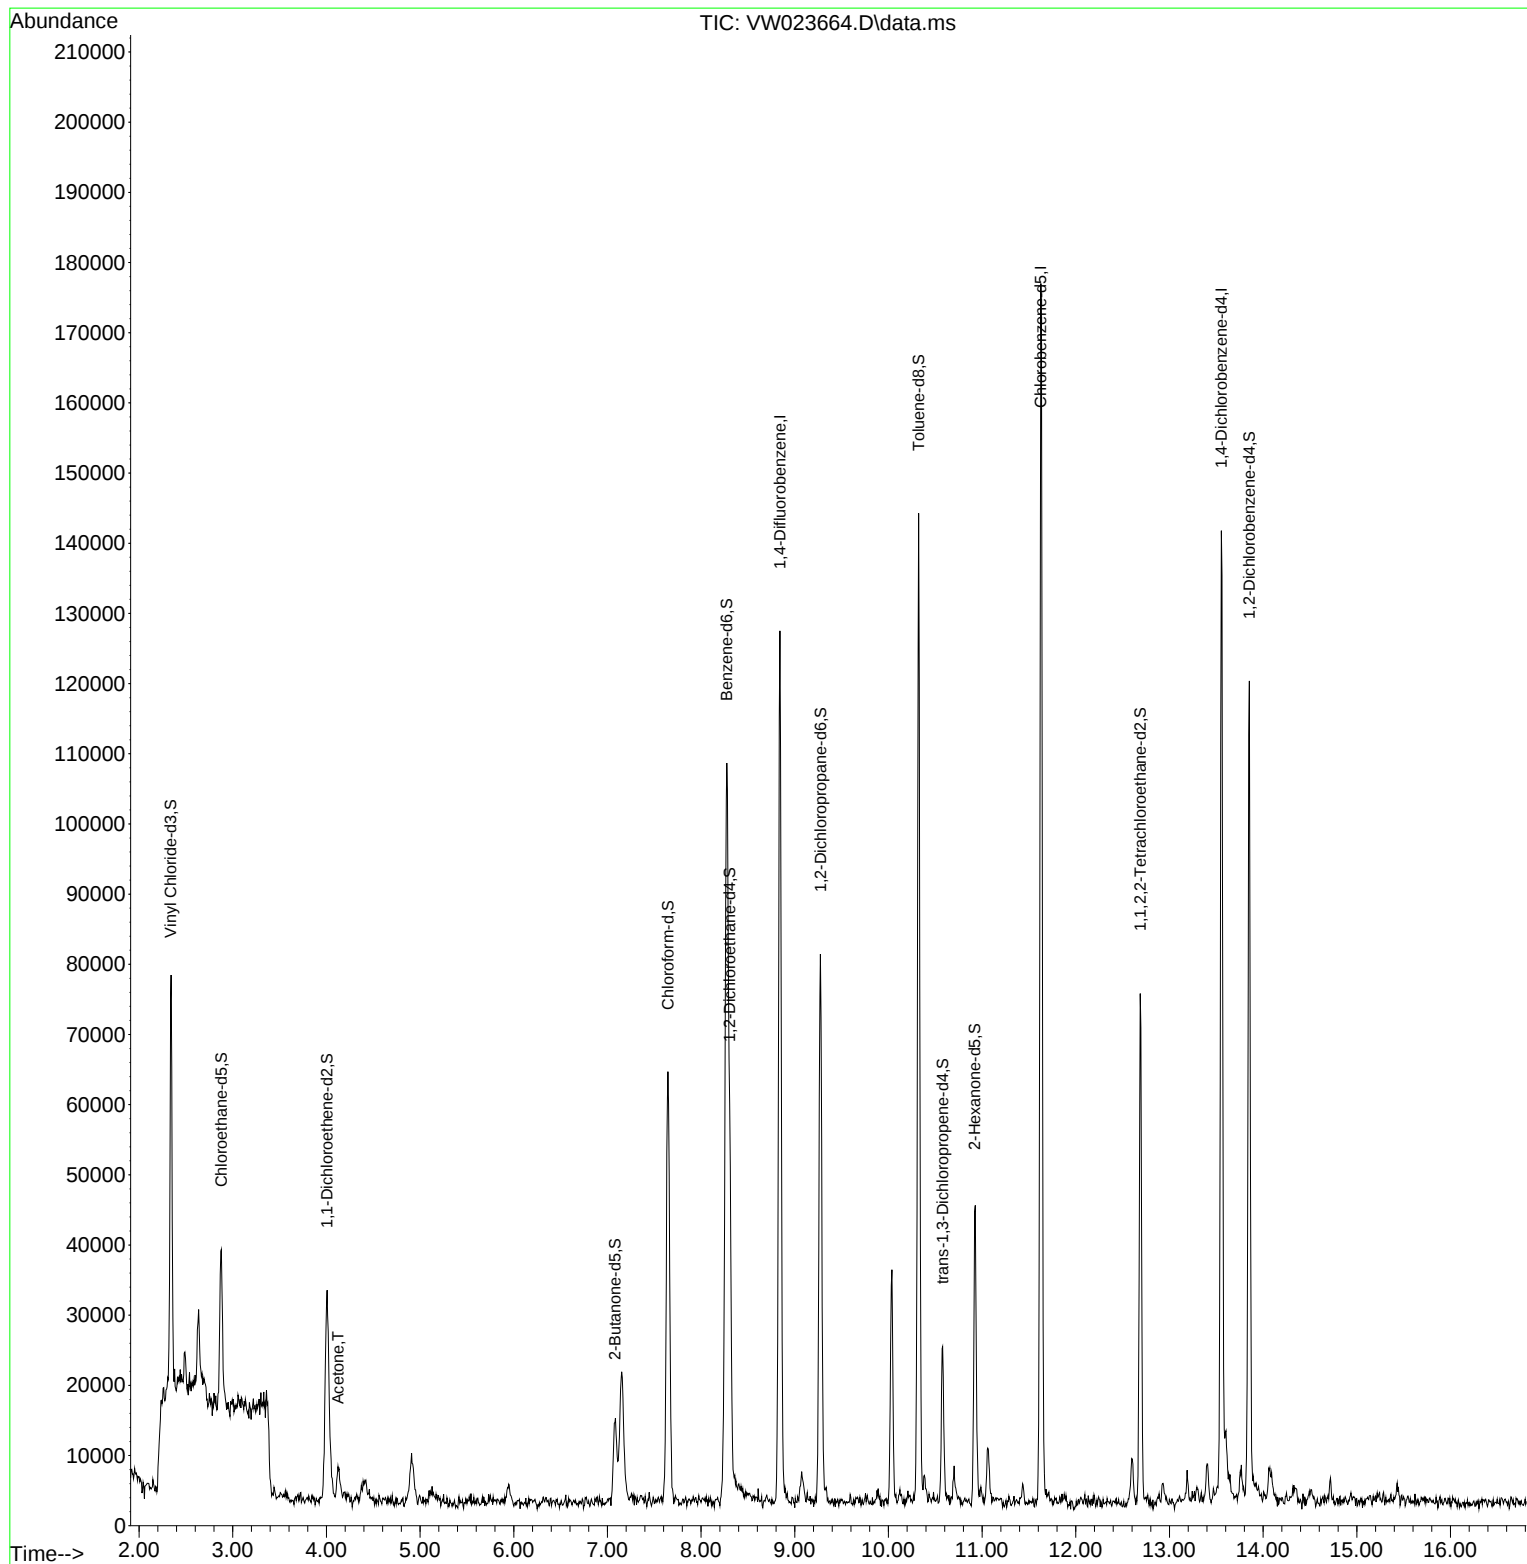

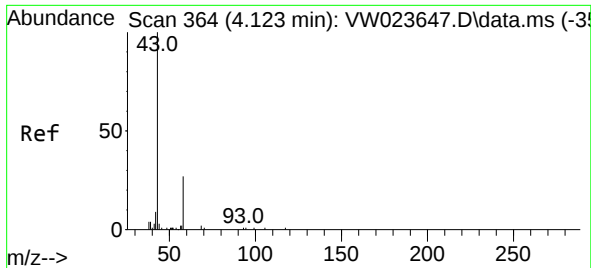

#13
Acetone
Concen: 30.304 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW023664.D
Acq: 13 Jul 2022 22:11

Instrument :
MSVOA_W
ClientSampleId :
F5B36RE

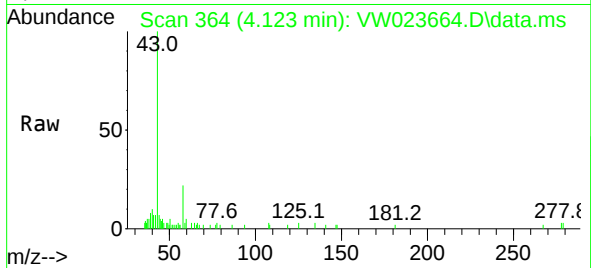

Tgt Ion: 43 Resp: 798
Ion Ratio Lower Upper
43 100
58 26.8 0.0 64.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

