

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023682.D
 Acq On : 14 Jul 2022 06:45
 Operator : SY/VA
 Sample : N3698-02
 Misc : 5.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B67

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/14/2022
 Supervised By : Mahesh Dadoda 07/15/2022

Quant Time: Jul 14 07:58:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	195805	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	168989	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	67092	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	87370	17.470	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.880%		
7) Chloroethane-d5	2.879	69	62362	18.692	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.760%		
11) 1,1-Dichloroethene-d2	4.013	63	52259	12.833	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	51.320%		
21) 2-Butanone-d5	7.074	46	46205	59.565	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	119.120%		
24) Chloroform-d	7.647	84	116892	20.504	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.000%		
26) 1,2-Dichloroethane-d4	8.305	65	76607	21.971	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.880%		
32) Benzene-d6	8.275	84	232370	26.452	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	105.800%		
36) 1,2-Dichloropropane-d6	9.275	67	72029	27.221	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	108.880%		
41) Toluene-d8	10.323	98	205321	23.043	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	92.160%		
43) trans-1,3-Dichloroprop...	10.579	79	24055	19.394	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.560%		
47) 2-Hexanone-d5	10.921	63	32609	58.605	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	117.220%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	72493	24.790	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	99.160%		
66) 1,2-Dichlorobenzene-d4	13.853	152	59340	24.776	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.120%		
Target Compounds						Qvalue
5) Vinyl chloride	2.355	62	88359	15.791	ug/L	98
13) Acetone	4.123	43	16043	29.252	ug/L	70
17) trans-1,2-Dichloroethene	5.422	96	4367m	1.734	ug/L	
20) cis-1,2-Dichloroethene	7.165	96	96413	34.557	ug/L	97
29) Cyclohexane	7.952	56	23103	7.475	ug/L	88
33) Benzene	8.323	78	30857	3.213	ug/L	100
35) Methylcyclohexane	9.335	83	34353	8.896	ug/L #	82
42) Toluene	10.384	91	11102	1.014	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023682.D
Acq On : 14 Jul 2022 06:45
Operator : SY/VA
Sample : N3698-02
Misc : 5.81g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5B67

Quant Time: Jul 14 07:58:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 04:56:40 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 07/14/2022
Supervised By : Mahesh Dadoda 07/15/2022

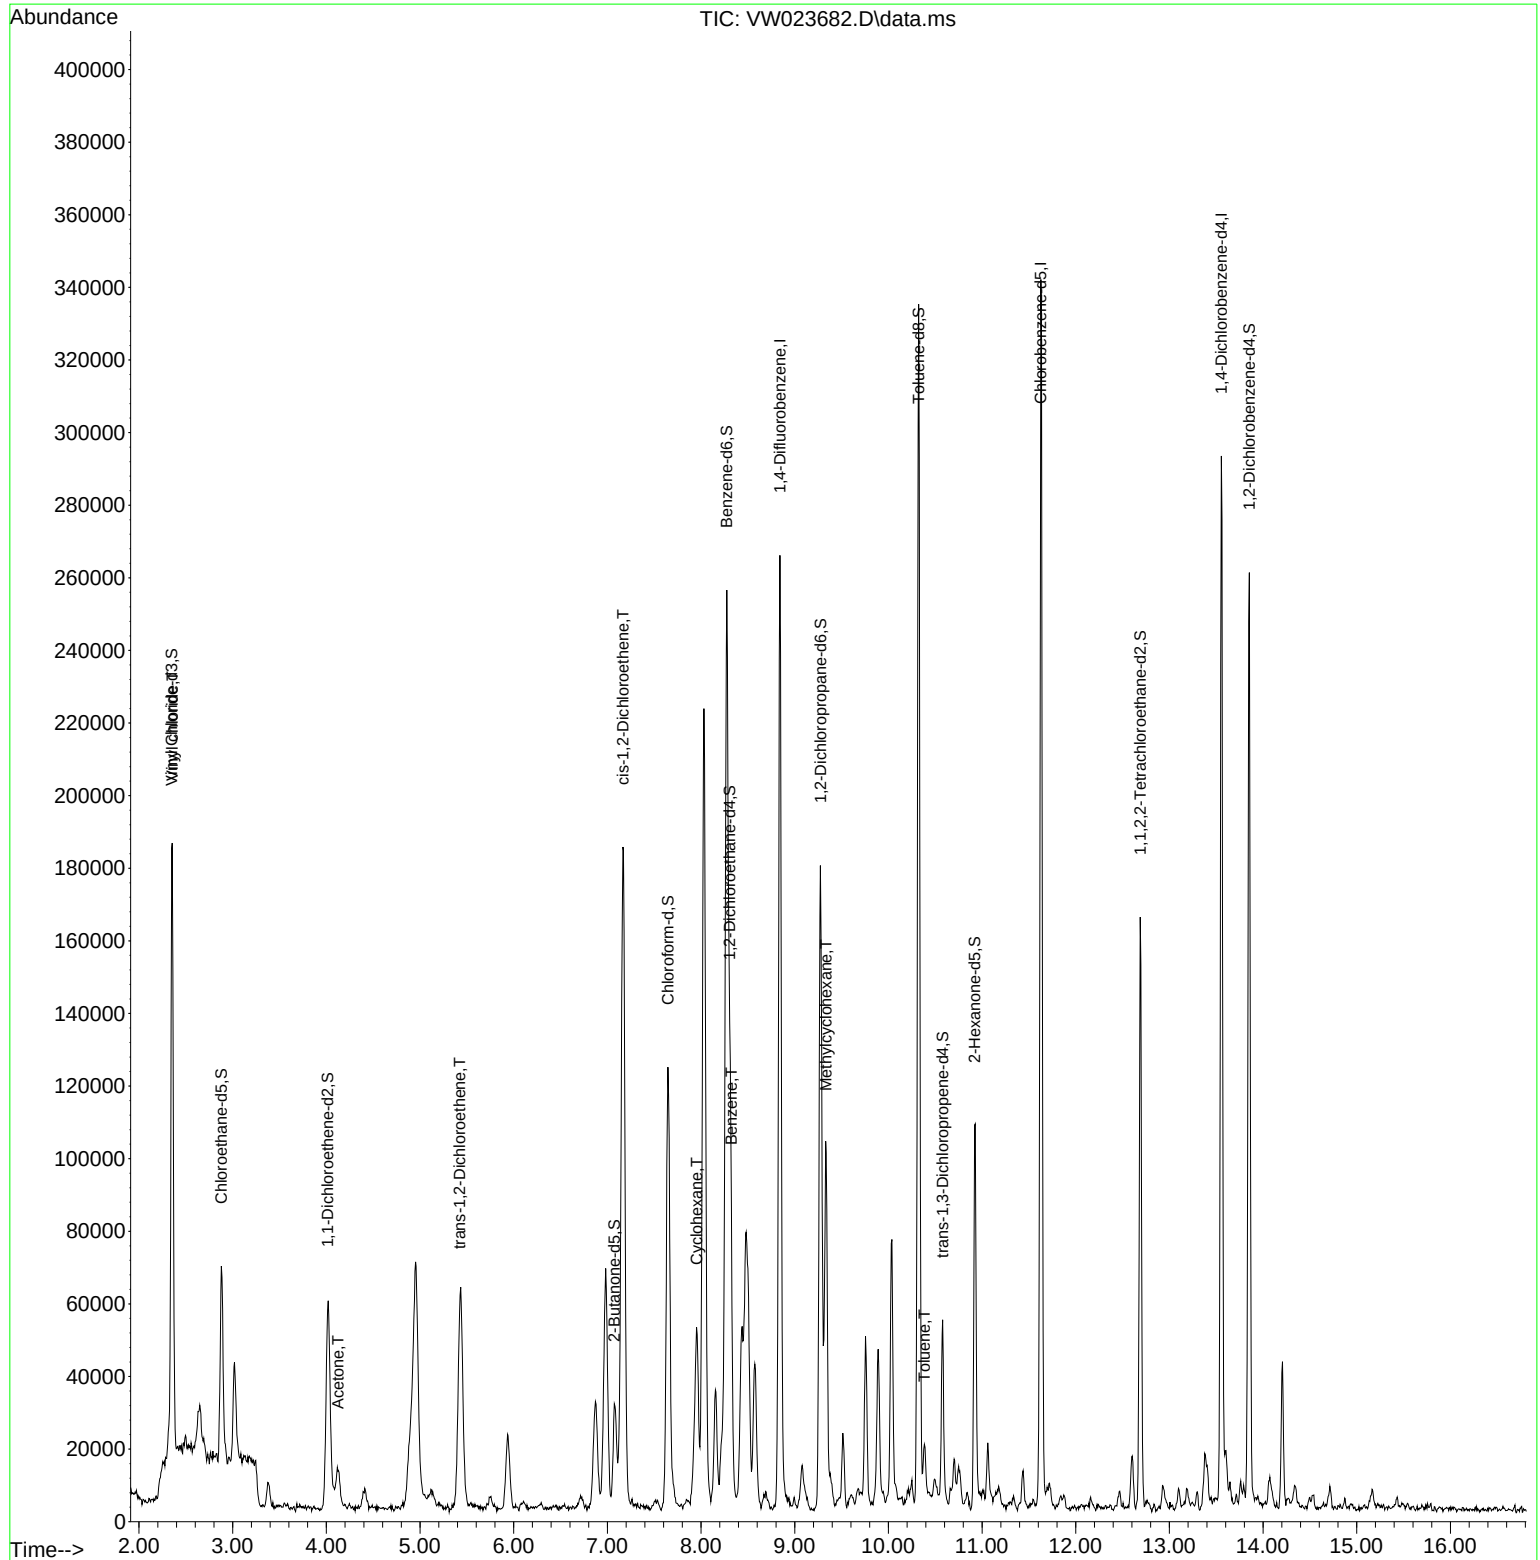

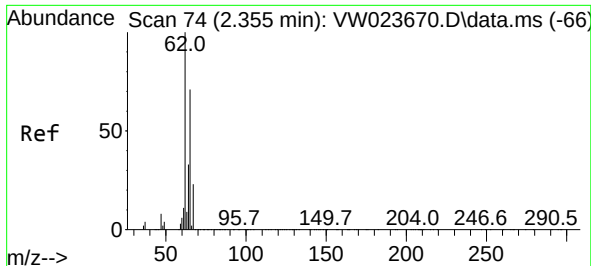

#5
 Vinyl chloride
 Concen: 15.791 ug/L
 RT: 2.355 min Scan# 74
 Delta R.T. 0.000 min
 Lab File: VW023682.D
 Acq: 14 Jul 2022 06:45




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B67

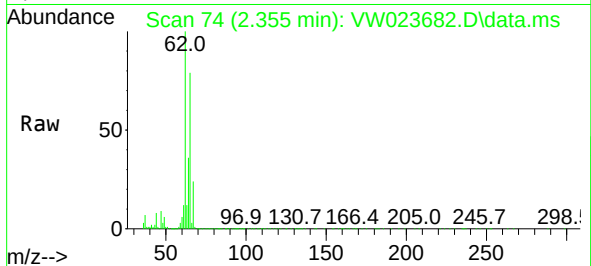

Tgt Ion: 62 Resp: 88359
 Ion Ratio Lower Upper
 62 100
 64 35.6 24.0 44.6




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 07/14/2022
 Supervised By :Mahesh Dadoda 07/15/2022

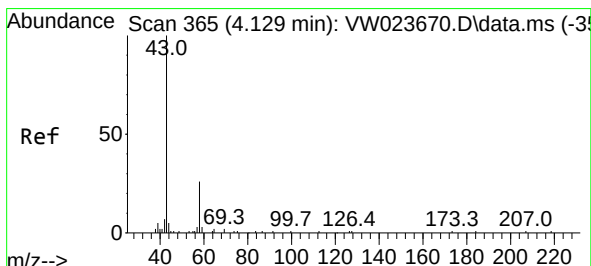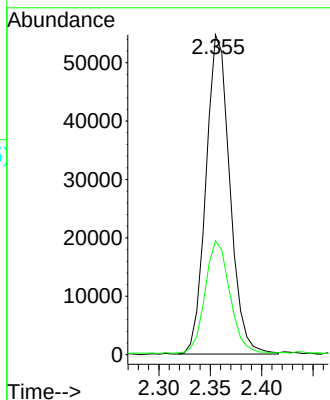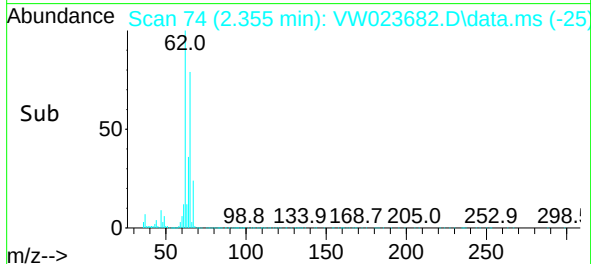

#13
 Acetone
 Concen: 29.252 ug/L
 RT: 4.123 min Scan# 364
 Delta R.T. -0.006 min
 Lab File: VW023682.D
 Acq: 14 Jul 2022 06:45


Tgt Ion: 43 Resp: 16043
 Ion Ratio Lower Upper
 43 100
 58 15.6 0.0 64.2

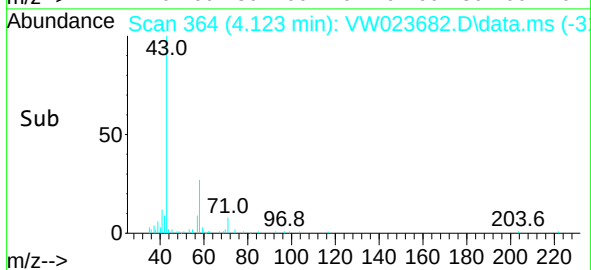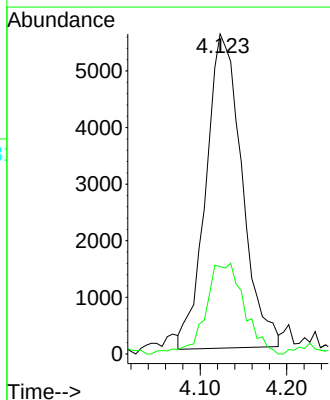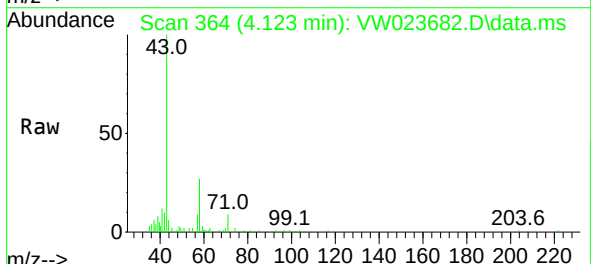

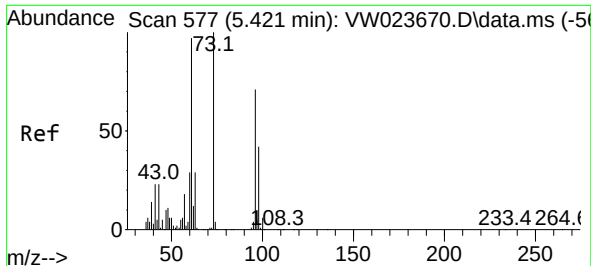

#17
trans-1,2-Dichloroethene
Concen: 1.734 ug/L m
RT: 5.422 min Scan# 51
Delta R.T. 0.000 min
Lab File: VW023682.D
Acq: 14 Jul 2022 06:45




Instrument :
MSVOA_W
ClientSampleId :
F5B67

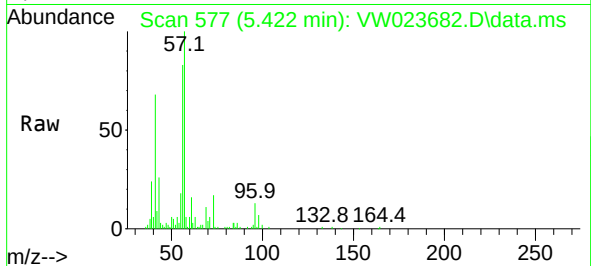

Tgt Ion: 96 Resp: 436
Ion Ratio Lower Upper
96 100
61 125.7 90.8 168.6
98 57.2 42.8 79.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

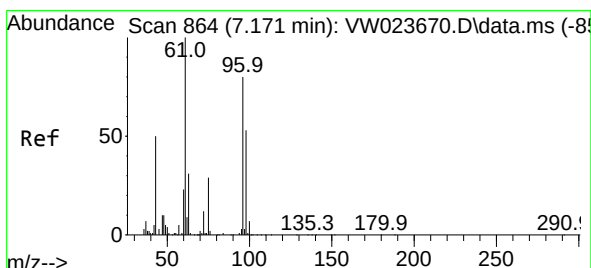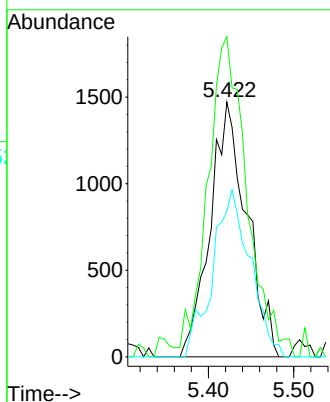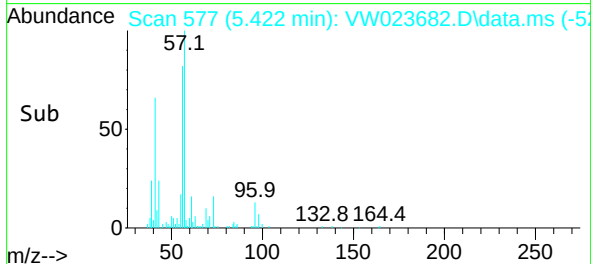

#20
cis-1,2-Dichloroethene
Concen: 34.557 ug/L
RT: 7.165 min Scan# 863
Delta R.T. -0.006 min
Lab File: VW023682.D
Acq: 14 Jul 2022 06:45


Tgt Ion: 96 Resp: 96413
Ion Ratio Lower Upper
96 100
61 126.1 90.6 168.2
68 0.2 0.2 0.4

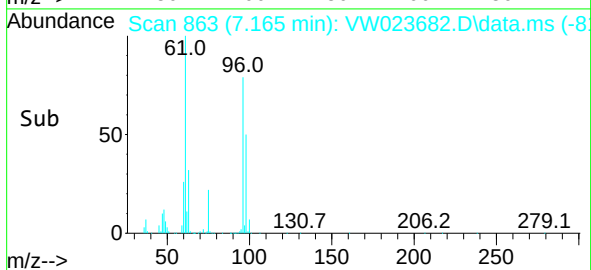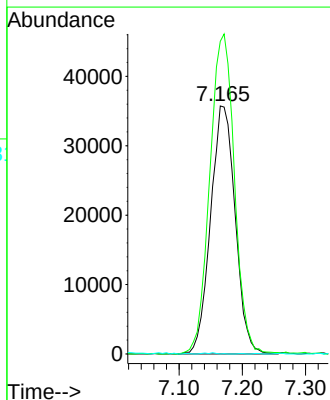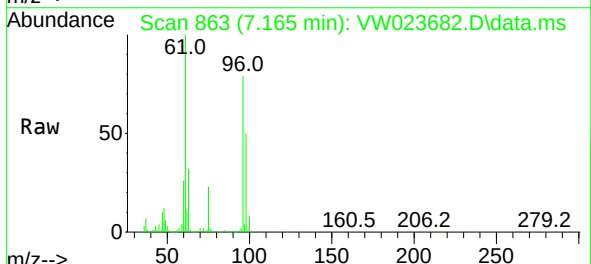

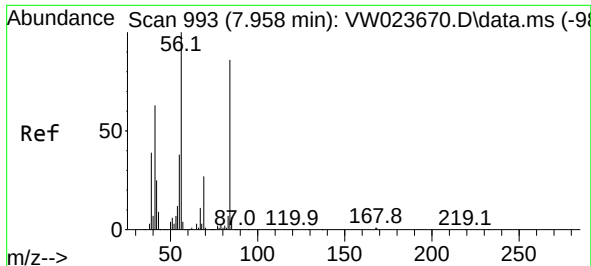

#29
Cyclohexane
Concen: 7.475 ug/L
RT: 7.952 min Scan# 993
Delta R.T. -0.006 min
Lab File: VW023682.D
Acq: 14 Jul 2022 06:45




Instrument :
MSVOA_W
ClientSampleId :
F5B67

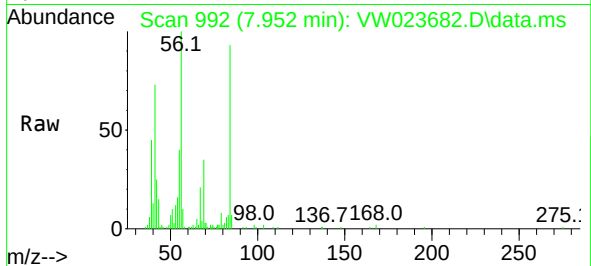

Tgt Ion: 56 Resp: 2310
Ion Ratio Lower Upper
56 100
69 38.0 25.4 38.0
84 82.0 75.0 112.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

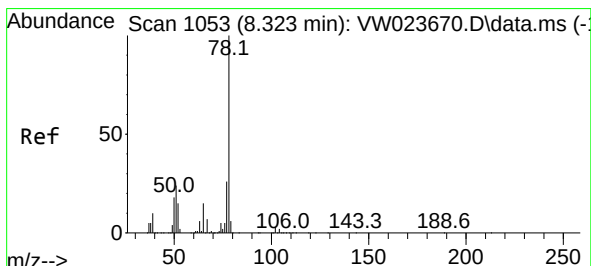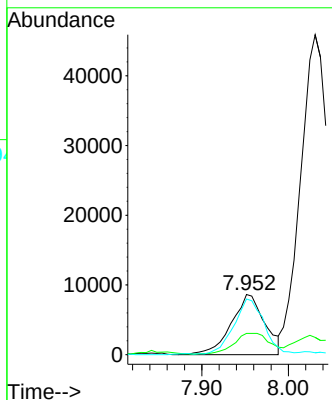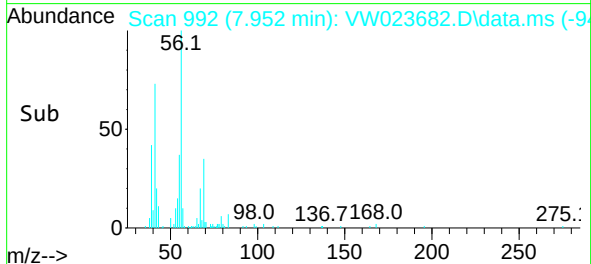

#33
Benzene
Concen: 3.213 ug/L
RT: 8.323 min Scan# 1053
Delta R.T. 0.000 min
Lab File: VW023682.D
Acq: 14 Jul 2022 06:45


Tgt Ion: 78 Resp: 30857

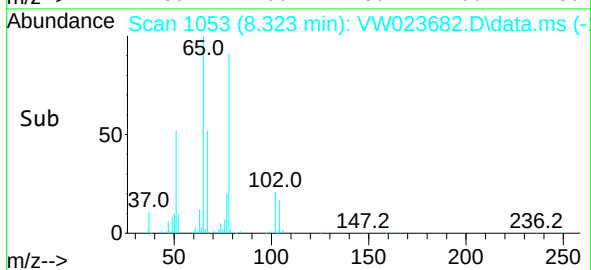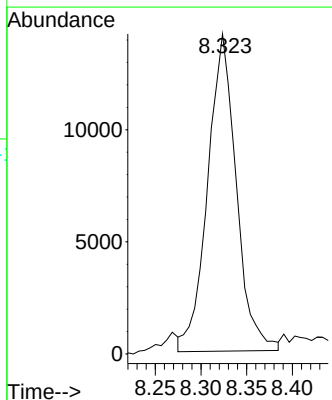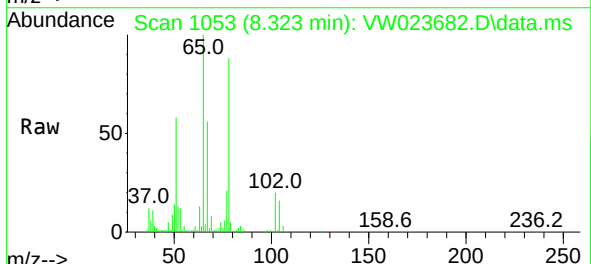

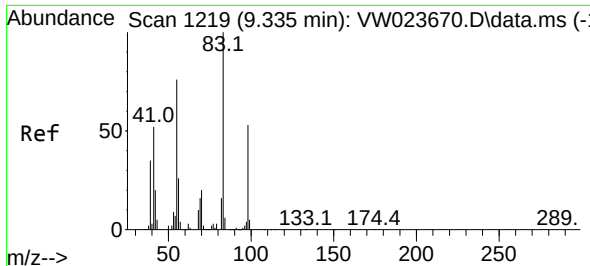

#35
Methylcyclohexane
Concen: 8.896 ug/L
RT: 9.335 min Scan# 1219
Delta R.T. 0.000 min
Lab File: VW023682.D
Acq: 14 Jul 2022 06:45




Instrument :
MSVOA_W
ClientSampleId :
F5B67

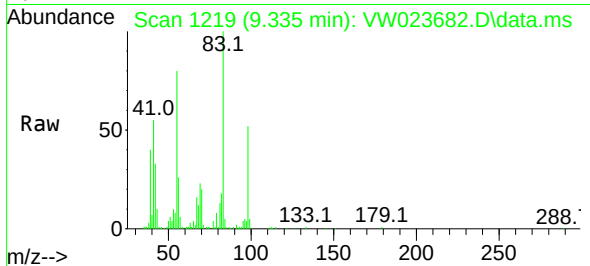


Tgt Ion: 83 Resp: 3435
Ion Ratio Lower Upper
83 100
55 98.4 60.8 91.2
98 52.8 39.5 59.3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/14/2022
Supervised By :Mahesh Dadoda 07/15/2022

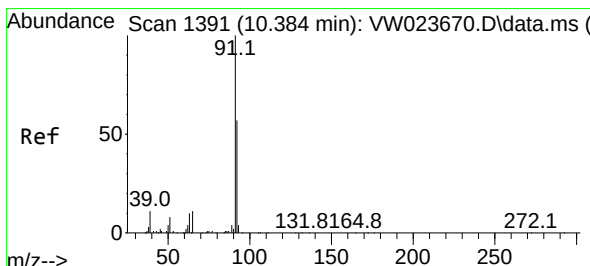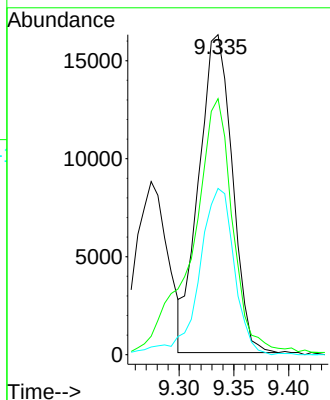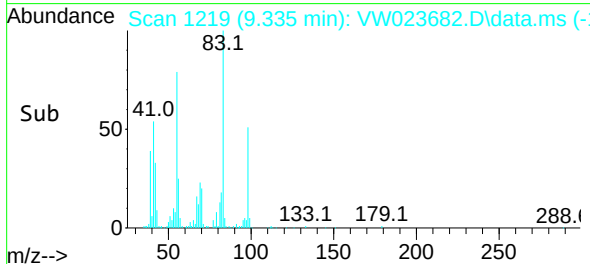

#42
Toluene
Concen: 1.014 ug/L
RT: 10.384 min Scan# 1391
Delta R.T. 0.000 min
Lab File: VW023682.D
Acq: 14 Jul 2022 06:45

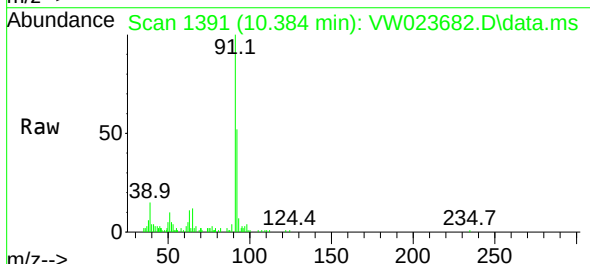

Tgt Ion: 91 Resp: 11102
Ion Ratio Lower Upper
91 100
92 52.4 39.9 74.1

