

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
 Data File : VW023693.D
 Acq On : 14 Jul 2022 11:14
 Operator : SY/VA
 Sample : N3678-19RE
 Misc : 6.74g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B40RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 01:33:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 14 04:56:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	47456	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	43332	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	16834	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	29635	24.450	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.800%
7) Chloroethane-d5	2.879	69	23270	28.778	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.120%
11) 1,1-Dichloroethene-d2	4.007	63	19063	19.314	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.240%
21) 2-Butanone-d5	7.080	46	10275m	54.653	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.300%
24) Chloroform-d	7.647	84	33907	24.541	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.160%
26) 1,2-Dichloroethane-d4	8.305	65	20777m	24.587	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.360%
32) Benzene-d6	8.275	84	57529	25.540	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.160%
36) 1,2-Dichloropropane-d6	9.274	67	18860	27.796	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.200%
41) Toluene-d8	10.323	98	46964	20.555	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	10.579	79	6831	21.478	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.920%
47) 2-Hexanone-d5	10.920	63	5787	40.560	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.120%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	17885	23.852	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	14955	24.886	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.560%
Target Compounds						Qvalue
5) Vinyl chloride	2.349	62	51284	37.816	ug/L	99
13) Acetone	4.123	43	4533m	34.103	ug/L	
17) trans-1,2-Dichloroethene	5.434	96	1399m	2.292	ug/L	
20) cis-1,2-Dichloroethene	7.171	96	8837m	13.069	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071322\
Data File : VW023693.D
Acq On : 14 Jul 2022 11:14
Operator : SY/VA
Sample : N3678-19RE
Misc : 6.74g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5B40RE

Quant Time: Jul 15 01:33:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 14 04:56:40 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022

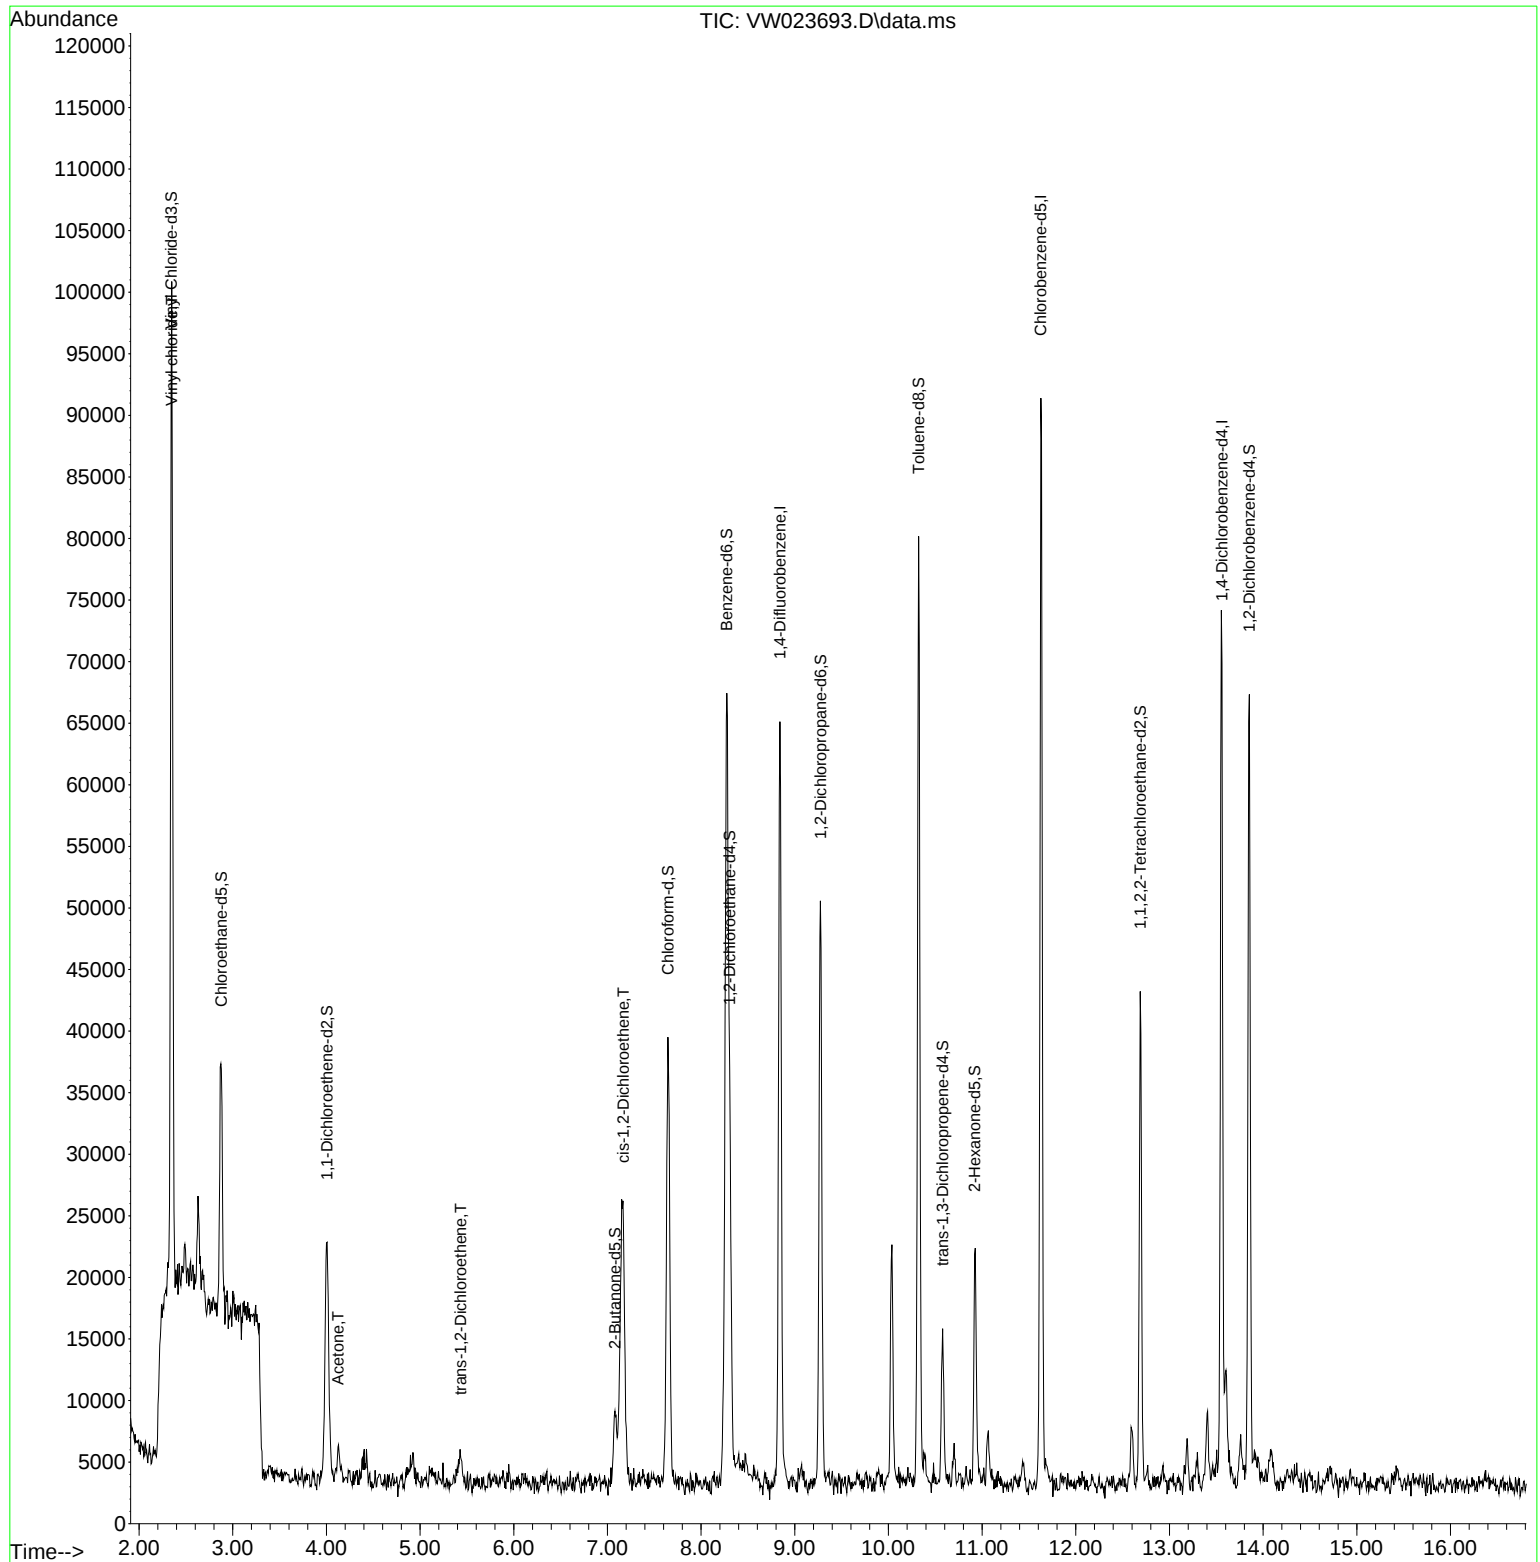

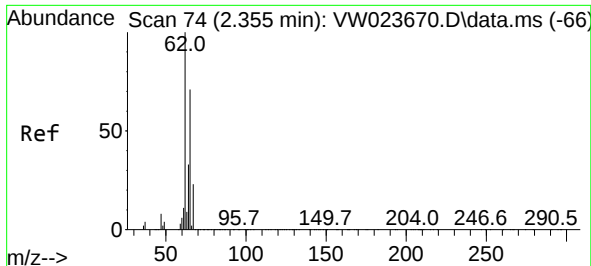

#5
 Vinyl chloride
 Concen: 37.816 ug/L
 RT: 2.349 min Scan# 71
 Delta R.T. -0.006 min
 Lab File: VW023693.D
 Acq: 14 Jul 2022 11:14




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B40RE

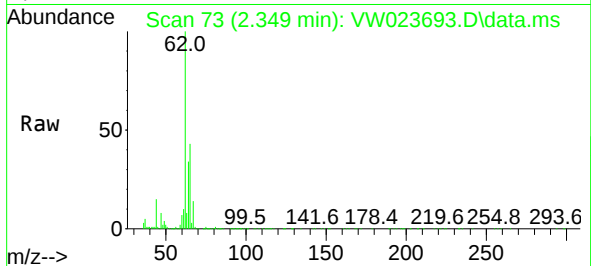

Tgt Ion: 62 Resp: 51284
 Ion Ratio Lower Upper
 62 100
 64 33.6 24.0 44.6




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

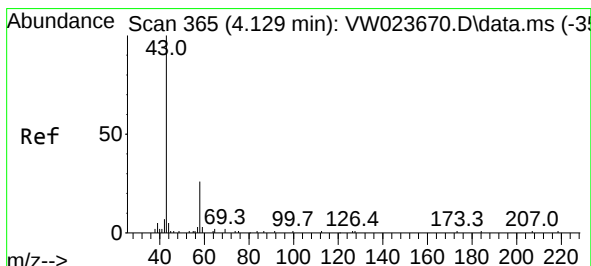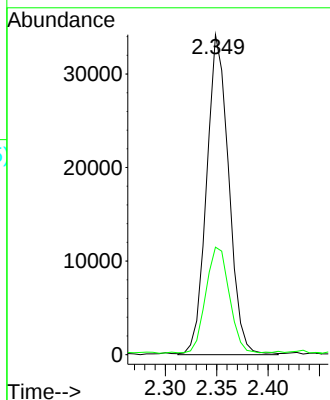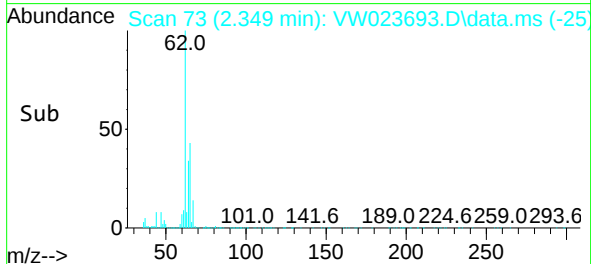

#13
 Acetone
 Concen: 34.103 ug/L m
 RT: 4.123 min Scan# 364
 Delta R.T. -0.006 min
 Lab File: VW023693.D
 Acq: 14 Jul 2022 11:14


Tgt Ion: 43 Resp: 4533
 Ion Ratio Lower Upper
 43 100
 58 14.6 0.0 64.2

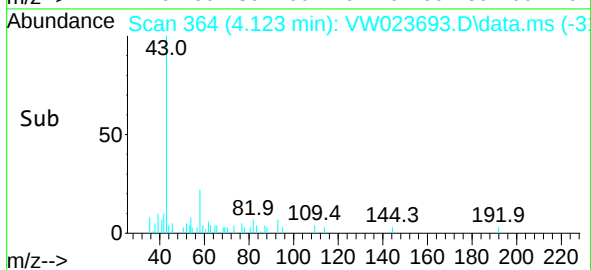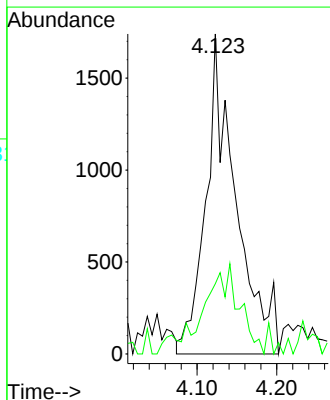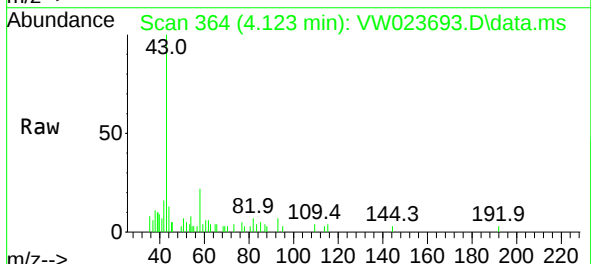

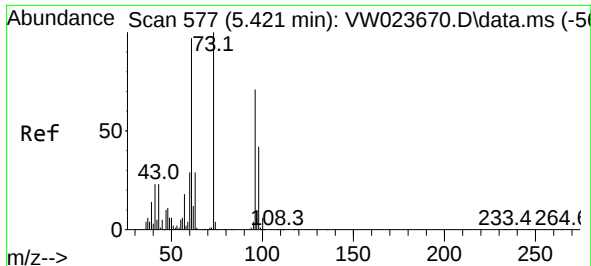

#17
trans-1,2-Dichloroethene
Concen: 2.292 ug/L m
RT: 5.434 min Scan# 577
Delta R.T. 0.012 min
Lab File: VW023693.D
Acq: 14 Jul 2022 11:14




Instrument :
MSVOA_W
ClientSampleId :
F5B40RE

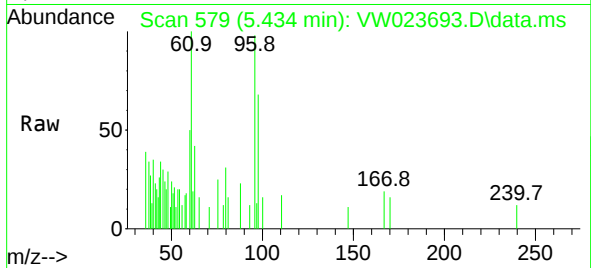

Tgt Ion: 96 Resp: 1399
Ion Ratio Lower Upper
96 100
61 101.8 90.8 168.6
98 69.2 42.8 79.6

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022

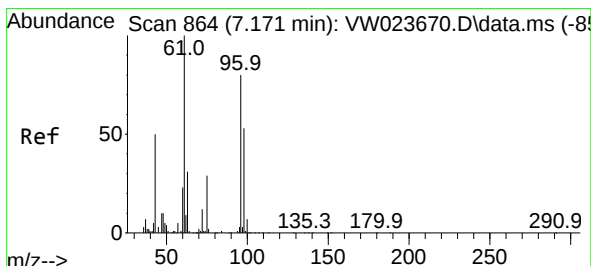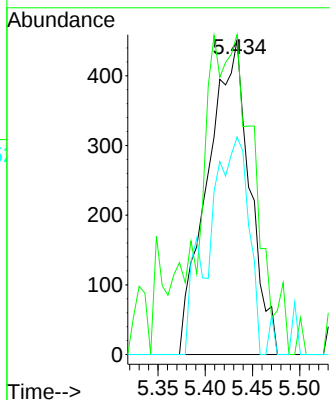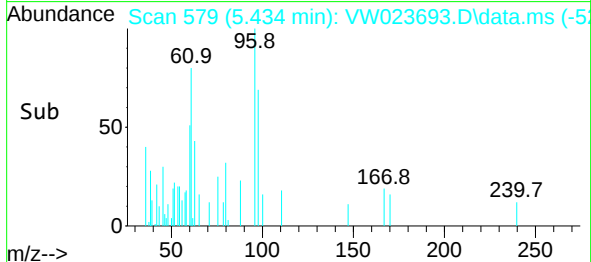

#20
cis-1,2-Dichloroethene
Concen: 13.069 ug/L m
RT: 7.171 min Scan# 864
Delta R.T. -0.000 min
Lab File: VW023693.D
Acq: 14 Jul 2022 11:14

Tgt Ion: 96 Resp: 8837
Ion Ratio Lower Upper
96 100
61 112.0 90.6 168.2
68 2.3 0.2 0.4#

