




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023702.D
 Acq On : 14 Jul 2022 15:59
 Operator : SY/VA
 Sample : N3679-11RE
 Misc : 6.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B51RE

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:43:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

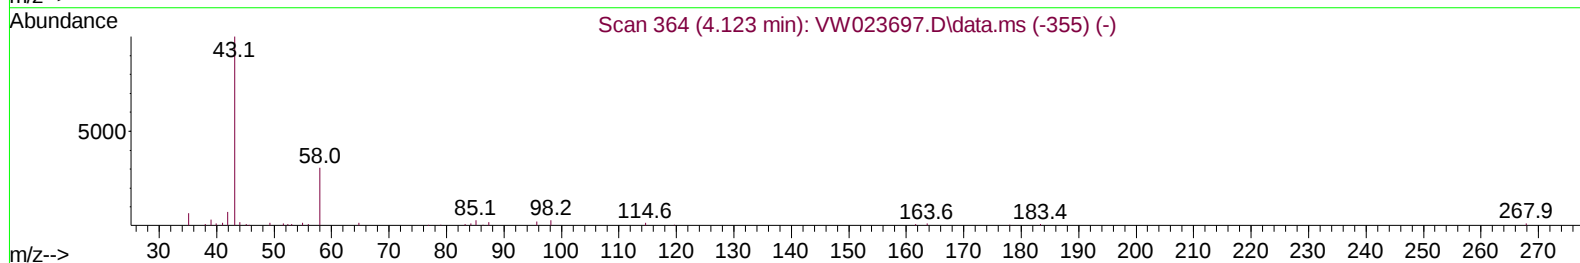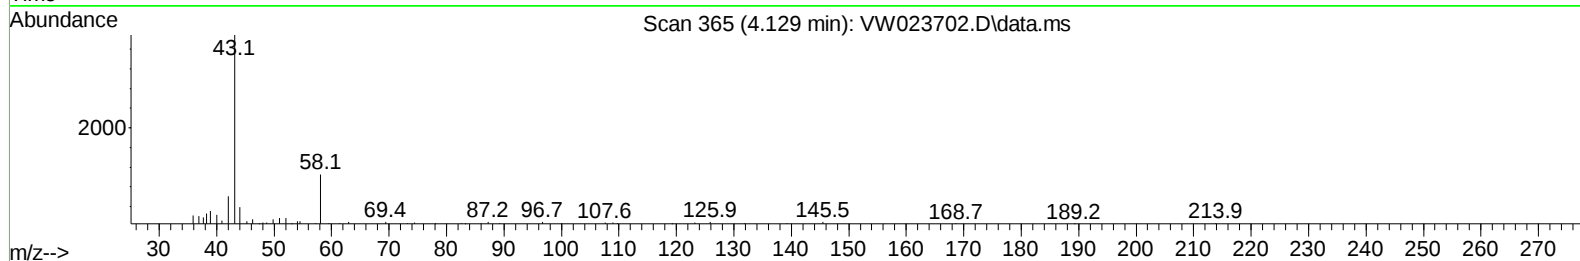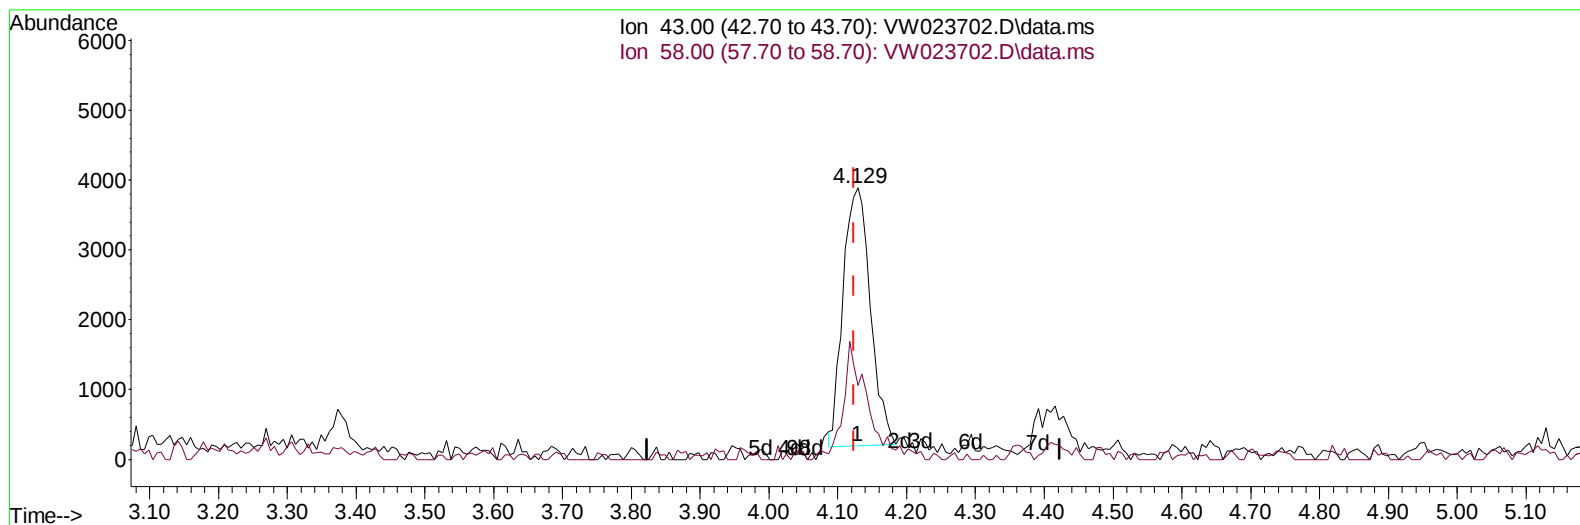

TIC: VW023702.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 28.34 ug/L

response 10127

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	38.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023702.D
 Acq On : 14 Jul 2022 15:59
 Operator : SY/VA
 Sample : N3679-11RE
 Misc : 6.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B51RE

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:43:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

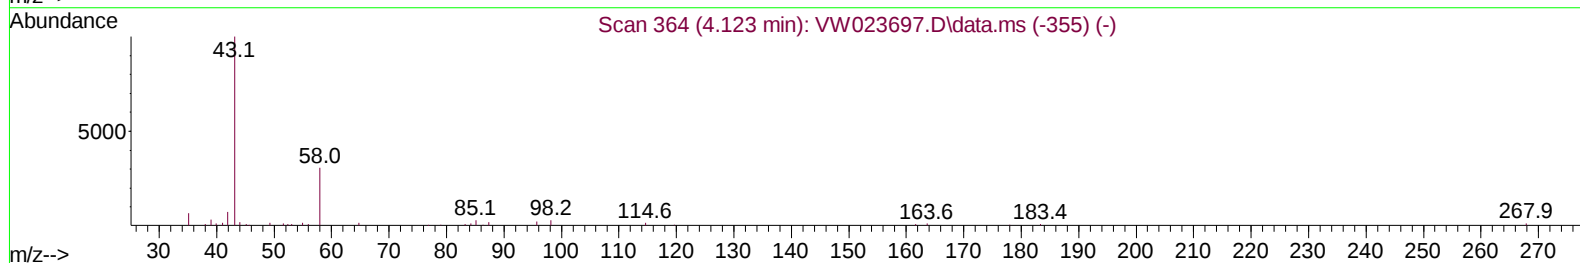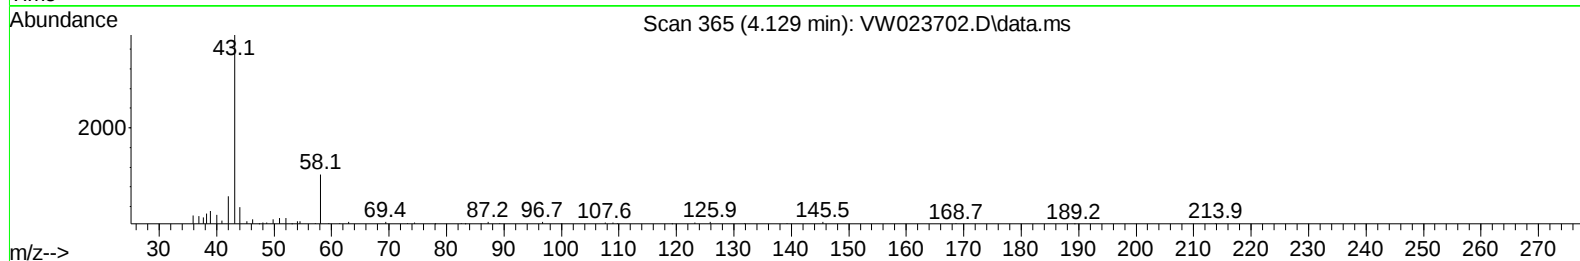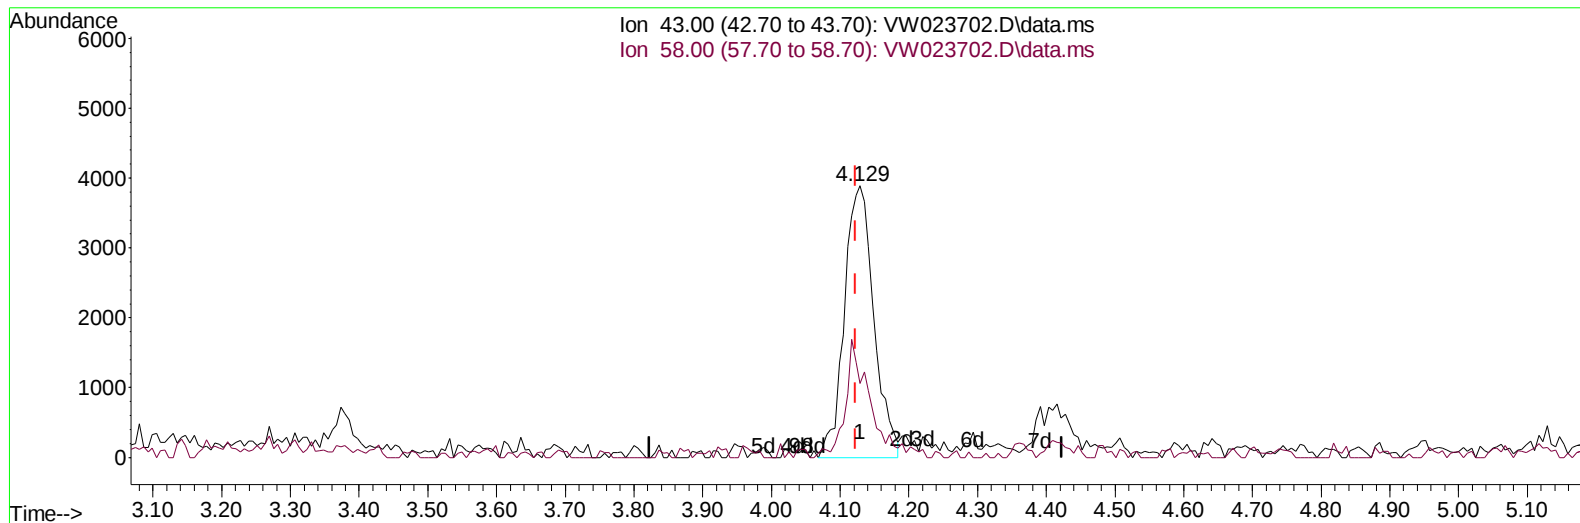

TIC: VW023702.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 32.50 ug/L m

response 11611

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	33.26
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023702.D
 Acq On : 14 Jul 2022 15:59
 Operator : SY/VA
 Sample : N3679-11RE
 Misc : 6.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B51RE

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:43:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		127560	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		124044	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		49814	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		72017	22.105	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	88.400%	
7) Chloroethane-d5	2.873	69		45468	20.920	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.680%	
11) 1,1-Dichloroethene-d2	4.007	63		38458	14.496	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	58.000%	
21) 2-Butanone-d5	7.080	46		30208	59.777	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	119.560%	
24) Chloroform-d	7.647	84		86051	23.170	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	92.680%	
26) 1,2-Dichloroethane-d4	8.305	65		54077	23.807	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	95.240%	
32) Benzene-d6	8.275	84		156944	24.339	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	97.360%	
36) 1,2-Dichloropropane-d6	9.274	67		48838	25.144	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	100.560%	
41) Toluene-d8	10.323	98		138575	21.187	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	84.760%	
43) trans-1,3-Dichloroprop...	10.579	79		18791	20.639	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	82.560%	
47) 2-Hexanone-d5	10.927	63		21579	52.834	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	105.660%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		52336	24.382	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.520%	
66) 1,2-Dichlorobenzene-d4	13.853	152		47926	26.951	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	107.800%	
Target Compounds							
13) Acetone	4.129	43		11611m	32.498	ug/L	
14) Carbon disulfide	4.367	76		3957	0.995	ug/L #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023702.D
Acq On : 14 Jul 2022 15:59
Operator : SY/VA
Sample : N3679-11RE
Misc : 6.56g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B51RE

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:43:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 03:40:01 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

