




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023712.D
 Acq On : 14 Jul 2022 20:06
 Operator : SY/VA
 Sample : N3700-01
 Misc : 5.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C08

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:45:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

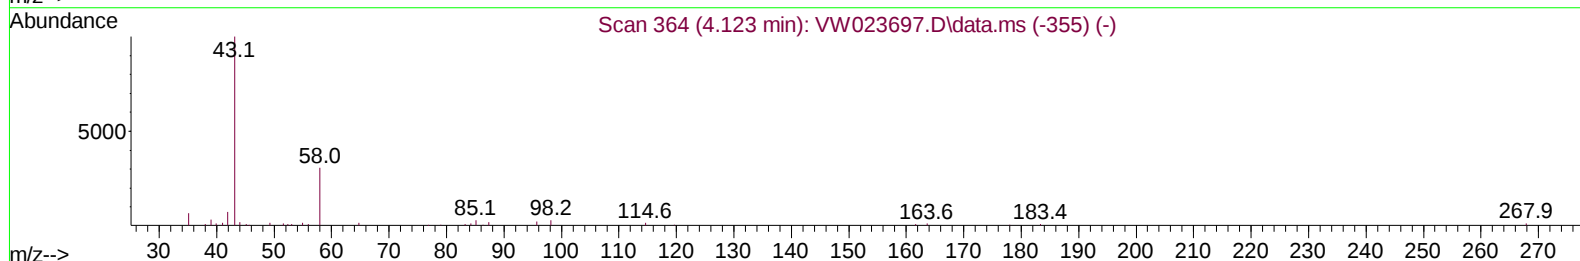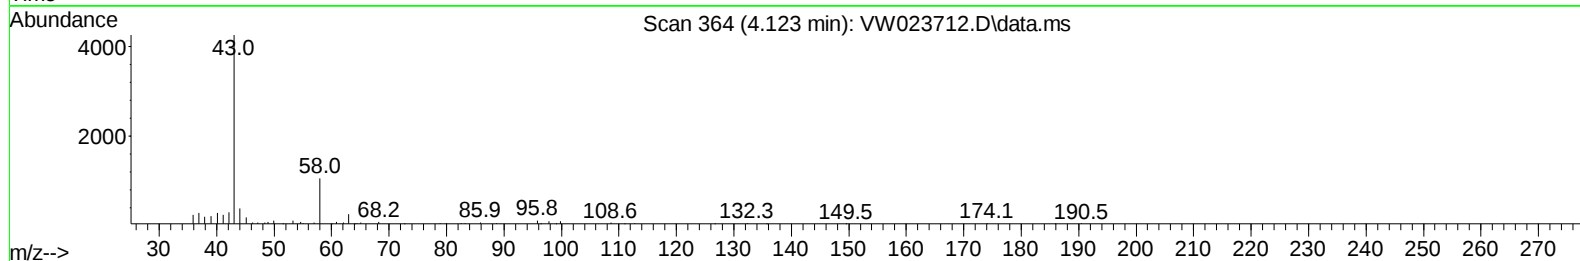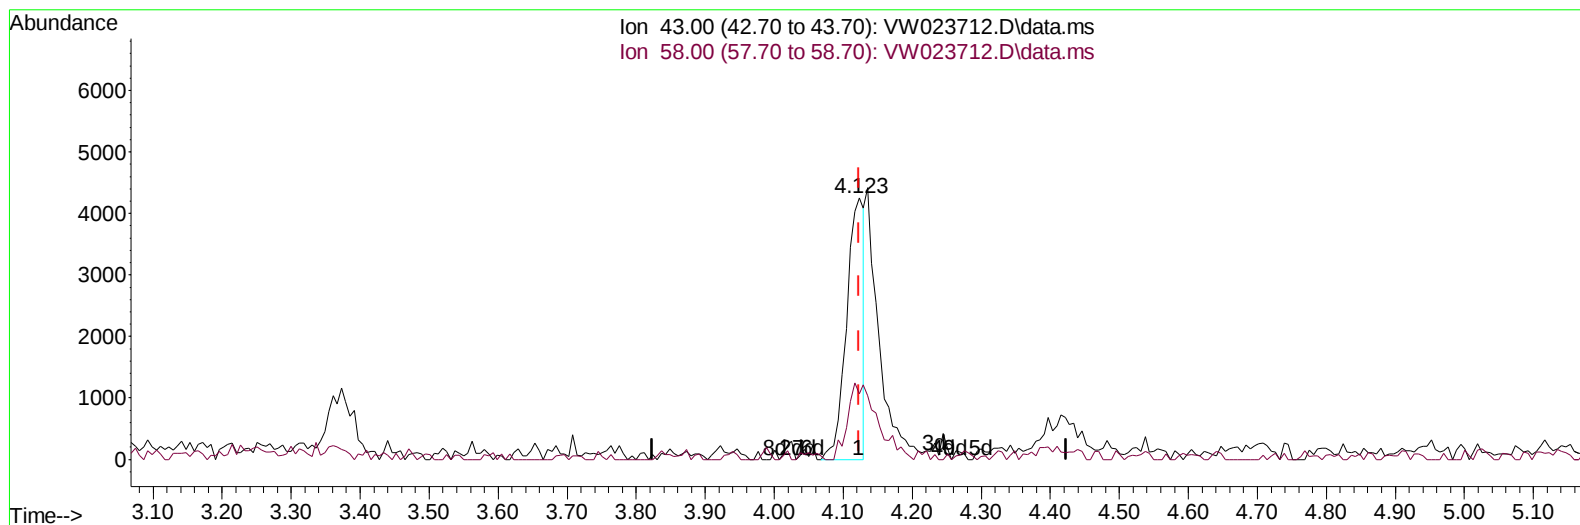

TIC: VW023712.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 12.71 ug/L

response 7488

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	21.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023712.D
 Acq On : 14 Jul 2022 20:06
 Operator : SY/VA
 Sample : N3700-01
 Misc : 5.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C08

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:45:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

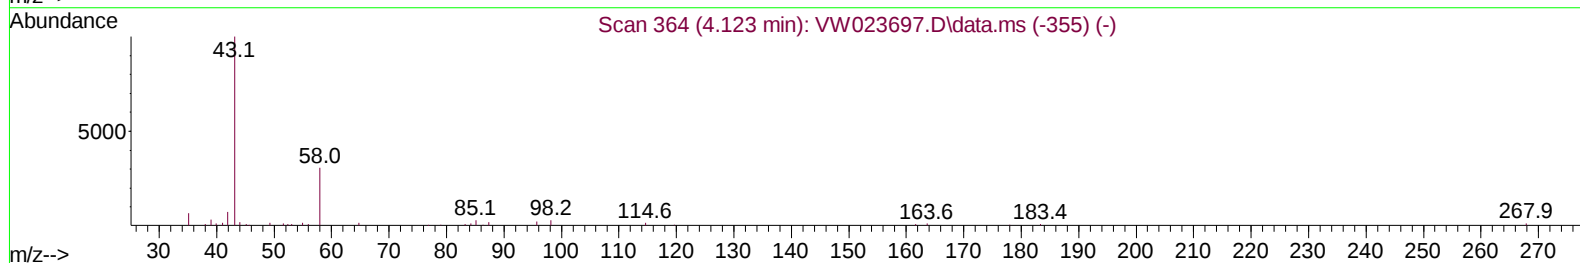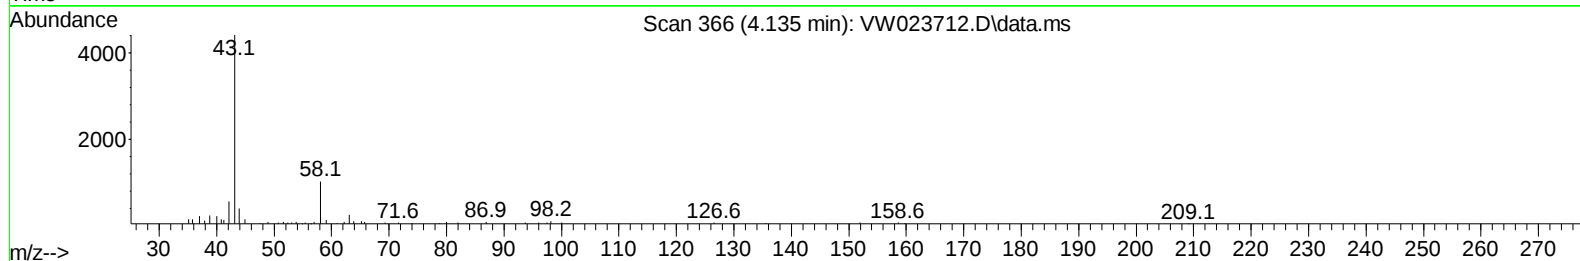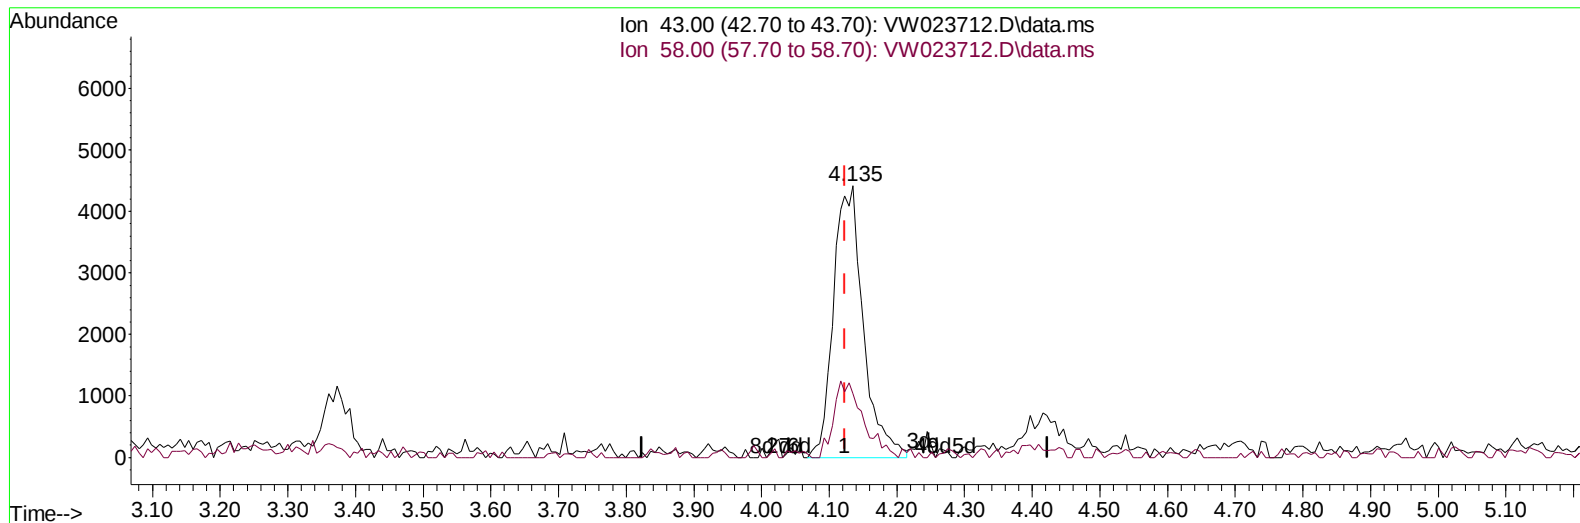

TIC: VW023712.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 22.78 ug/L m

response 13426

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	11.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023712.D
 Acq On : 14 Jul 2022 20:06
 Operator : SY/VA
 Sample : N3700-01
 Misc : 5.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C08

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 03:45:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

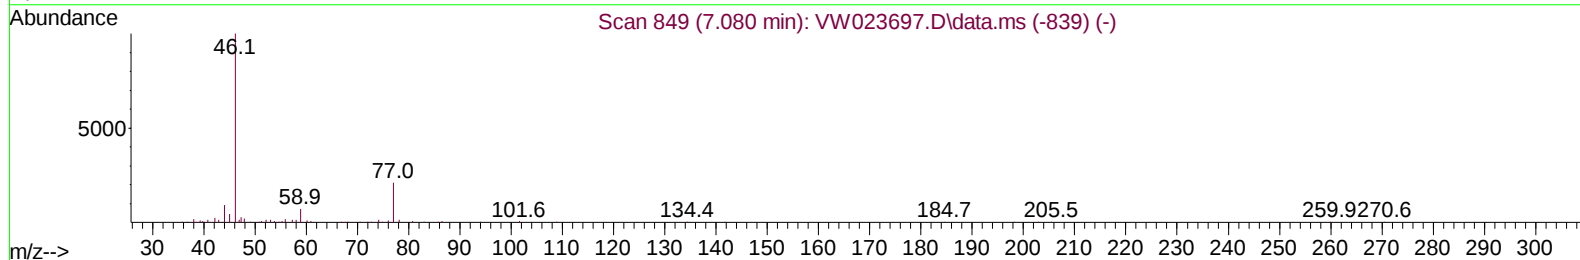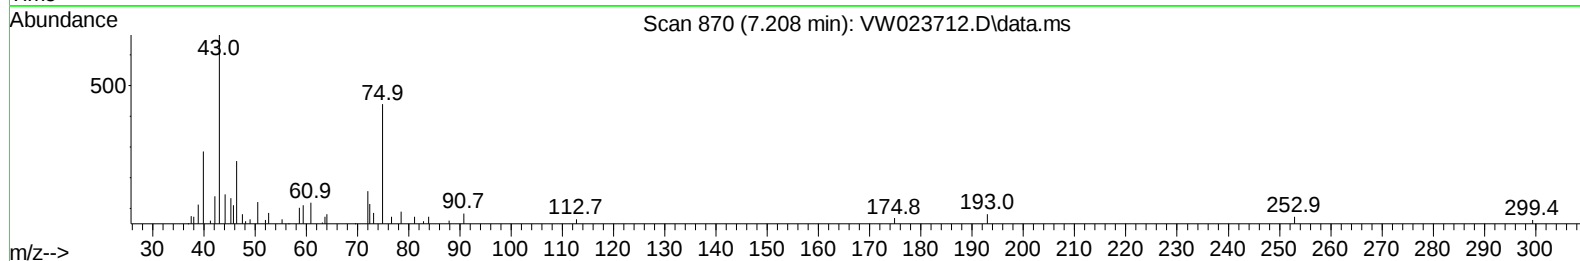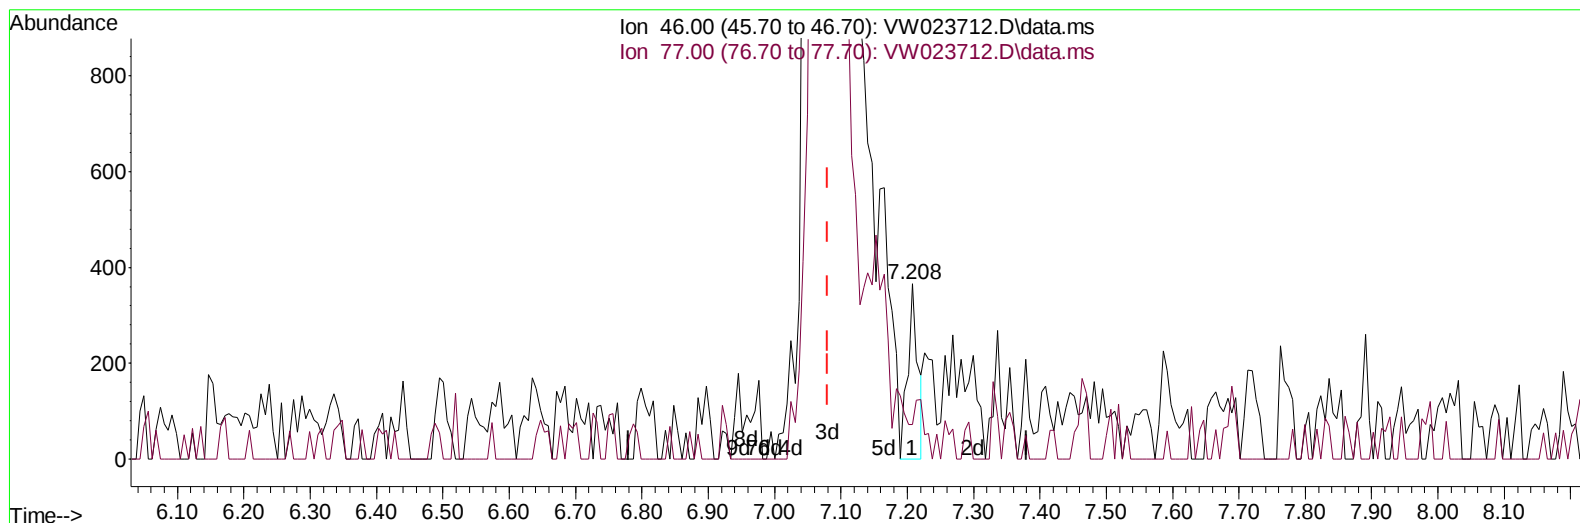

TIC: VW023712.D\data.ms

(21) 2-Butanone-d5 (S)

7.208min (+ 0.128) 0.47 ug/L

response 388

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	18.81
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023712.D
 Acq On : 14 Jul 2022 20:06
 Operator : SY/VA
 Sample : N3700-01
 Misc : 5.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C08

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:45:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

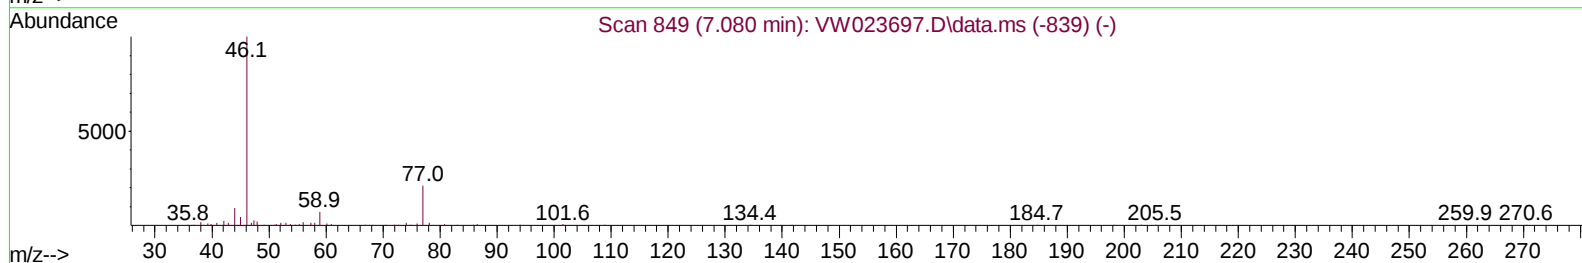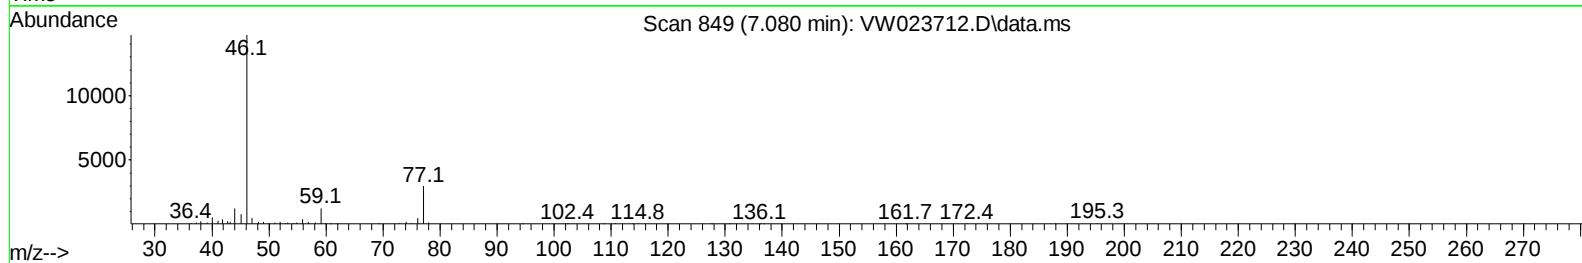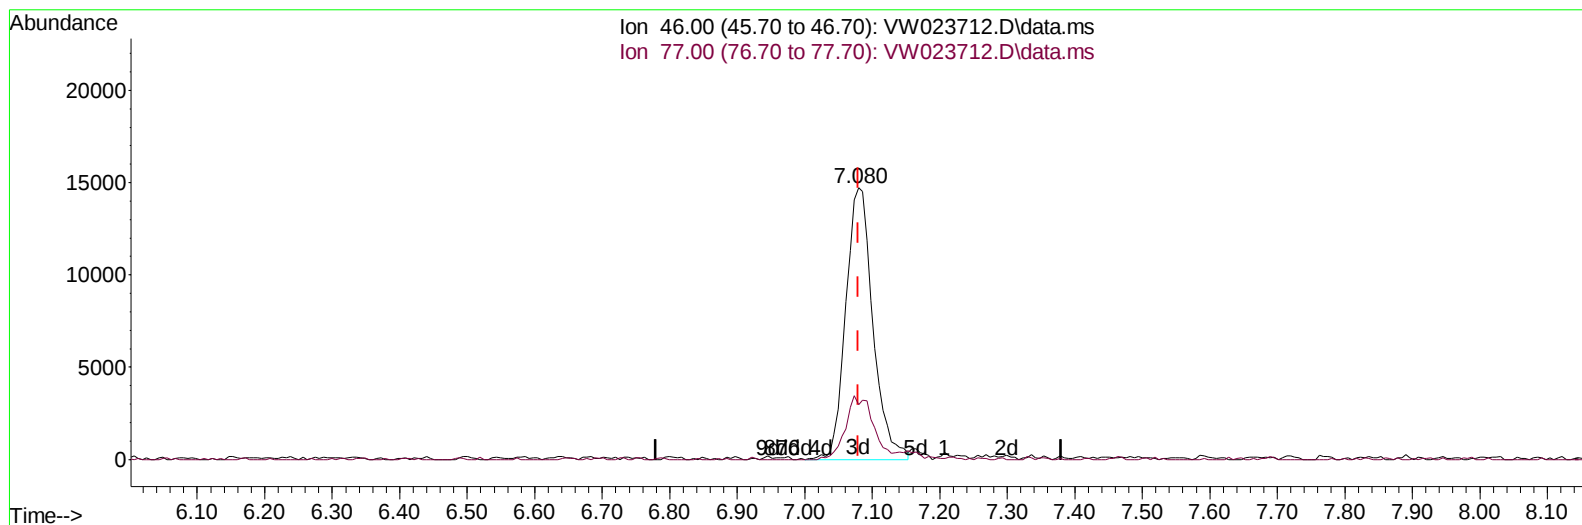

TIC: VW023712.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (-0.000) 49.22 ug/L m

response 41021

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	0.18#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023712.D
 Acq On : 14 Jul 2022 20:06
 Operator : SY/VA
 Sample : N3700-01
 Misc : 5.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C08

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:45:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		210379	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		195714	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		76663	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		91871	17.098	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	68.400%		
7) Chloroethane-d5	2.873	69		72794	20.307	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.240%		
11) 1,1-Dichloroethene-d2	4.007	63		47199	10.787	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	43.160%#		
21) 2-Butanone-d5	7.080	46		41021m	49.218	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	98.440%		
24) Chloroform-d	7.647	84		114512	18.695	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	74.800%		
26) 1,2-Dichloroethane-d4	8.305	65		72965	19.477	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	77.920%		
32) Benzene-d6	8.275	84		203646	20.017	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	80.080%		
36) 1,2-Dichloropropane-d6	9.274	67		67182	21.922	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	87.680%		
41) Toluene-d8	10.323	98		184601	17.888	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	71.560%		
43) trans-1,3-Dichloroprop...	10.573	79		22356	15.563	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	62.240%		
47) 2-Hexanone-d5	10.926	63		30829	47.841	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	95.680%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		68804	20.316	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	81.280%		
66) 1,2-Dichlorobenzene-d4	13.853	152		56783	20.749	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	83.000%		
Target Compounds							
13) Acetone	4.135	43		13426m	22.785	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023712.D
Acq On : 14 Jul 2022 20:06
Operator : SY/VA
Sample : N3700-01
Misc : 5.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C08

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 03:45:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 03:40:01 2022
Response via : Initial Calibration

